

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
 Data File : PL064657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2021 17:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:46:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.108	67719547	53855059	22.246	22.609
28)	SA Decachlor...	8.165	9.273	55510453	42659005	17.615	20.836
Target Compounds							
4)	MA Heptachlor	0.000	5.302	0	3115017	N.D.	0.894 #
6)	B beta-BHC	0.000	4.984	0	3408054	N.D.	2.014 #
7)	B delta-BHC	0.000	5.221f	0	2586376	N.D.	0.840 #
16)	A 4,4'-DDD	0.000	6.950f	0	1239283	N.D.	0.538 #
23)	Chlordane-1	4.320f	0.000	4721706	0	42.955	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
Data File : PL064657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2021 17:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:46:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

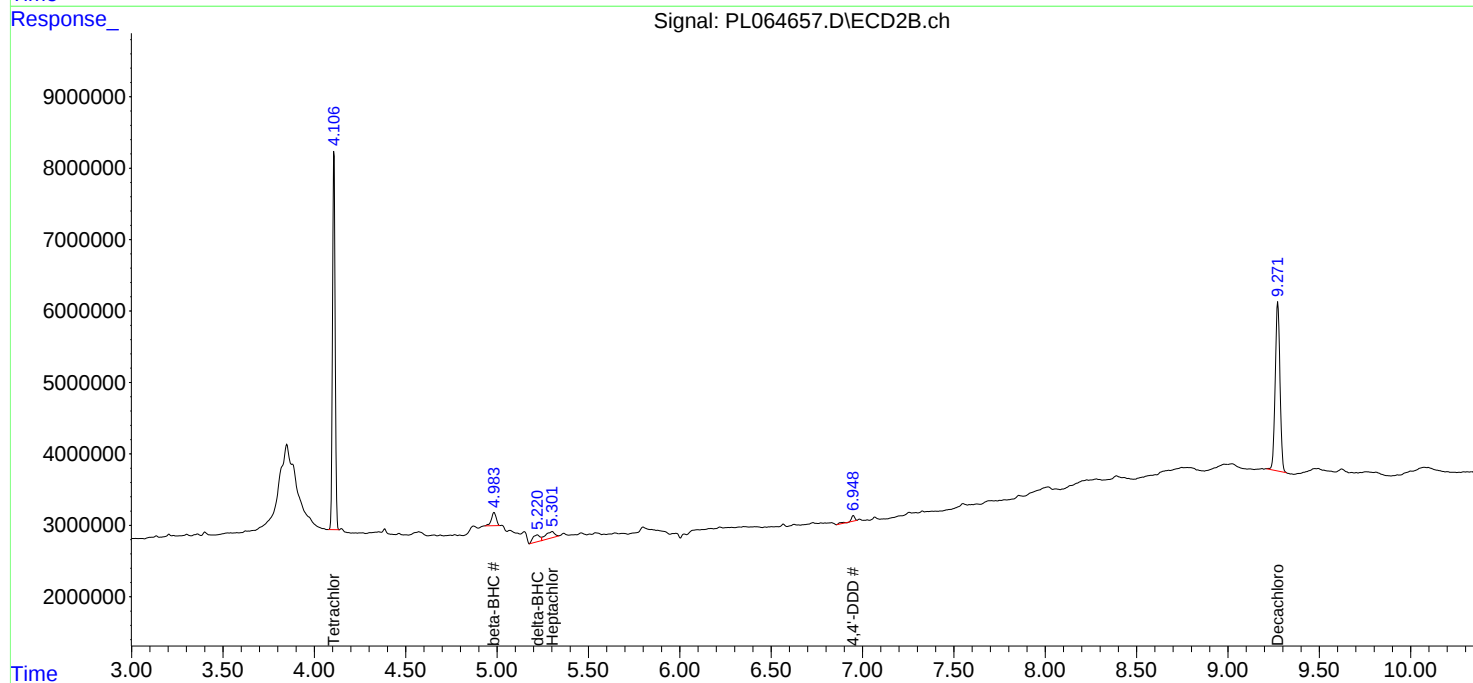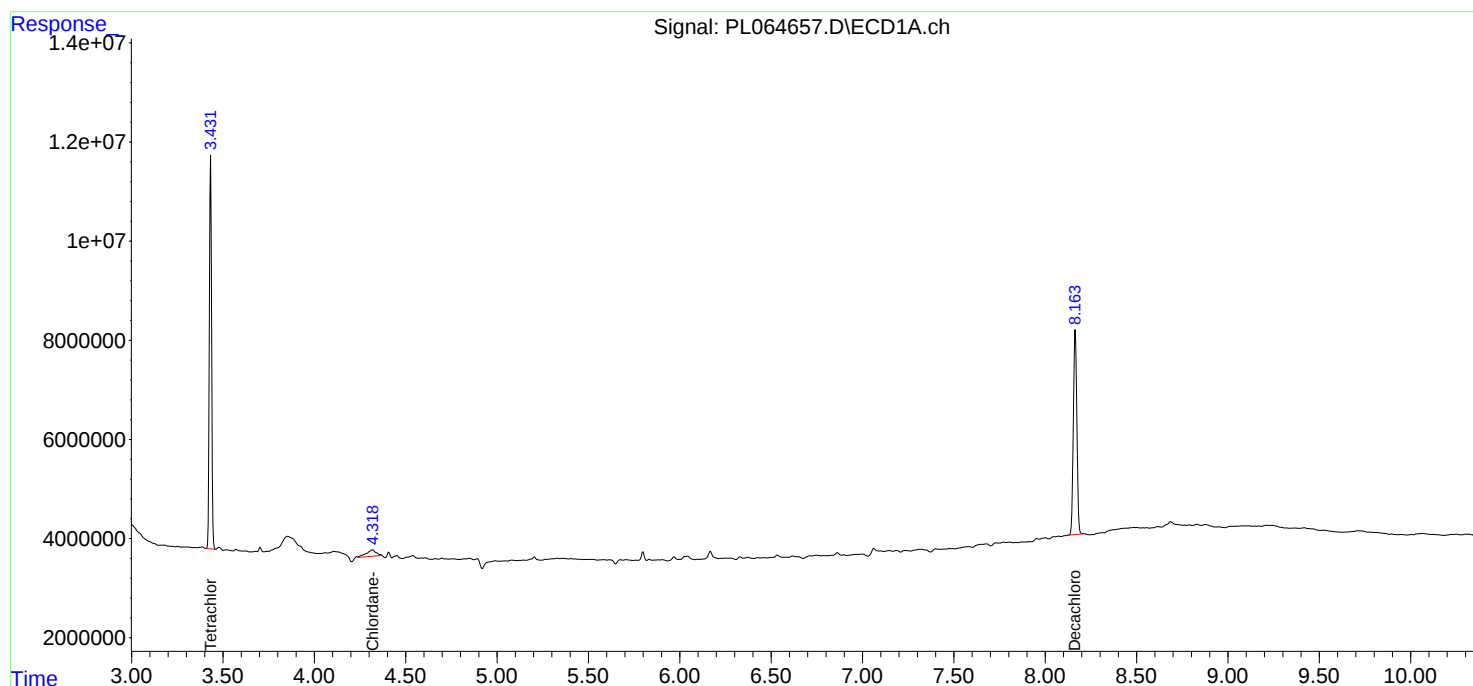


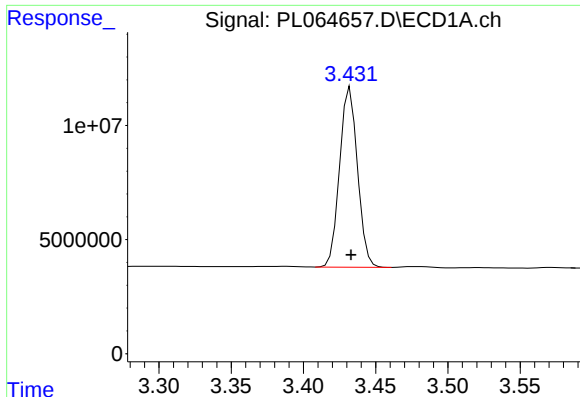

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 67719547
Conc: 22.25 ng/ml

Instrument :
ECD_O
ClientSampleId :

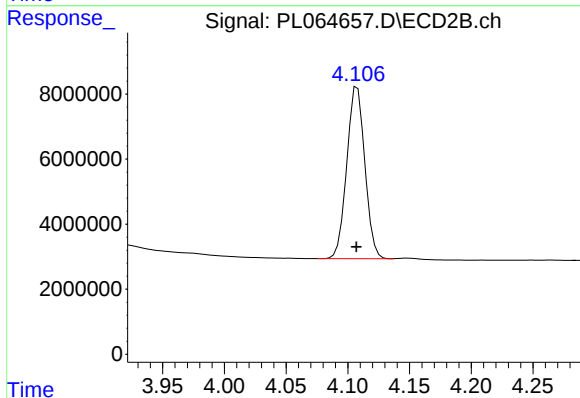


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 53855059
Conc: 22.61 ng/ml

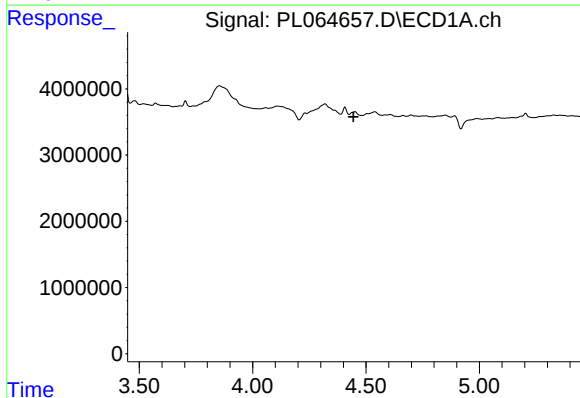


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

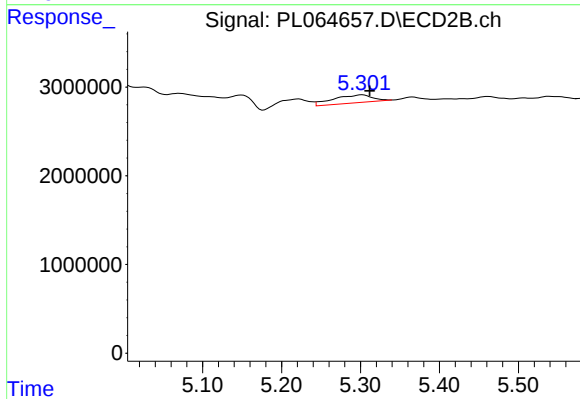

#4 Heptachlor


R.T.: 5.302 min
Delta R.T.: -0.009 min
Response: 3115017
Conc: 0.89 ng/ml

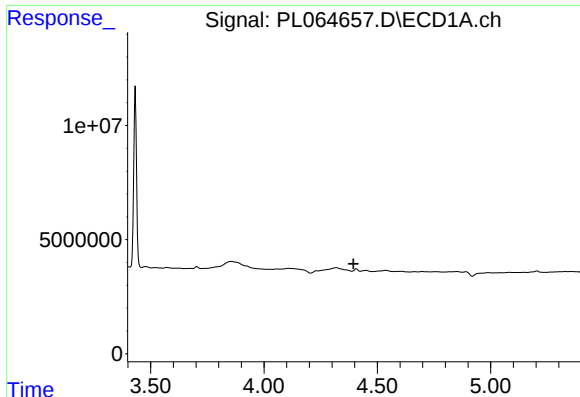

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

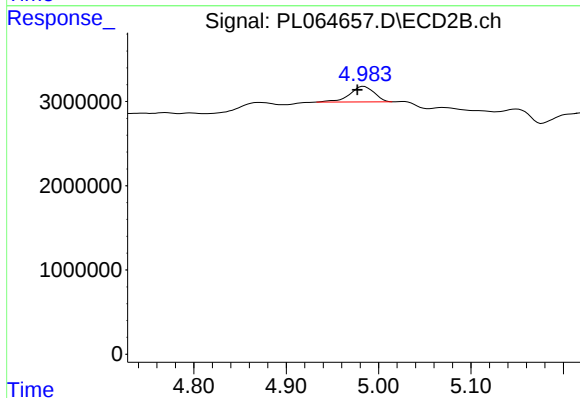


#6 beta-BHC

R.T.: 4.984 min
Delta R.T.: 0.007 min
Response: 3408054
Conc: 2.01 ng/ml

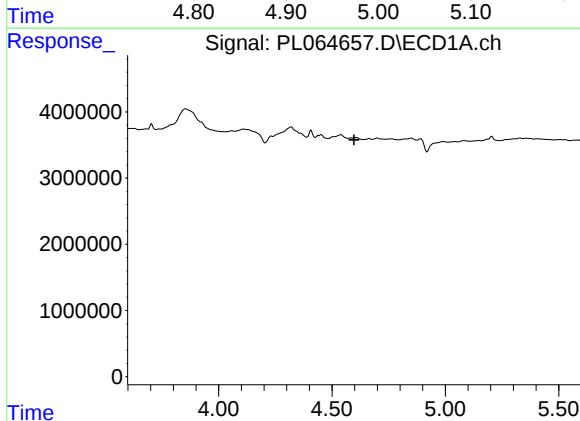


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

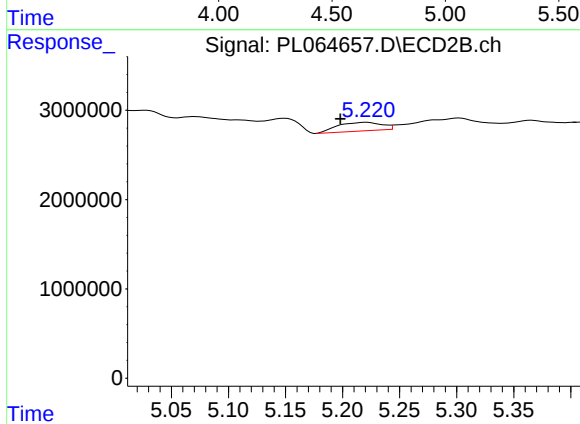

#7 delta-BHC


R.T.: 5.221 min
Delta R.T.: 0.023 min
Response: 2586376
Conc: 0.84 ng/ml

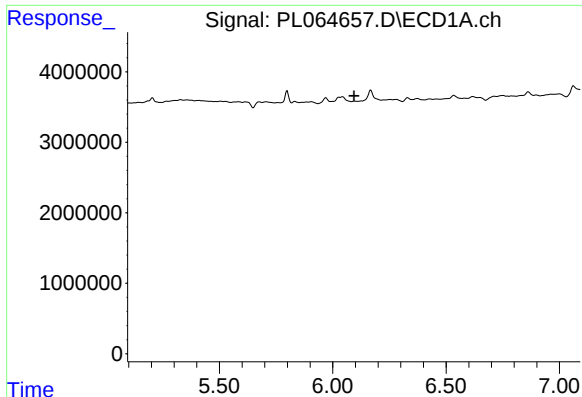

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

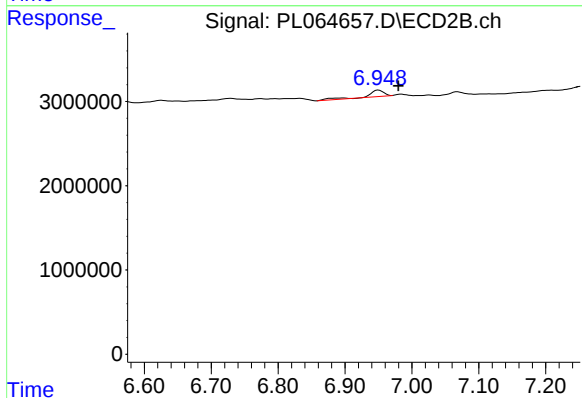


#16 4,4'-DDD

R.T.: 6.950 min
Delta R.T.: -0.030 min
Response: 1239283
Conc: 0.54 ng/ml

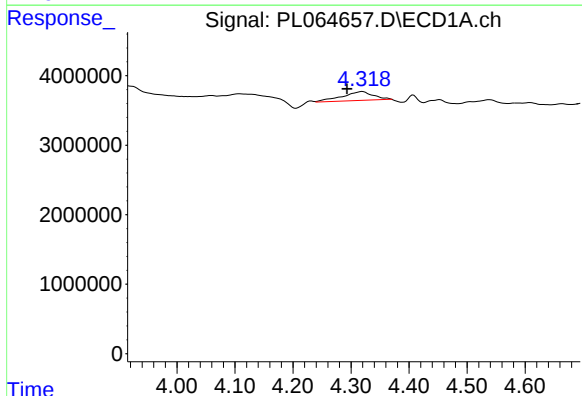


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.026 min
Response: 4721706
Conc: 42.95 ng/ml

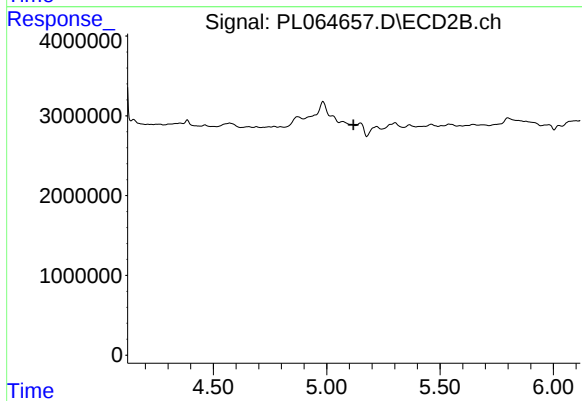

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

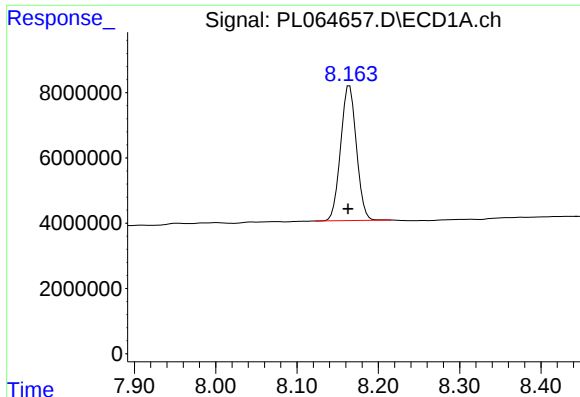

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.002 min
Response: 55510453
Conc: 17.61 ng/ml

Instrument :
ECD_O
ClientSampleId :

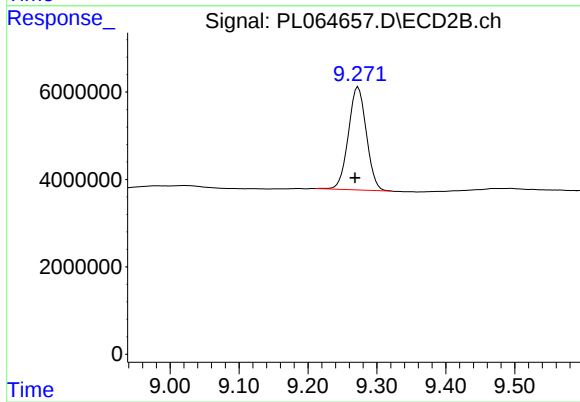

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.004 min
Response: 42659005
Conc: 20.84 ng/ml