

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0020521\
 Data File : P0075571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2021 13:38
 Operator : AJ/MA
 Sample : M1293-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TEST-PIT-4

Manual Integrations
 APPROVED

Ankita
 2/8/2021 4:50:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 14:56:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.995	1650261	766729	16.307m	15.950m
2) SA Decachlor...	10.943	9.243	1849699	845118	19.171	17.410m
Target Compounds						
31) L7 AR-1260-1	7.942	6.813	394274	250969	85.461	92.447
32) L7 AR-1260-2	8.209	7.010	949163	286747	147.054	86.438 #
33) L7 AR-1260-3	8.576	7.161	388484	251791	71.193	84.721
34) L7 AR-1260-4	8.804	7.641	692551	221972	134.724	85.327 #
35) L7 AR-1260-5	9.132	7.888	875447	450259	74.183	71.150

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020521\
Data File : PO075571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2021 13:38
Operator : AJ/MA
Sample : M1293-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 14:56:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

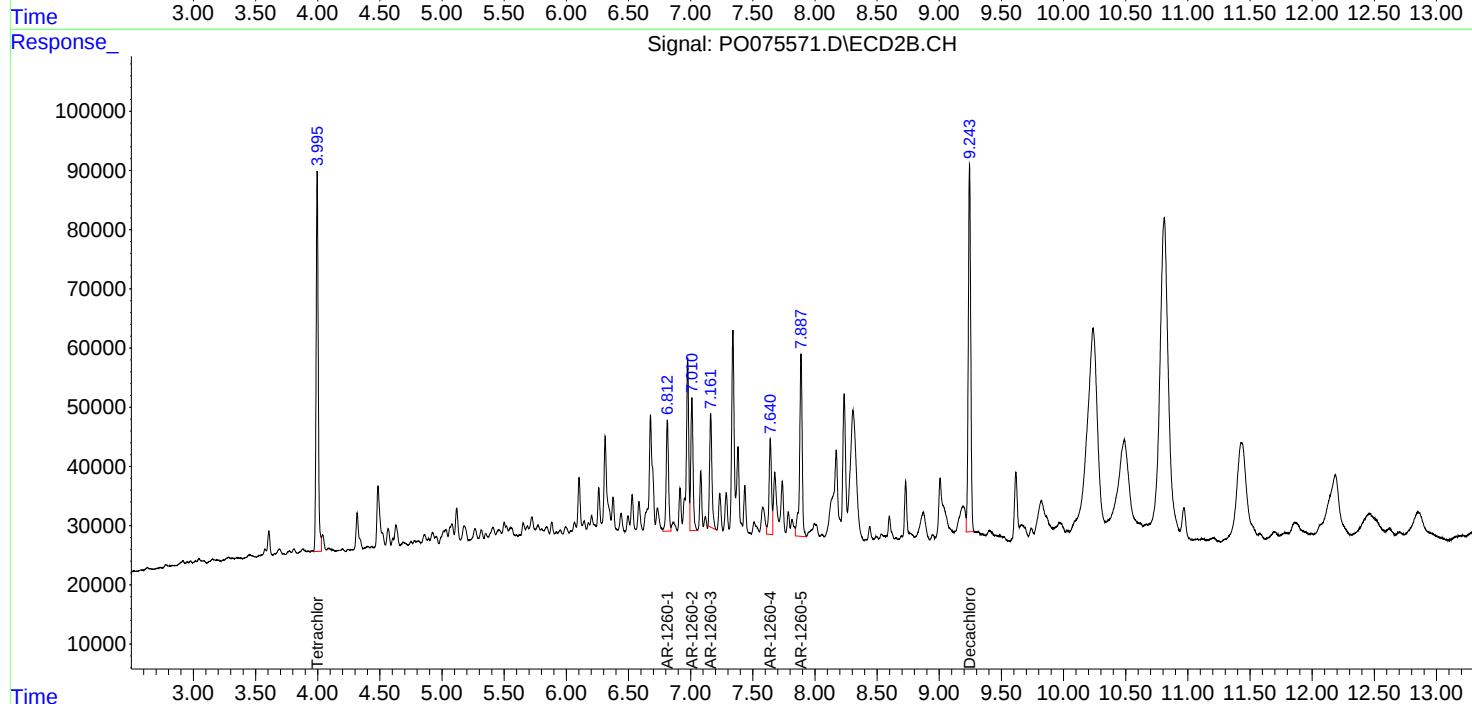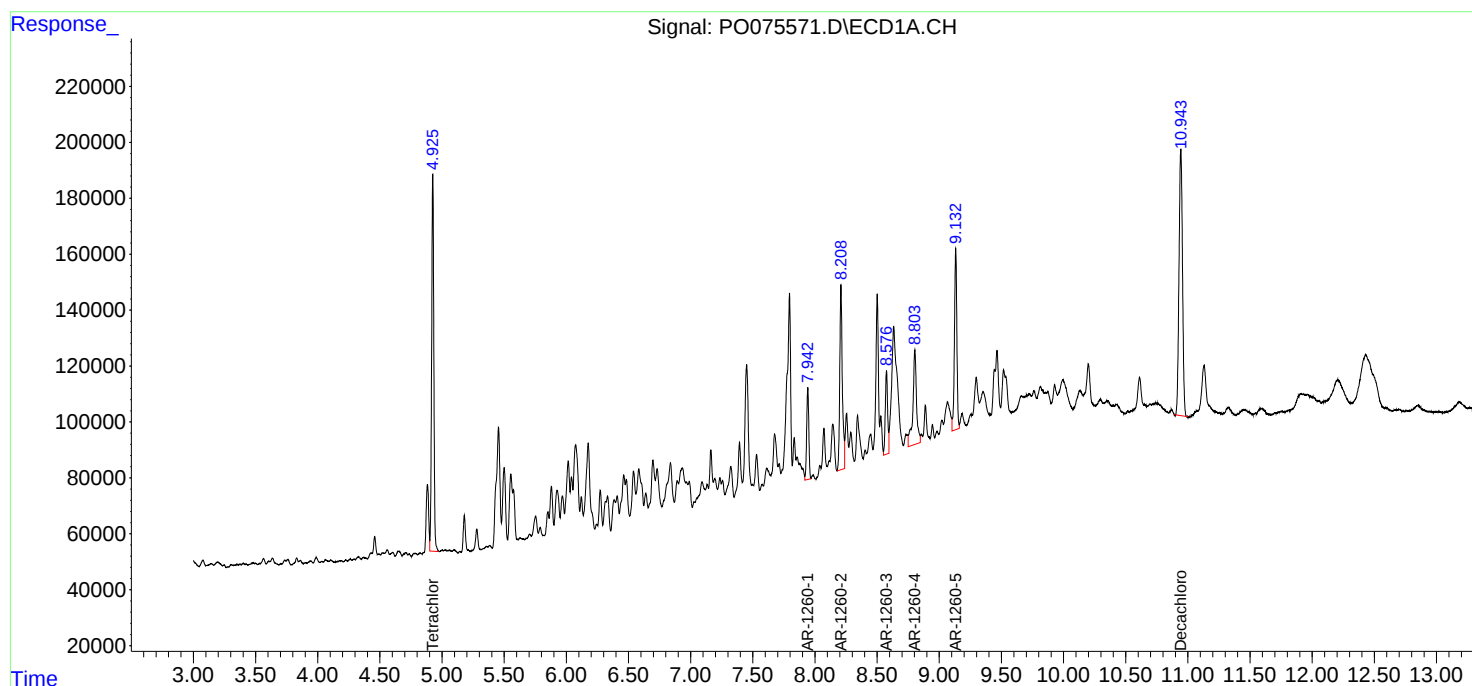

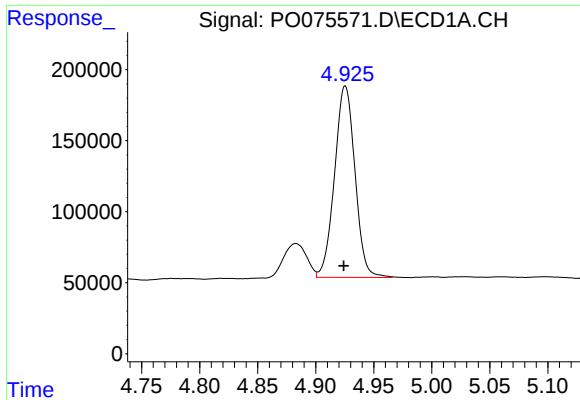


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: 0.000 min
Response: 1650261
Conc: 16.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:37 PM

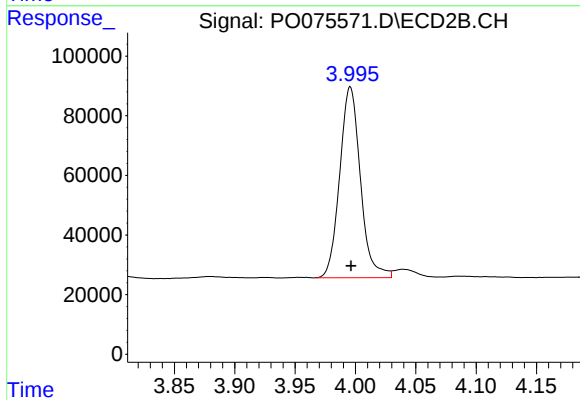


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 766729
Conc: 15.95 ng/ml m

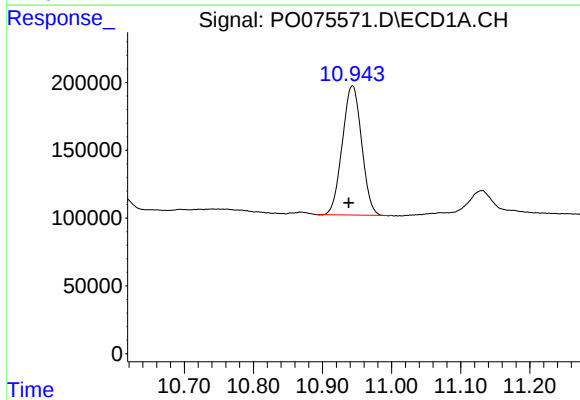


#2 Decachlorobiphenyl

R.T.: 10.943 min
Delta R.T.: 0.006 min
Response: 1849699
Conc: 19.17 ng/ml

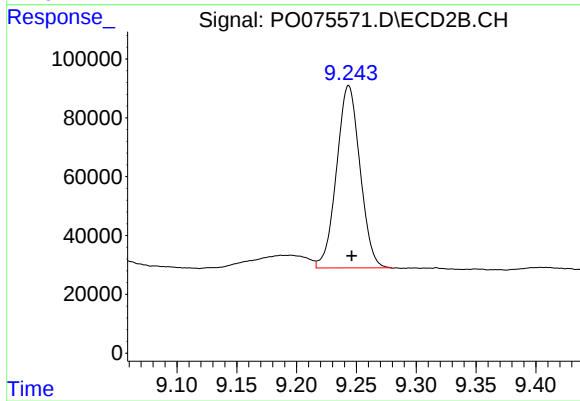

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 845118
Conc: 17.41 ng/ml m

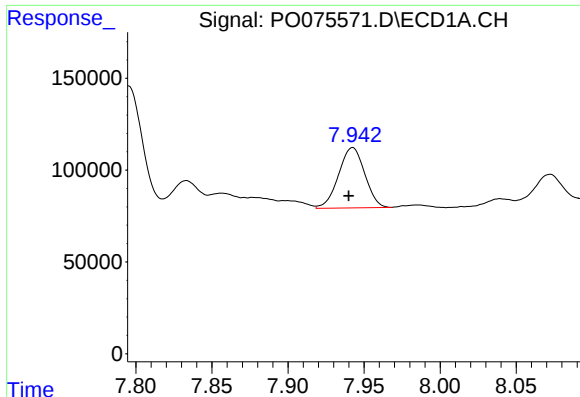


#31 AR-1260-1

R.T.: 7.942 min
Delta R.T.: 0.003 min
Response: 394274
Conc: 85.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:37 PM

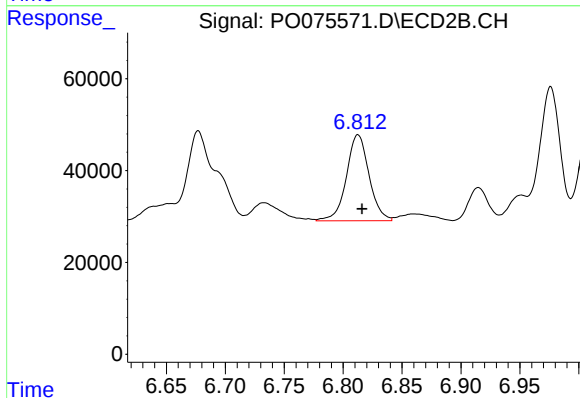


#31 AR-1260-1

R.T.: 6.813 min
Delta R.T.: -0.003 min
Response: 250969
Conc: 92.45 ng/ml

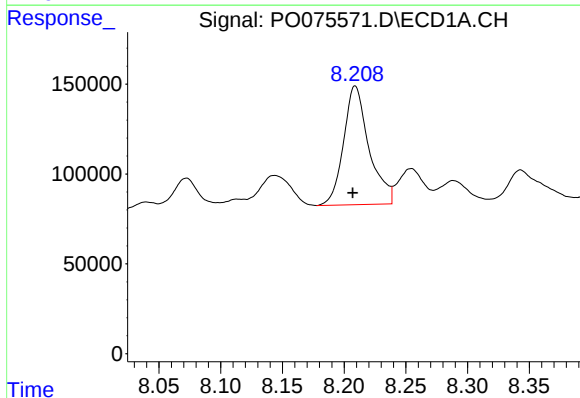


#32 AR-1260-2

R.T.: 8.209 min
Delta R.T.: 0.002 min
Response: 949163
Conc: 147.05 ng/ml

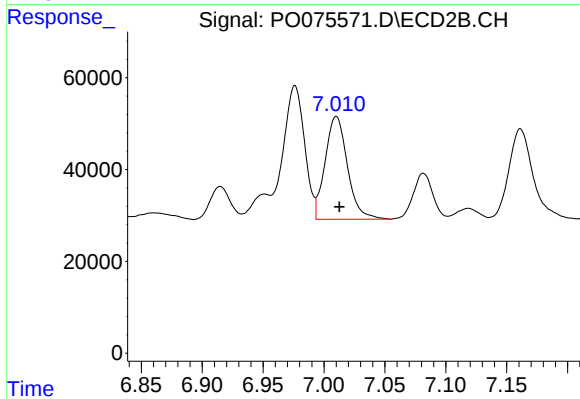

#32 AR-1260-2

R.T.: 7.010 min
Delta R.T.: -0.002 min
Response: 286747
Conc: 86.44 ng/ml

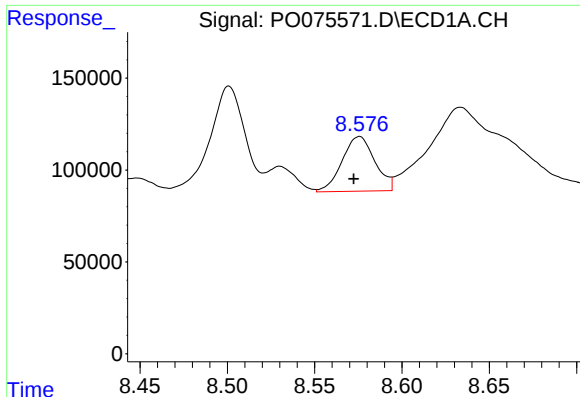


#33 AR-1260-3

R.T.: 8.576 min
Delta R.T.: 0.003 min
Response: 388484
Conc: 71.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:37 PM

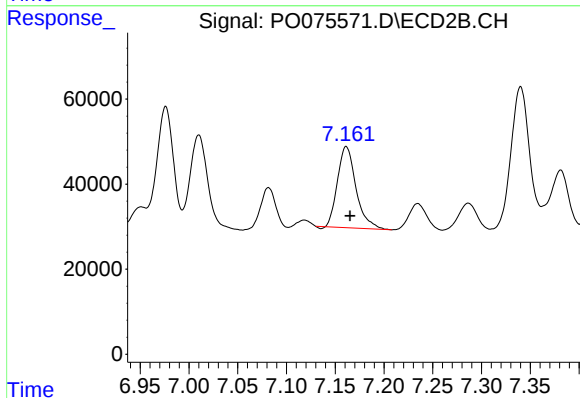


#33 AR-1260-3

R.T.: 7.161 min
Delta R.T.: -0.004 min
Response: 251791
Conc: 84.72 ng/ml

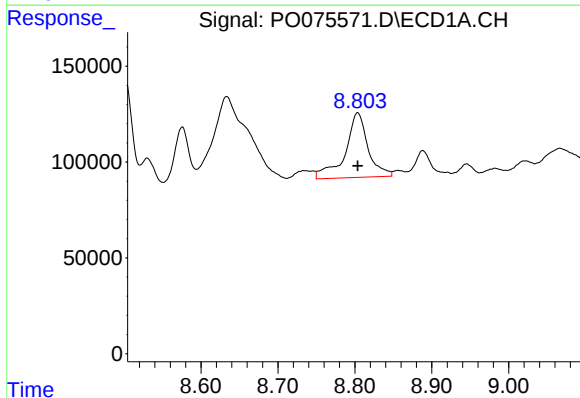


#34 AR-1260-4

R.T.: 8.804 min
Delta R.T.: 0.000 min
Response: 692551
Conc: 134.72 ng/ml

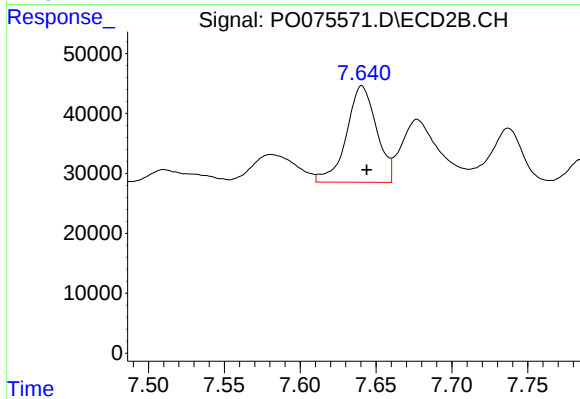

#34 AR-1260-4

R.T.: 7.641 min
Delta R.T.: -0.003 min
Response: 221972
Conc: 85.33 ng/ml

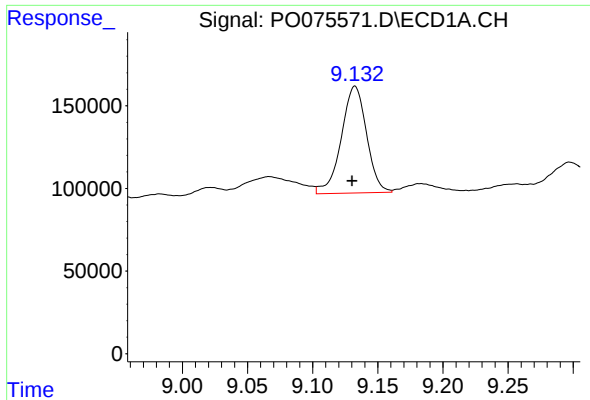


#35 AR-1260-5

R.T.: 9.132 min
Delta R.T.: 0.002 min
Response: 875447
Conc: 74.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:37 PM

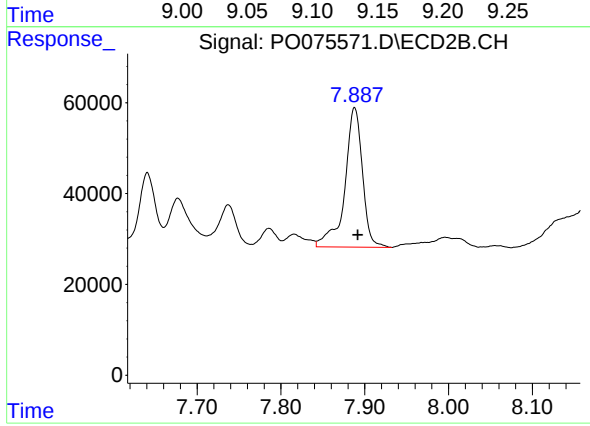

#35 AR-1260-5

R.T.: 7.888 min
Delta R.T.: -0.004 min
Response: 450259
Conc: 71.15 ng/ml