

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
 Data File : P0075572.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2021 14:10
 Operator : AJ/MA
 Sample : M1290-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WOOSPK-063-0002

Manual Integrations
 APPROVED

Ankita
 2/8/2021 4:50:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 14:56:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.939	3.995	1620737	960344	16.015m	19.977m
2) SA Decachlor...	10.963f	9.247	1892249	865125	19.612m	17.822

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
Data File : P0075572.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2021 14:10
Operator : AJ/MA
Sample : M1290-09
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WOOSPK-063-0002


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 14:56:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

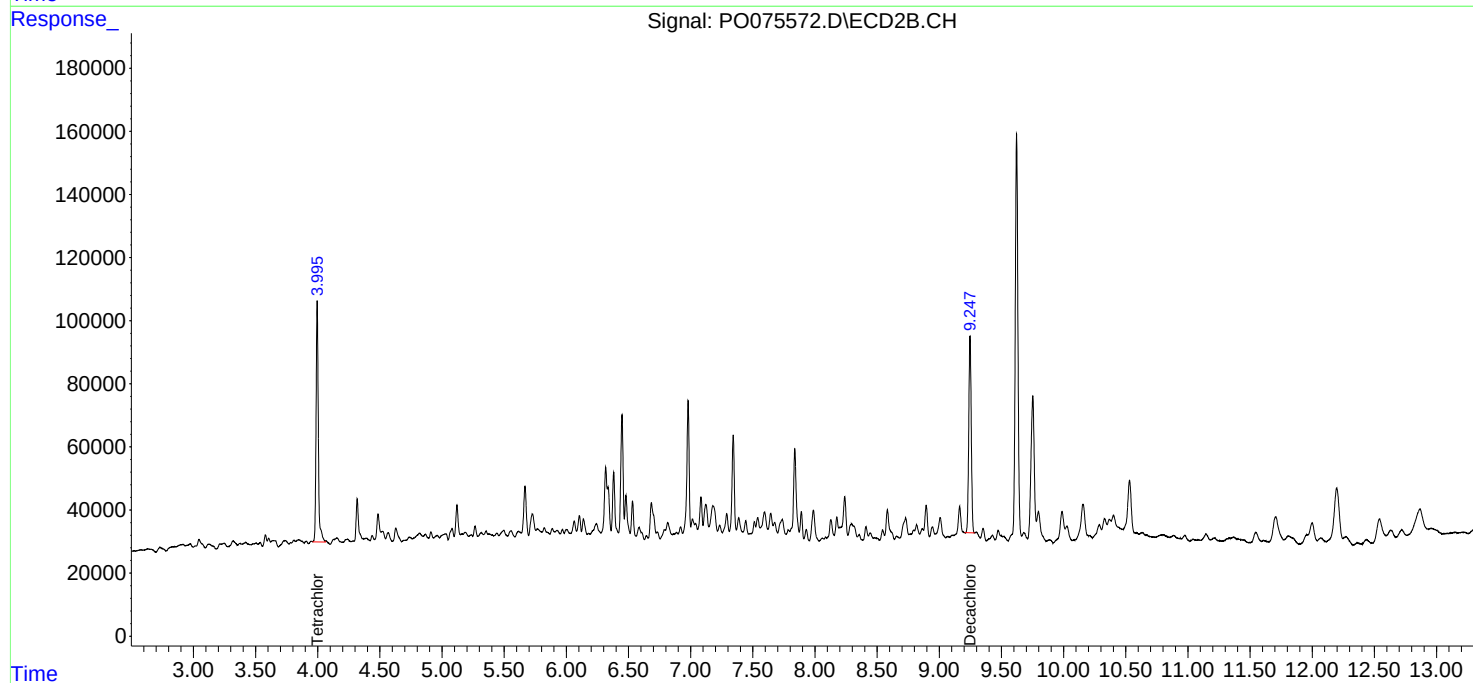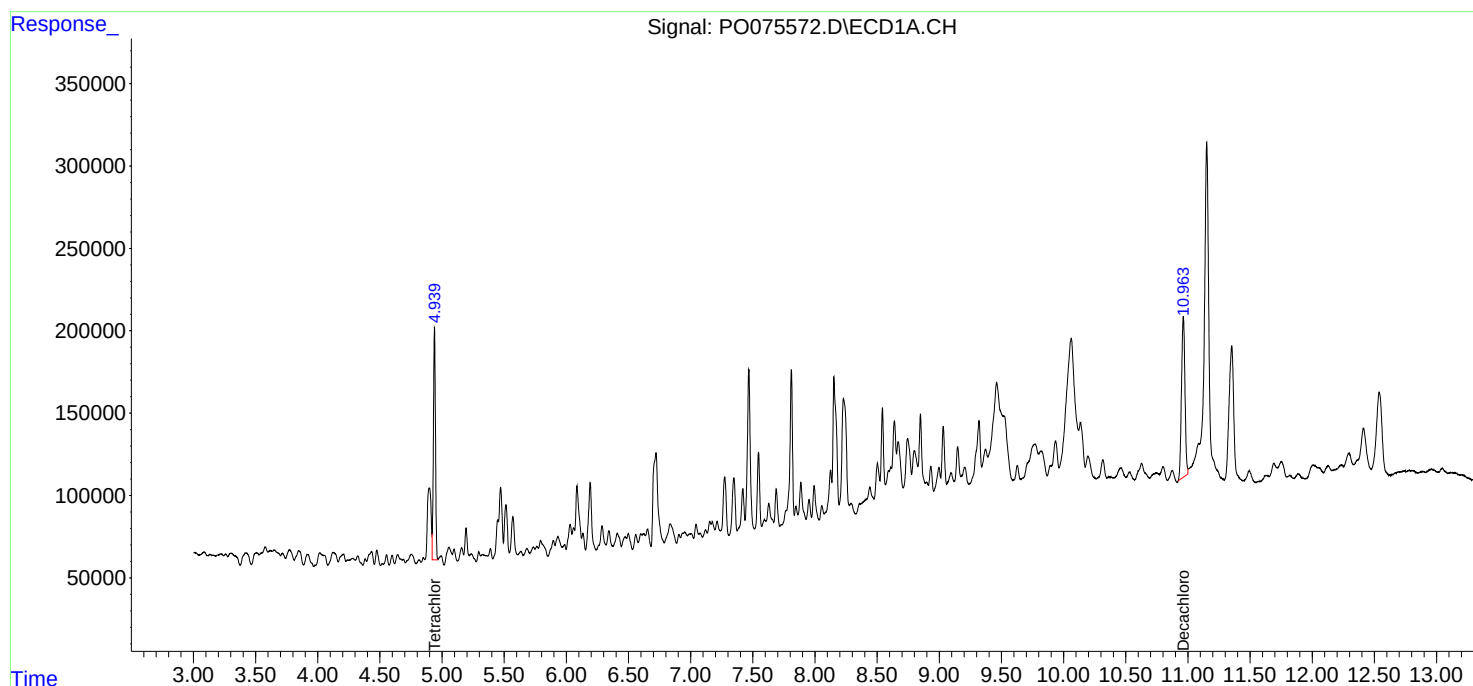

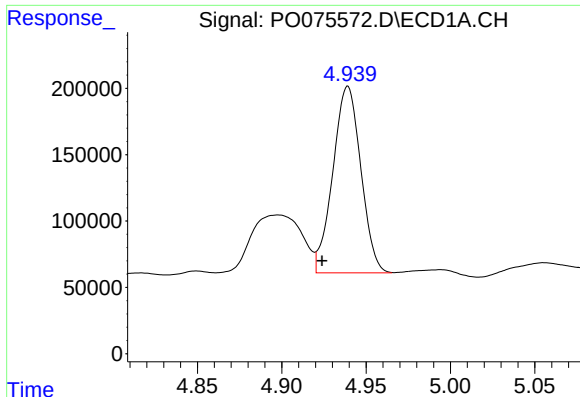


#1 Tetrachloro-m-xylene

R.T.: 4.939 min
Delta R.T.: 0.015 min
Response: 1620737
Conc: 16.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
WOOSPK-063-0002


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:39 PM

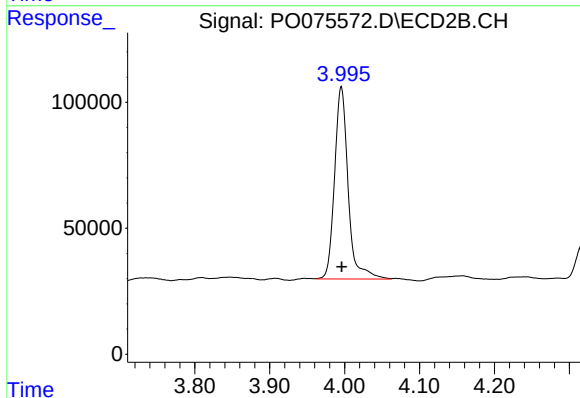


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.001 min
Response: 960344
Conc: 19.98 ng/ml m

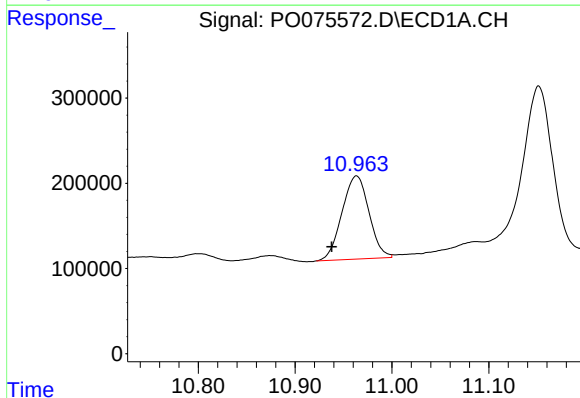

#2 Decachlorobiphenyl

R.T.: 10.963 min
Delta R.T.: 0.025 min
Response: 1892249
Conc: 19.61 ng/ml m

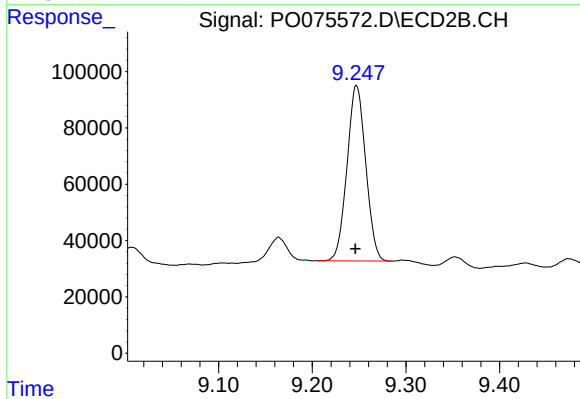

#2 Decachlorobiphenyl

R.T.: 9.247 min
Delta R.T.: 0.001 min
Response: 865125
Conc: 17.82 ng/ml