

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
 Data File : P0075574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2021 15:18
 Operator : AJ/MA
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 17:26:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Ankita

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

2/8/2021 4:50:41 PM

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.996	5530968	2682858	54.653	55.810
2) SA Decachlor...	10.941	9.245	5180328	2430889	53.692	50.079
Target Compounds						
26) L6 AR-1254-1	7.161	6.104	2140985	1566176	496.763	505.678
27) L6 AR-1254-2	7.391	6.262	3335321	1373351	494.697	511.425
28) L6 AR-1254-3	7.774	6.678	3513491	2149589	509.489m	504.125
29) L6 AR-1254-4	8.071	6.917	2835490	1436640	469.023	492.896
30) L6 AR-1254-5	8.501	7.342	2704434	1869234	483.809	481.621

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020521\
Data File : PO075574.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2021 15:18
Operator : AJ/MA
Sample : AR1254CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500



Manual Integrations
APPROVED


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 17:26:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Ankita

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

2/8/2021 4:50:41 PM

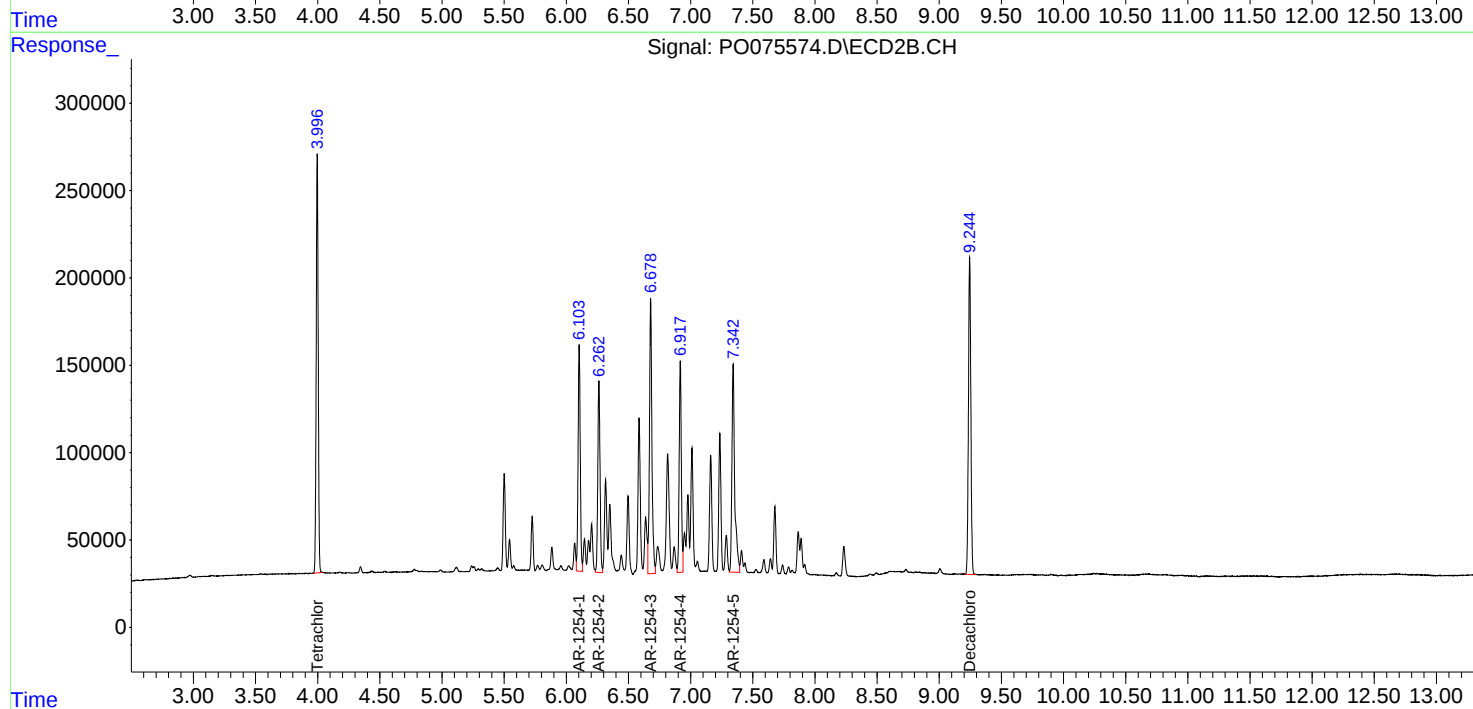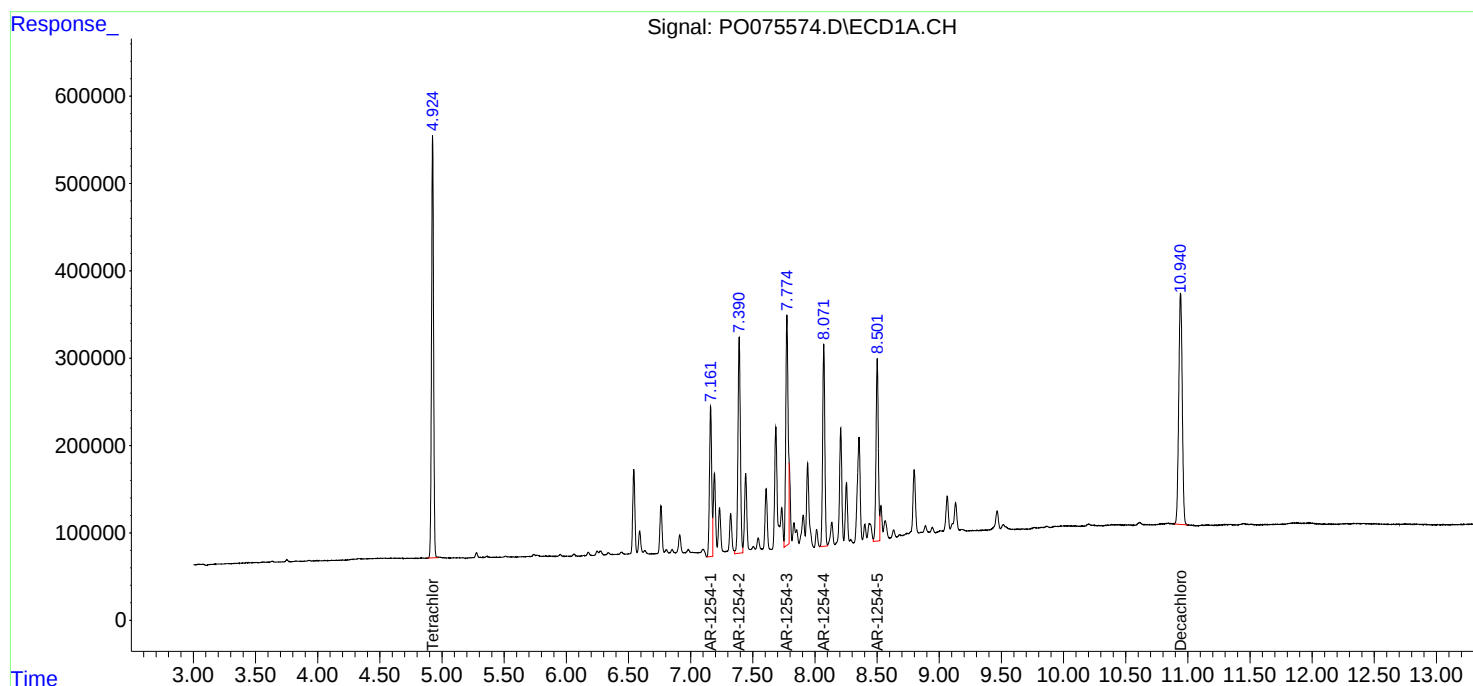

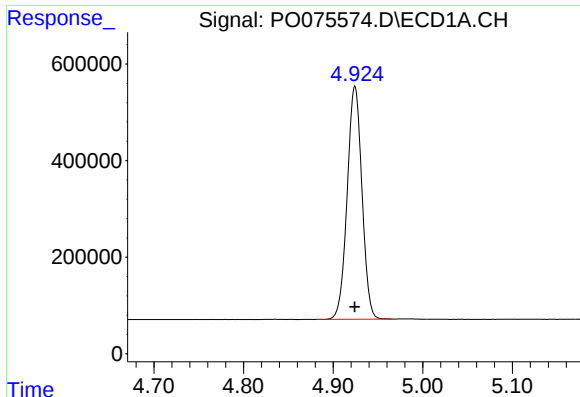


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 5530968
Conc: 54.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

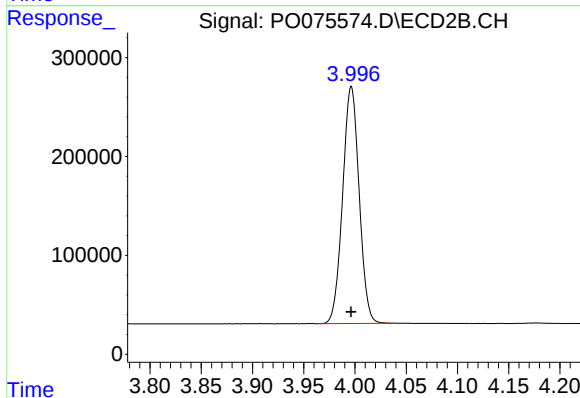


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 2682858
Conc: 55.81 ng/ml


Ankita

2/8/2021 4:50:41 PM

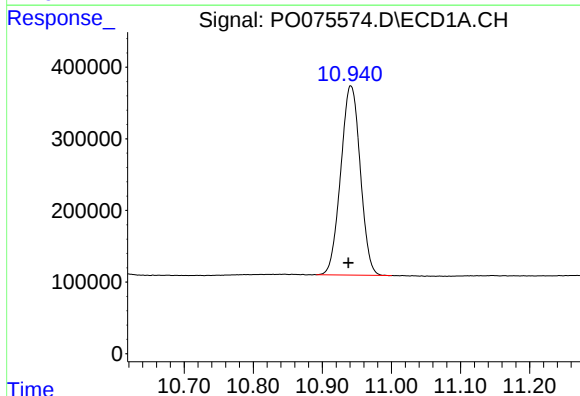


#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: 0.004 min
Response: 5180328
Conc: 53.69 ng/ml

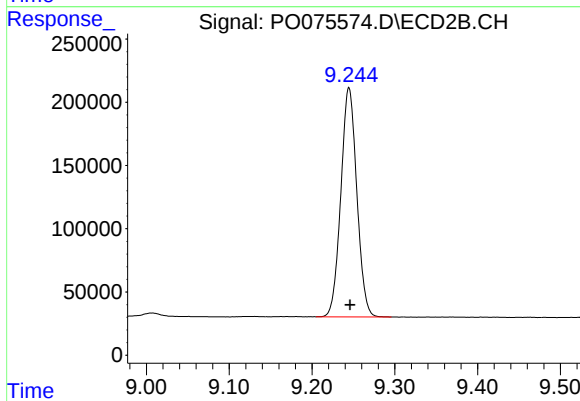

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.001 min
Response: 2430889
Conc: 50.08 ng/ml

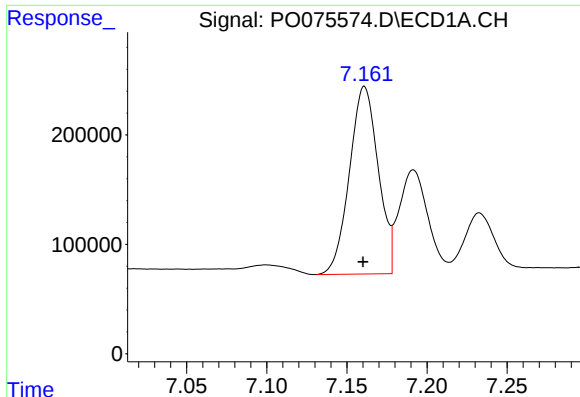


#26 AR-1254-1

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 2140985
Conc: 496.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:41 PM

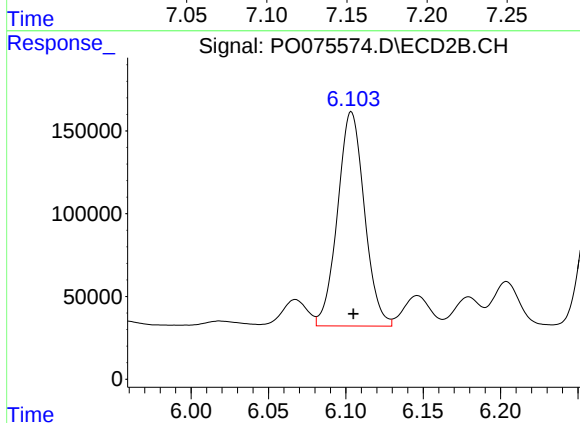


#26 AR-1254-1

R.T.: 6.104 min
Delta R.T.: -0.001 min
Response: 1566176
Conc: 505.68 ng/ml

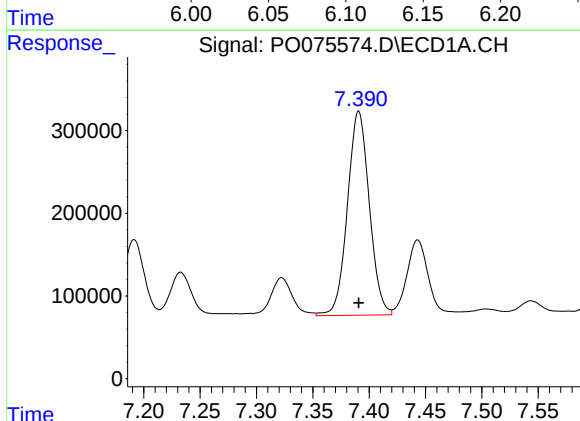


#27 AR-1254-2

R.T.: 7.391 min
Delta R.T.: 0.000 min
Response: 3335321
Conc: 494.70 ng/ml

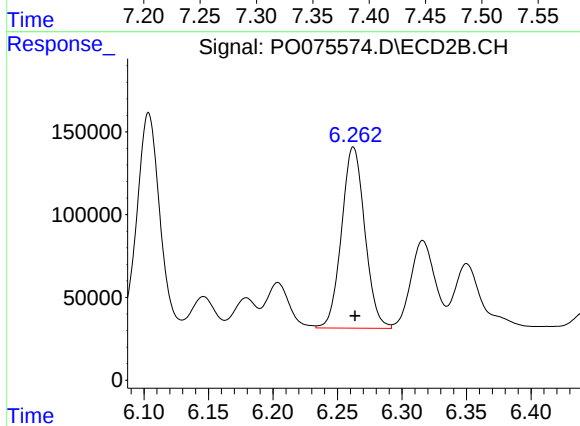

#27 AR-1254-2

R.T.: 6.262 min
Delta R.T.: -0.001 min
Response: 1373351
Conc: 511.43 ng/ml

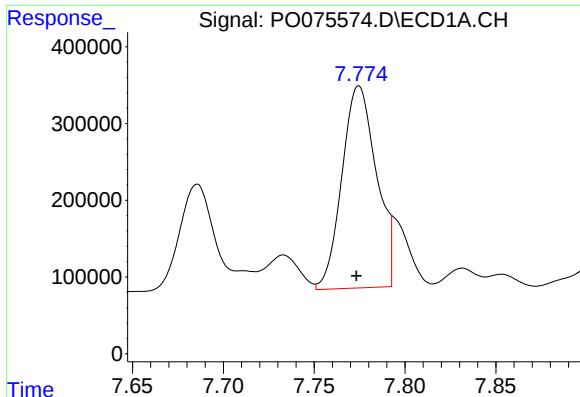


#28 AR-1254-3

R.T.: 7.774 min
Delta R.T.: 0.001 min
Response: 3513491
Conc: 509.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:41 PM

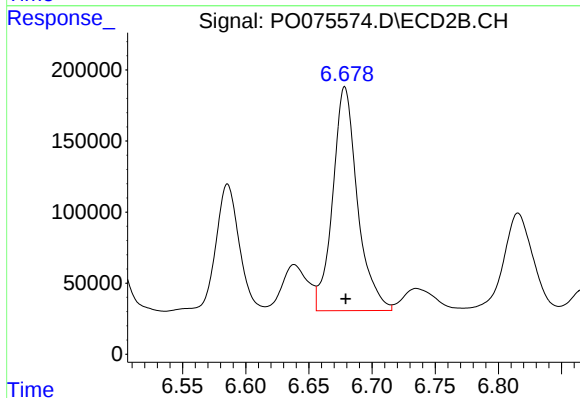


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 2149589
Conc: 504.13 ng/ml

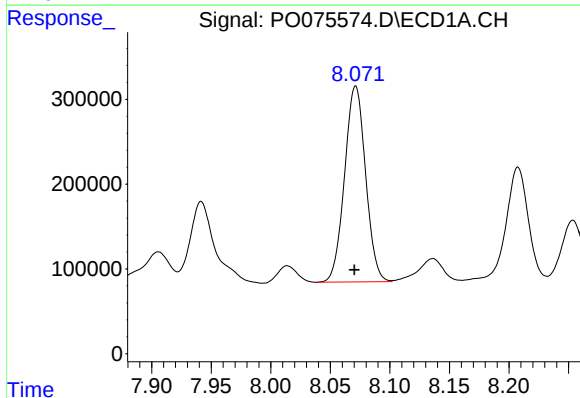


#29 AR-1254-4

R.T.: 8.071 min
Delta R.T.: 0.000 min
Response: 2835490
Conc: 469.02 ng/ml

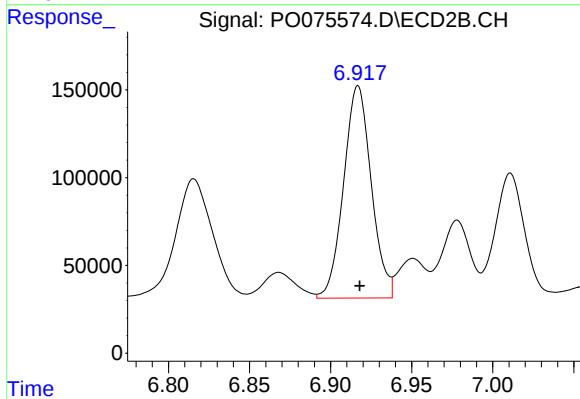

#29 AR-1254-4

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 1436640
Conc: 492.90 ng/ml

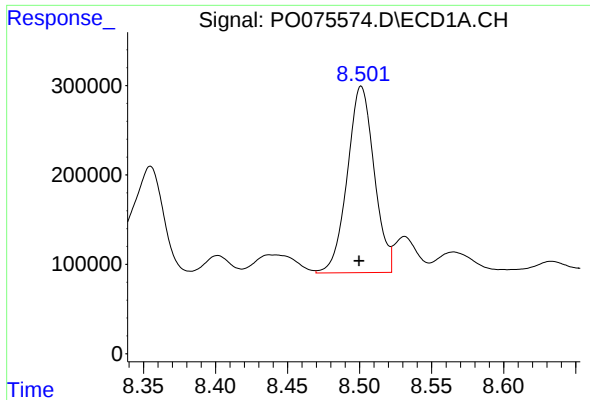


#30 AR-1254-5

R.T.: 8.501 min
Delta R.T.: 0.002 min
Response: 2704434
Conc: 483.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
2/8/2021 4:50:41 PM

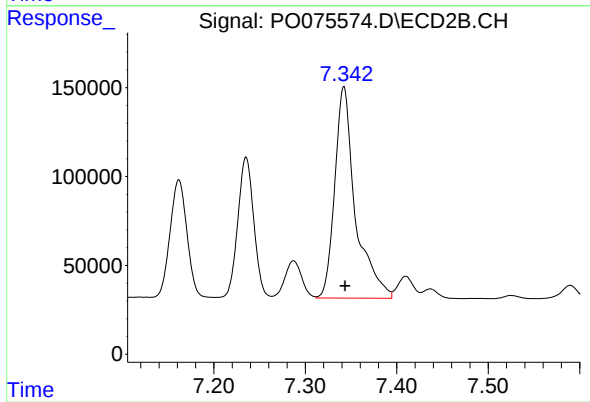

#30 AR-1254-5

R.T.: 7.342 min
Delta R.T.: -0.001 min
Response: 1869234
Conc: 481.62 ng/ml