

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
 Data File : P0075580.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2021 18:10
 Operator : AJ/MA
 Sample : M1291-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-008-1015

Manual Integrations
 APPROVED

Ankita
 2/8/2021 4:51:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 23:56:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.994	2144689	1064986	21.192	22.154
2) SA Decachlor...	10.937	9.244	1904724	939327	19.742	19.351
Target Compounds						
36) L8 AR-1262-1	8.574	7.339	82783	12261	9.486m	5.621m#
37) L8 AR-1262-2	9.128	7.886	83506	54278	5.522m	7.078 #
38) L8 AR-1262-3	9.439	8.171	148274	65168	14.193	19.692 #
39) L8 AR-1262-4	9.536	8.236	153820	74701	20.811	13.010 #
40) L8 AR-1262-5	10.195	8.729	87197	47071	16.814m	17.111

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
Data File : P0075580.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2021 18:10
Operator : AJ/MA
Sample : M1291-15
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
OU421-008-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 23:56:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

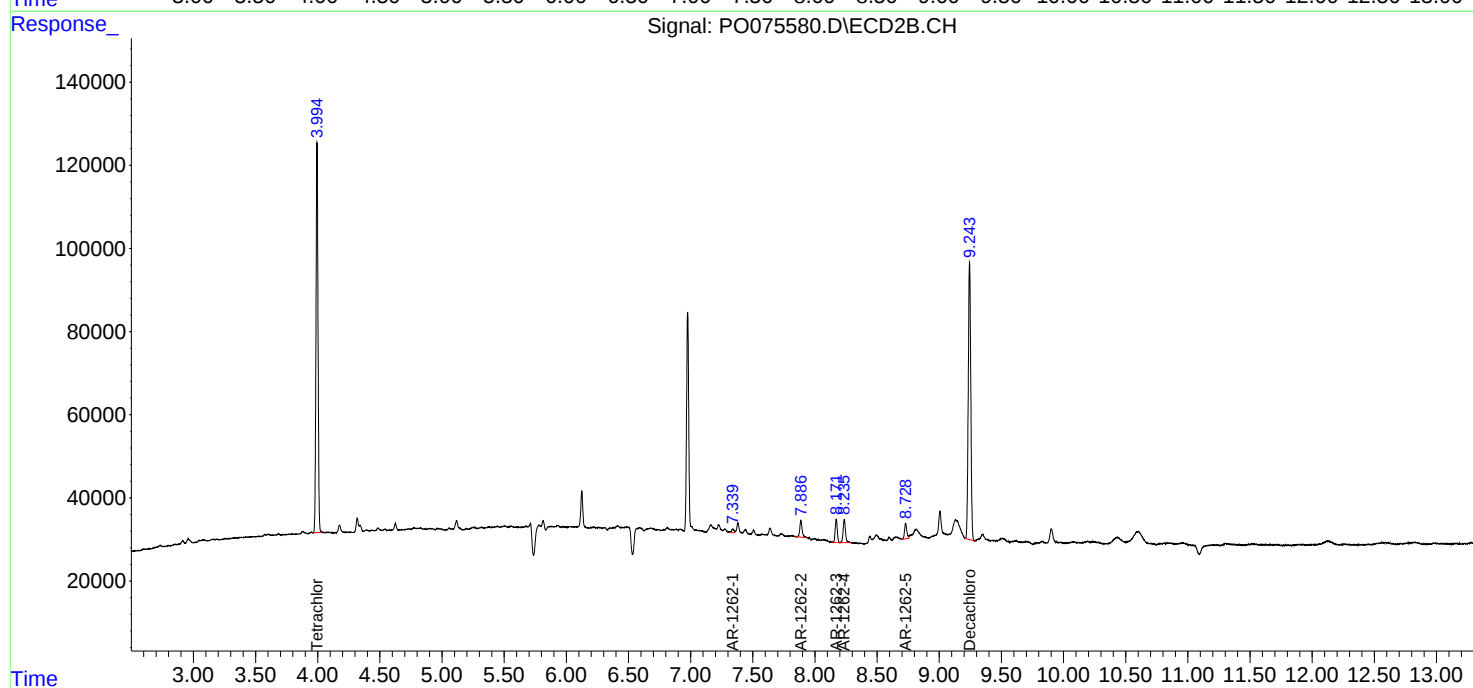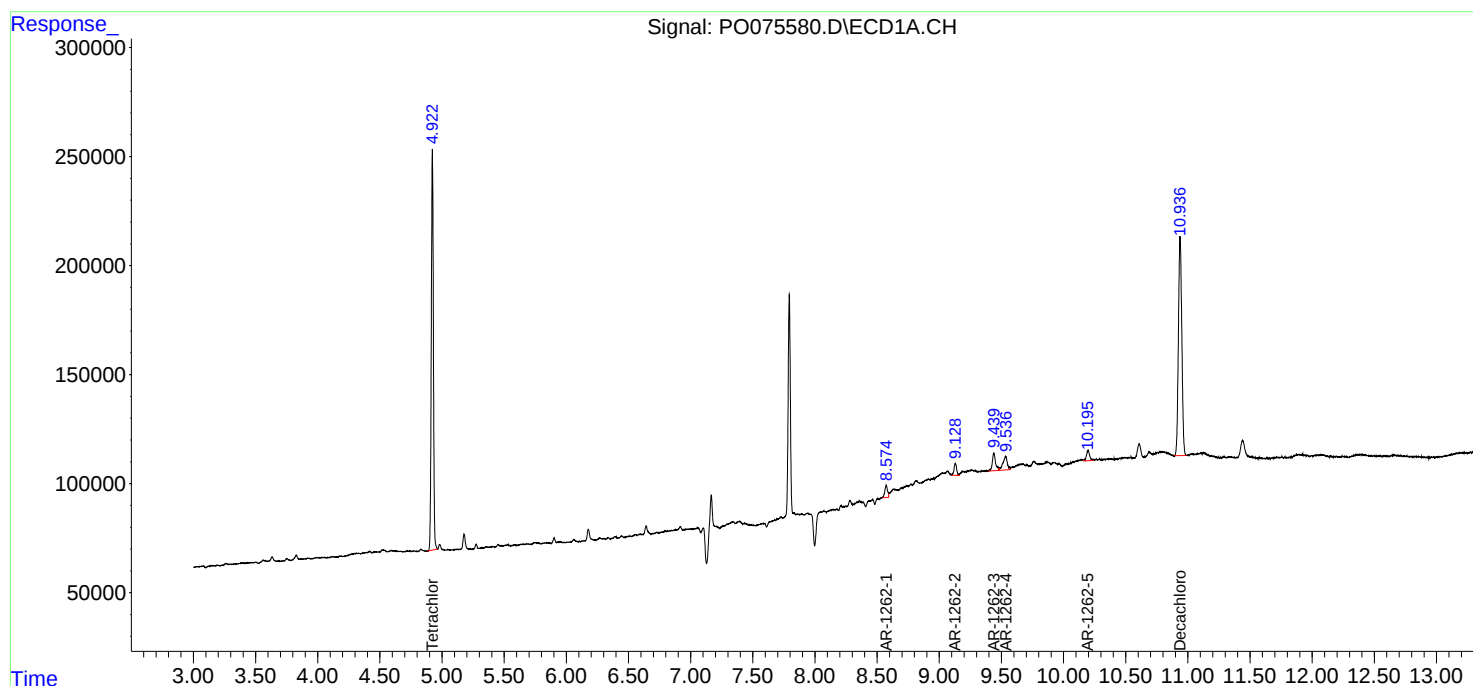

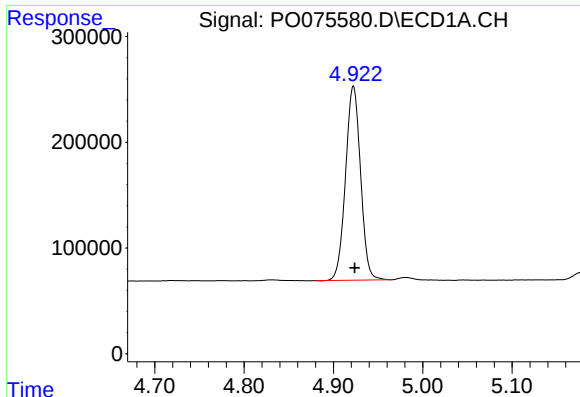


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 2144689
Conc: 21.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-008-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:02 PM

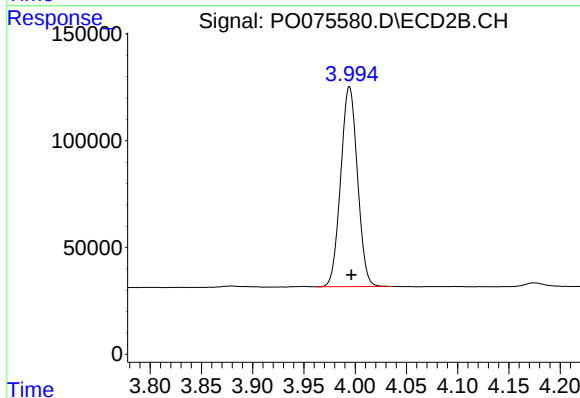


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1064986
Conc: 22.15 ng/ml

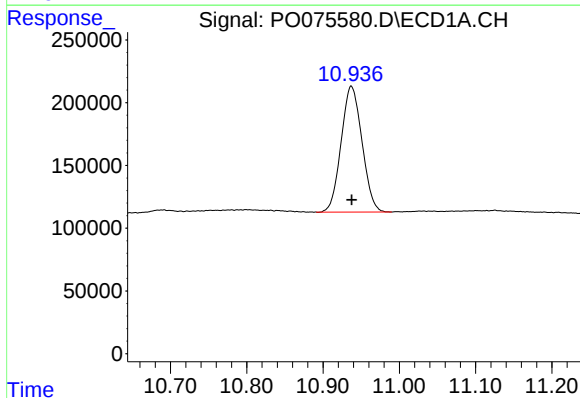


#2 Decachlorobiphenyl

R.T.: 10.937 min
Delta R.T.: 0.000 min
Response: 1904724
Conc: 19.74 ng/ml

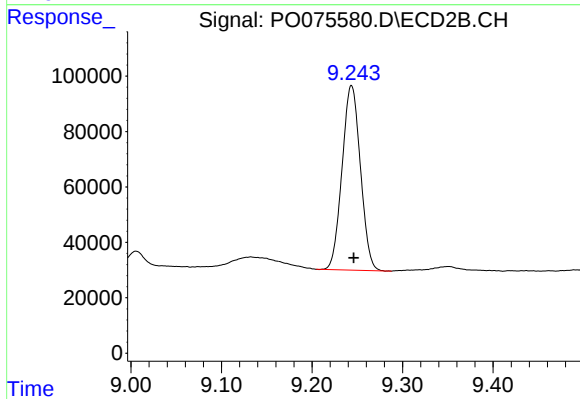

#2 Decachlorobiphenyl

R.T.: 9.244 min
Delta R.T.: -0.002 min
Response: 939327
Conc: 19.35 ng/ml

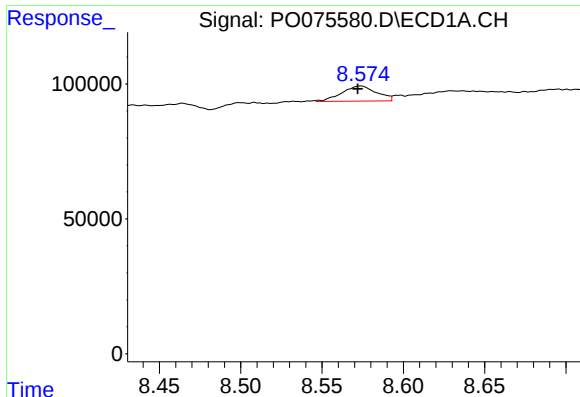


#36 AR-1262-1

R.T.: 8.574 min
Delta R.T.: 0.002 min
Response: 82783
Conc: 9.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-008-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:02 PM

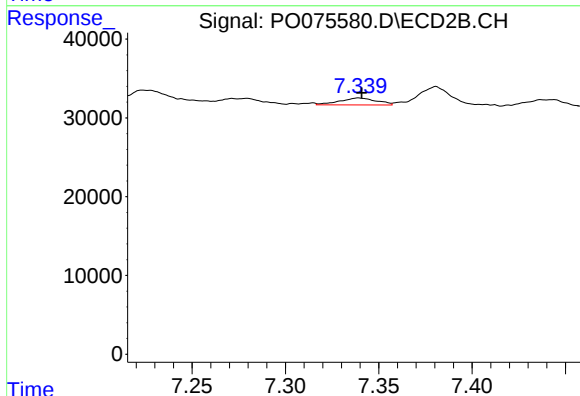


#36 AR-1262-1

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 12261
Conc: 5.62 ng/ml m

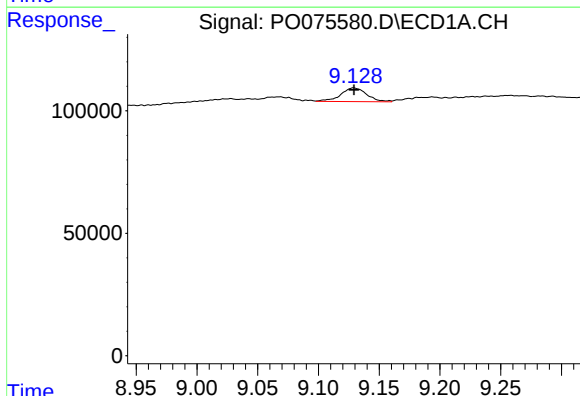


#37 AR-1262-2

R.T.: 9.128 min
Delta R.T.: 0.000 min
Response: 83506
Conc: 5.52 ng/ml m

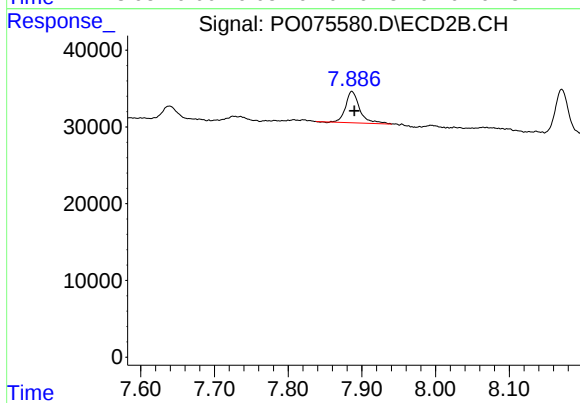

#37 AR-1262-2

R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 54278
Conc: 7.08 ng/ml

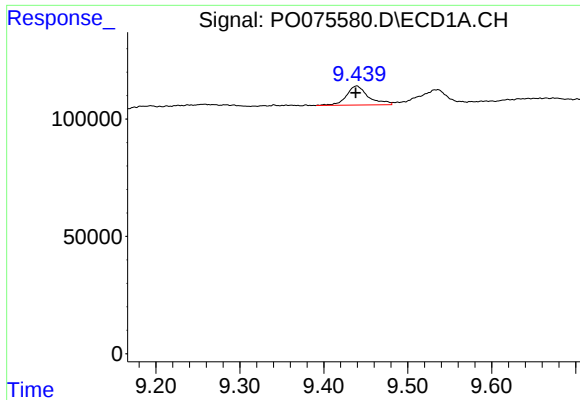


#38 AR-1262-3

R.T.: 9.439 min
Delta R.T.: 0.000 min
Response: 148274
Conc: 14.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-008-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:02 PM

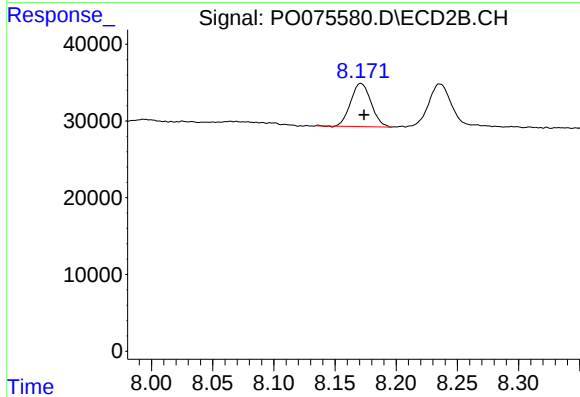


#38 AR-1262-3

R.T.: 8.171 min
Delta R.T.: -0.002 min
Response: 65168
Conc: 19.69 ng/ml

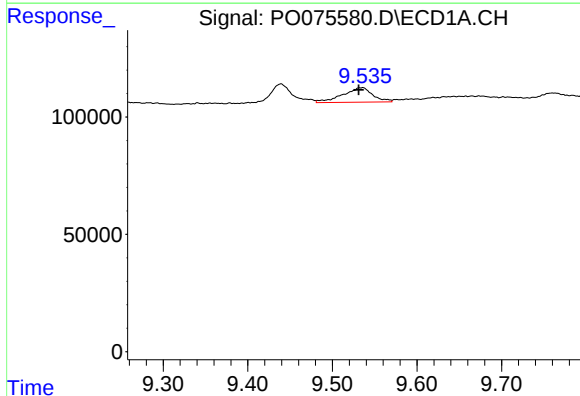


#39 AR-1262-4

R.T.: 9.536 min
Delta R.T.: 0.004 min
Response: 153820
Conc: 20.81 ng/ml

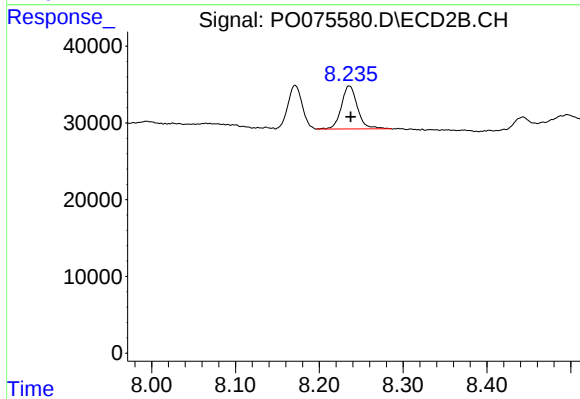

#39 AR-1262-4

R.T.: 8.236 min
Delta R.T.: -0.002 min
Response: 74701
Conc: 13.01 ng/ml

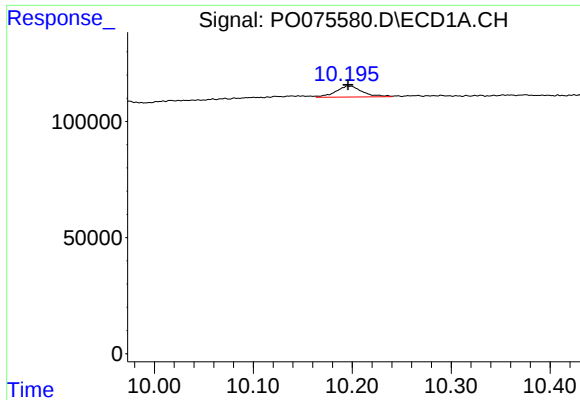


#40 AR-1262-5

R.T.: 10.195 min
Delta R.T.: -0.001 min
Response: 87197
Conc: 16.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-008-1015

Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:02 PM

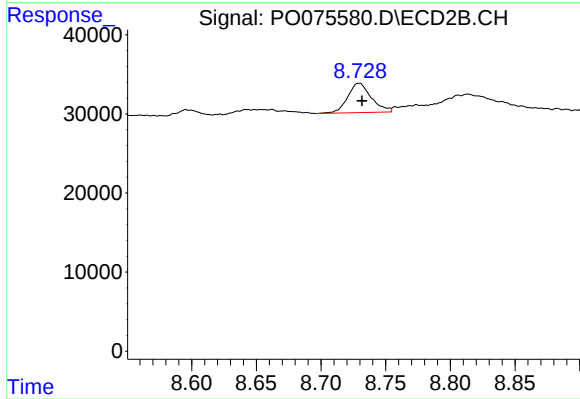

#40 AR-1262-5

R.T.: 8.729 min
Delta R.T.: -0.002 min
Response: 47071
Conc: 17.11 ng/ml