

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
 Data File : P0075584.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2021 19:18
 Operator : AJ/MA
 Sample : M1291-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-004-1015

Manual Integrations
 APPROVED

Ankita
 2/8/2021 4:51:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 23:58:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.994	2171425	1089839	21.456	22.671
2) SA Decachlor...	10.936	9.243	2022404	956166	20.961	19.698
Target Compounds						
36) L8 AR-1262-1	8.572	7.338	155606	43591	17.832	19.985
37) L8 AR-1262-2	9.130	7.887	156201	83609	10.329m	10.902
38) L8 AR-1262-3	9.438	8.171	289096	141488	27.673	42.754 #
39) L8 AR-1262-4	9.534	8.235	290345	147851	39.283	25.750 #
40) L8 AR-1262-5	10.197	8.729	194999	83402	37.602	30.319

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
Data File : P0075584.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2021 19:18
Operator : AJ/MA
Sample : M1291-19
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OU421-004-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 23:58:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

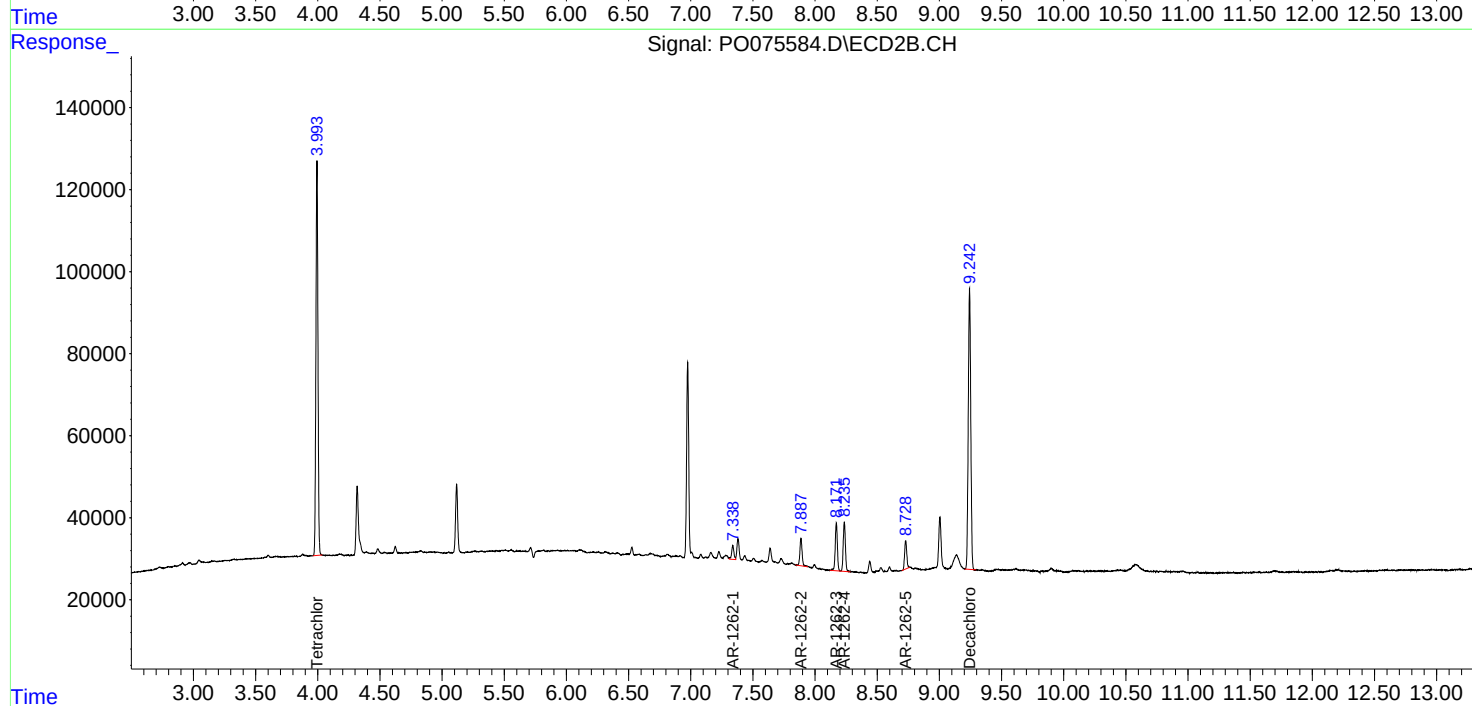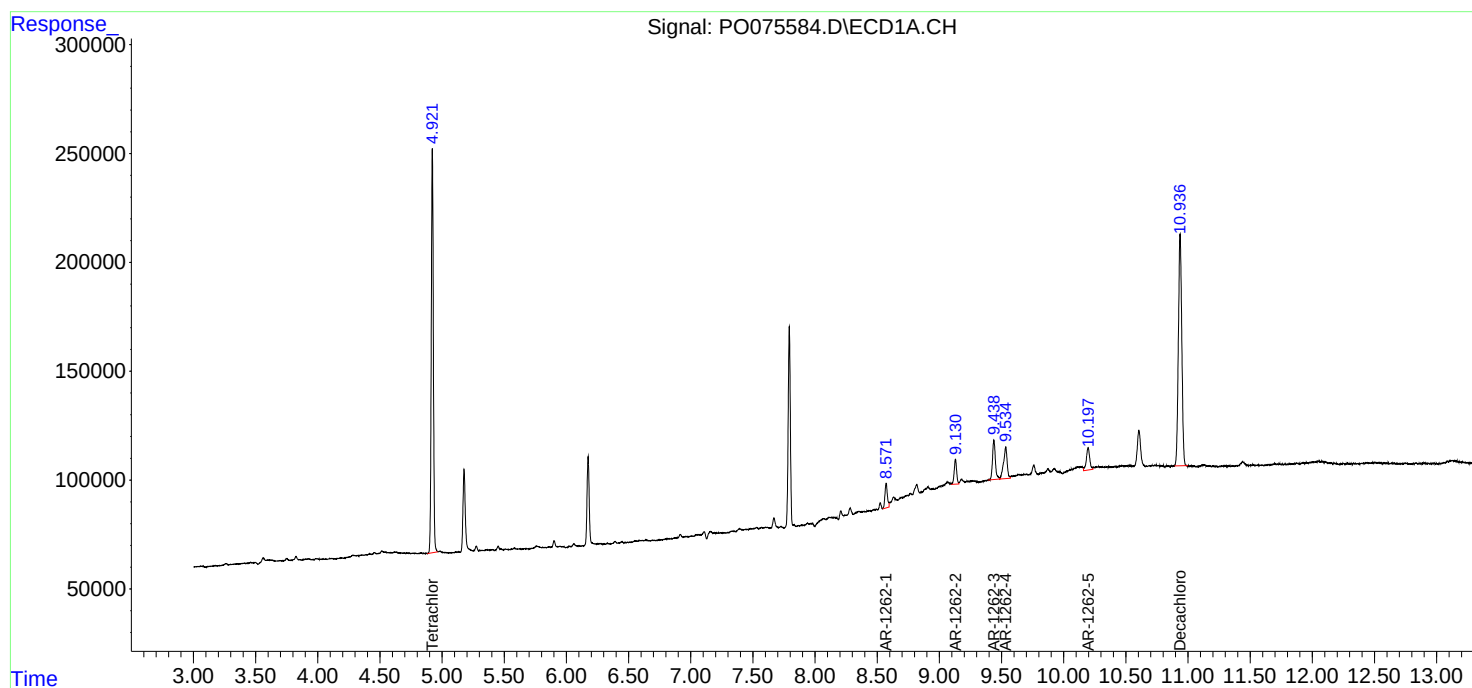

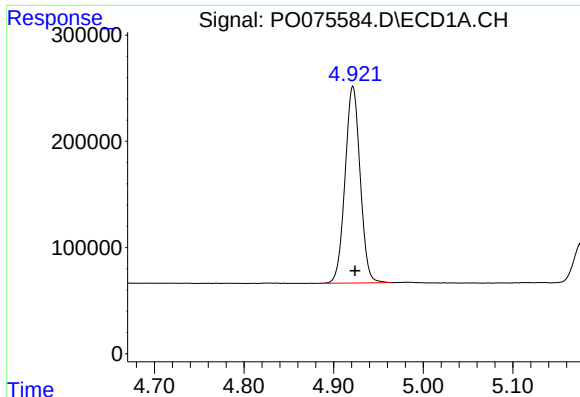


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 2171425
Conc: 21.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:36 PM

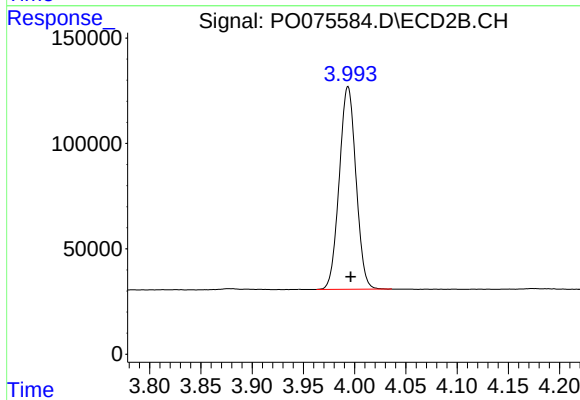


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.003 min
Response: 1089839
Conc: 22.67 ng/ml

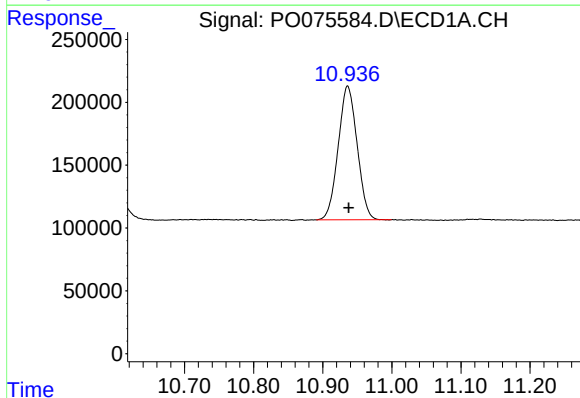


#2 Decachlorobiphenyl

R.T.: 10.936 min
Delta R.T.: -0.002 min
Response: 2022404
Conc: 20.96 ng/ml

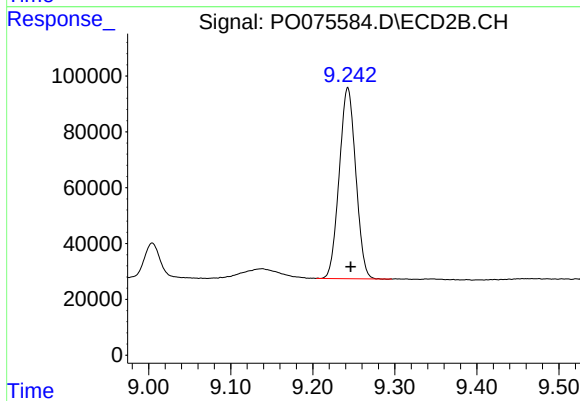

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 956166
Conc: 19.70 ng/ml

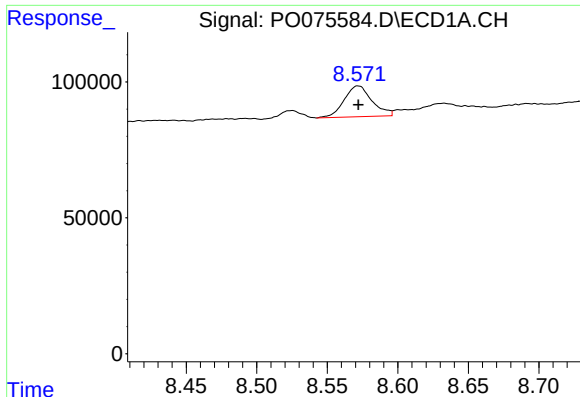


#36 AR-1262-1

R.T.: 8.572 min
Delta R.T.: 0.000 min
Response: 155606
Conc: 17.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:36 PM

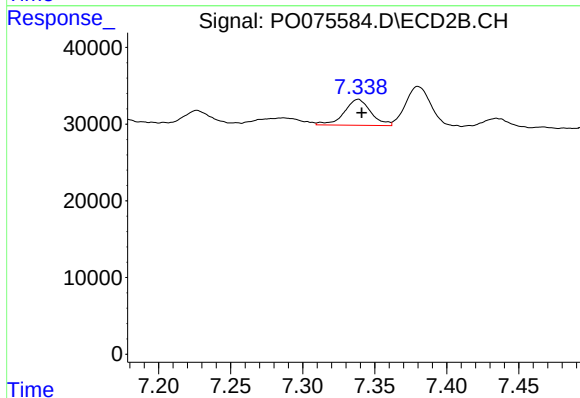


#36 AR-1262-1

R.T.: 7.338 min
Delta R.T.: -0.003 min
Response: 43591
Conc: 19.98 ng/ml

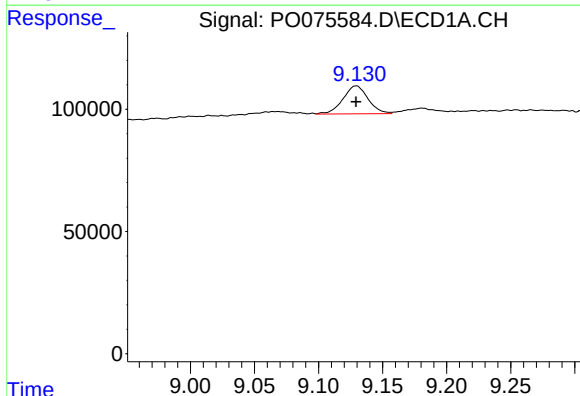


#37 AR-1262-2

R.T.: 9.130 min
Delta R.T.: 0.000 min
Response: 156201
Conc: 10.33 ng/ml m

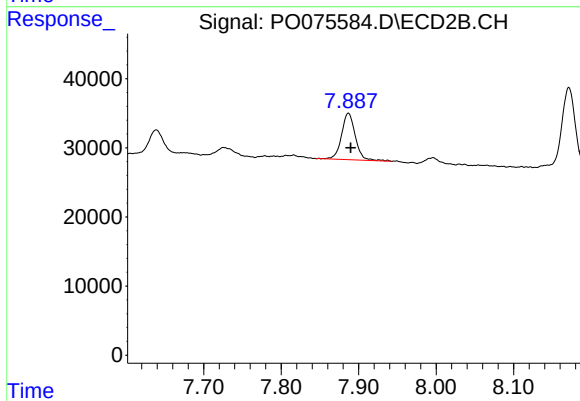

#37 AR-1262-2

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 83609
Conc: 10.90 ng/ml

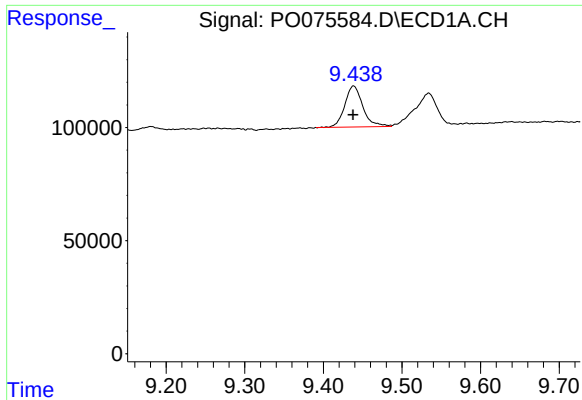


#38 AR-1262-3

R.T.: 9.438 min
Delta R.T.: 0.000 min
Response: 289096
Conc: 27.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-1015


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:36 PM

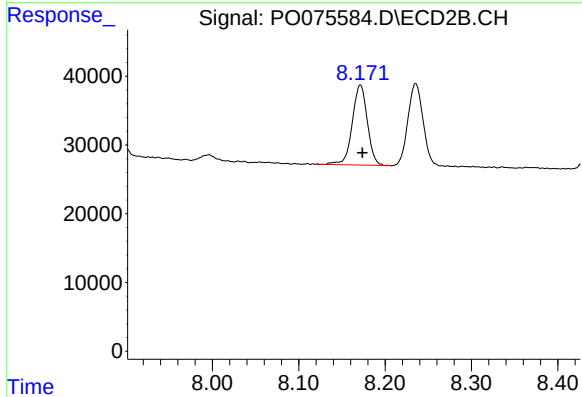


#38 AR-1262-3

R.T.: 8.171 min
Delta R.T.: -0.002 min
Response: 141488
Conc: 42.75 ng/ml

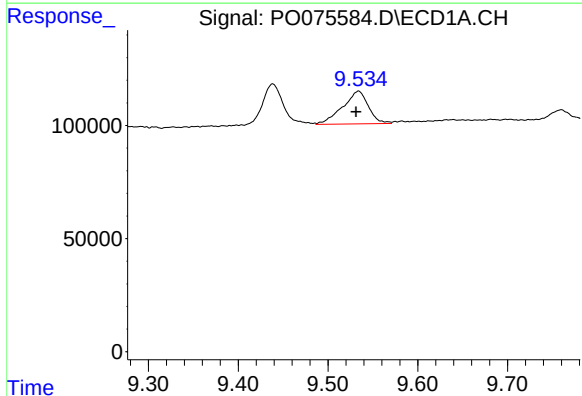


#39 AR-1262-4

R.T.: 9.534 min
Delta R.T.: 0.003 min
Response: 290345
Conc: 39.28 ng/ml

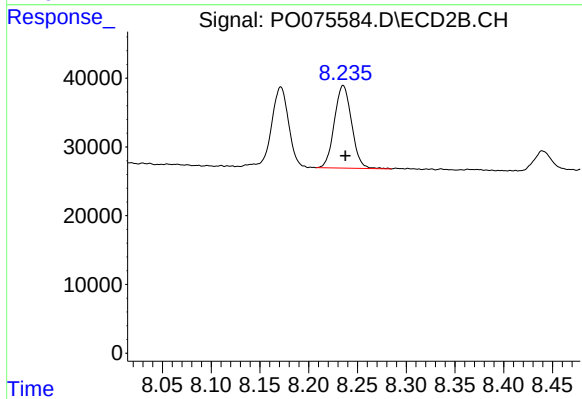

#39 AR-1262-4

R.T.: 8.235 min
Delta R.T.: -0.002 min
Response: 147851
Conc: 25.75 ng/ml

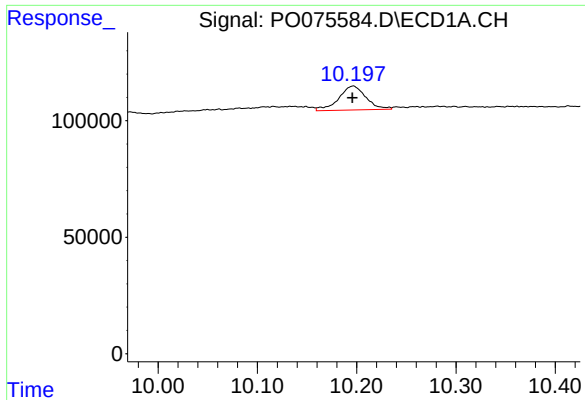


#40 AR-1262-5

R.T.: 10.197 min
Delta R.T.: 0.000 min
Response: 194999
Conc: 37.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-1015

Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:36 PM

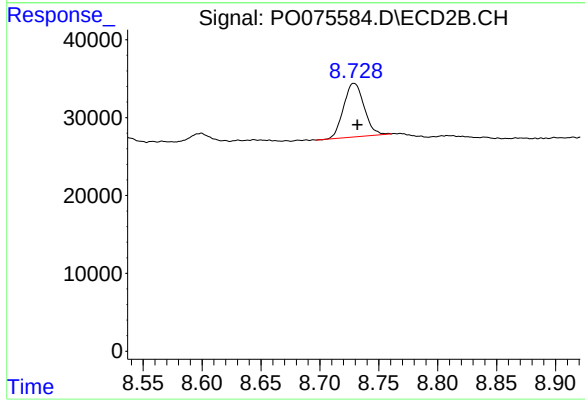

#40 AR-1262-5

R.T.: 8.729 min
Delta R.T.: -0.003 min
Response: 83402
Conc: 30.32 ng/ml