

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
 Data File : P0075607.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Feb 2021 4:09
 Operator : AJ/MA
 Sample : M1315-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TS-1

Manual Integrations
 APPROVED

Ankita
 2/8/2021 4:51:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 05:03:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.922	3.994	1658847	827144	16.391	17.207
2)	SA Decachlor...	10.935	9.241	1790505	887897	18.558	18.291
Target Compounds							
26)	L6 AR-1254-1	7.157	6.100	129225	94837	29.983	30.621
27)	L6 AR-1254-2	7.387	6.259	480552	145717	71.276m	54.264
28)	L6 AR-1254-3	7.771	6.675	500530	335045	72.581m	78.575
29)	L6 AR-1254-4	8.067	6.913	575657	284749	95.220	97.694
30)	L6 AR-1254-5	8.497	7.338	676354	1131868	120.996	291.634 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020521\
Data File : PO075607.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Feb 2021 4:09
Operator : AJ/MA
Sample : M1315-04
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TS-1


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 05:03:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

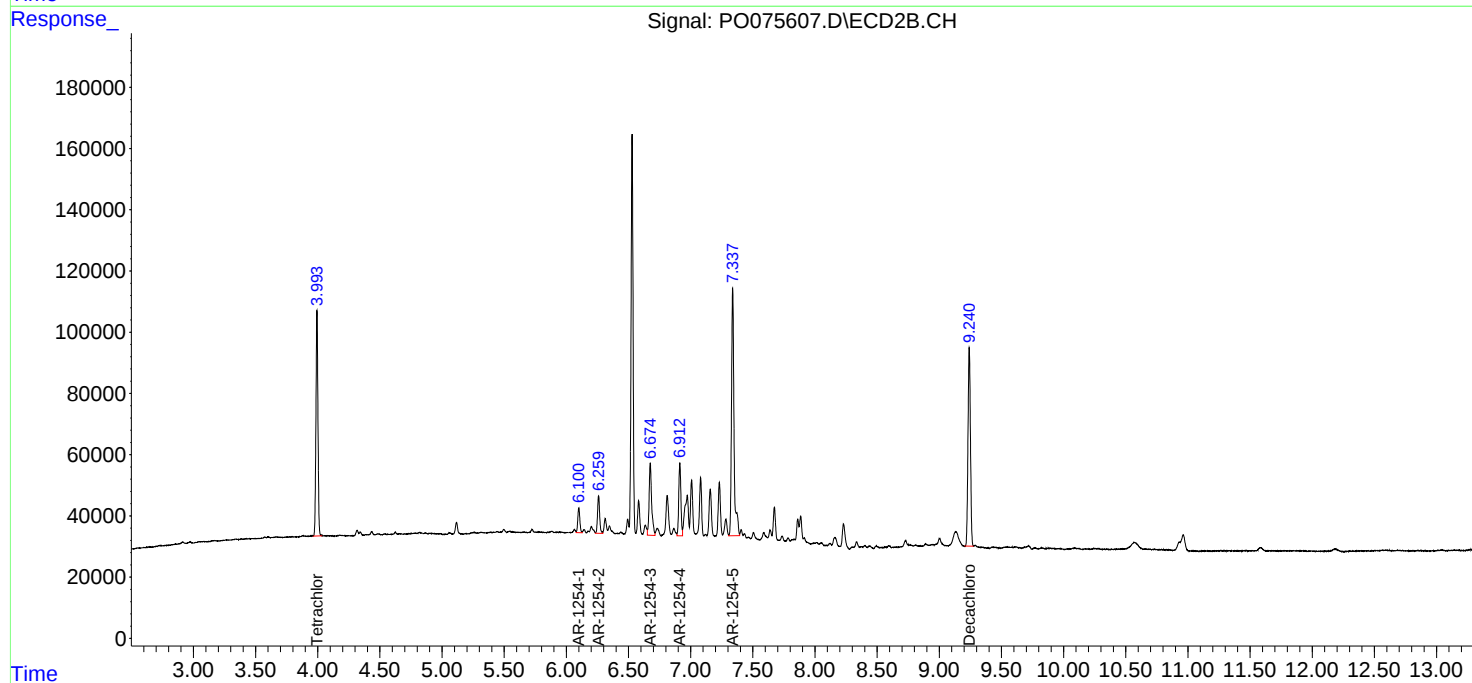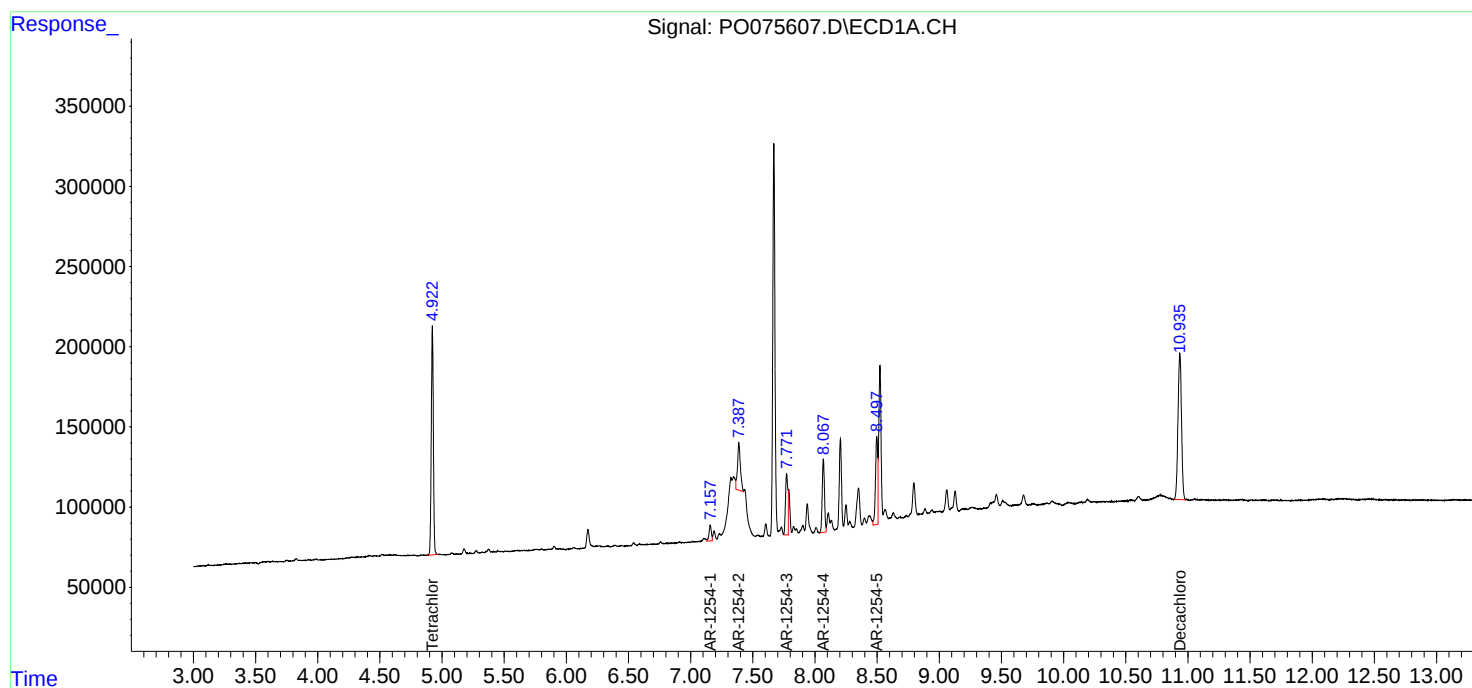

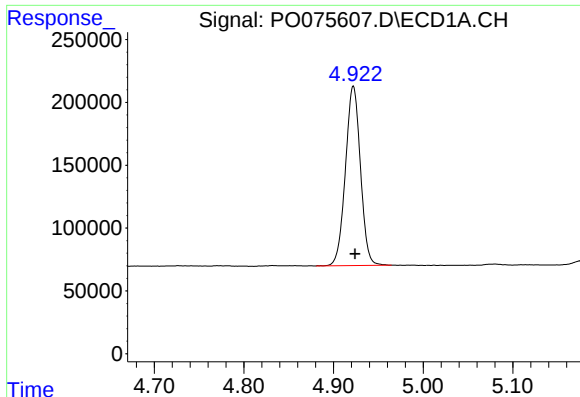


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 1658847
Conc: 16.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
TS-1


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:48 PM

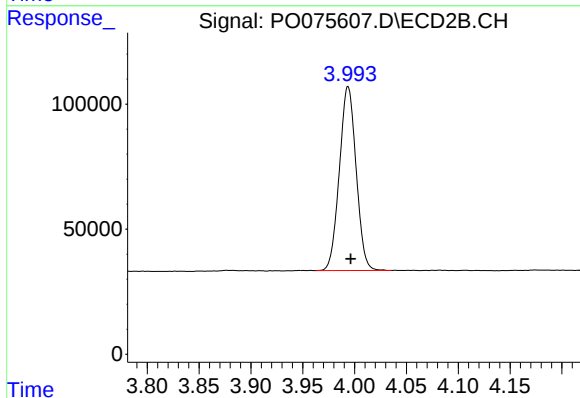


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.003 min
Response: 827144
Conc: 17.21 ng/ml

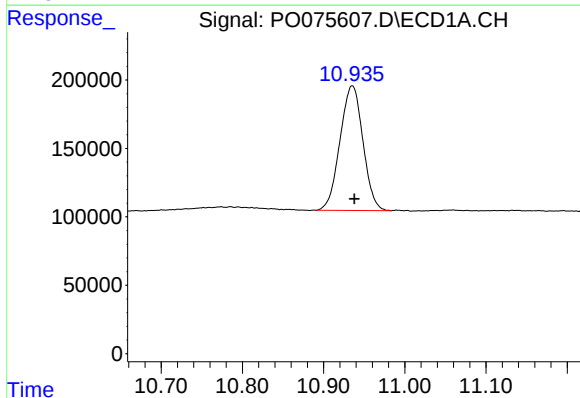


#2 Decachlorobiphenyl

R.T.: 10.935 min
Delta R.T.: -0.003 min
Response: 1790505
Conc: 18.56 ng/ml

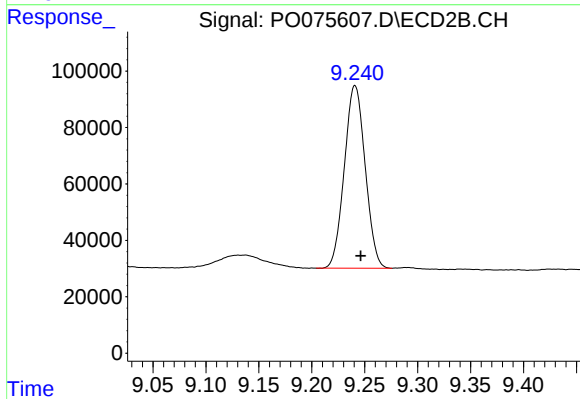

#2 Decachlorobiphenyl

R.T.: 9.241 min
Delta R.T.: -0.005 min
Response: 887897
Conc: 18.29 ng/ml

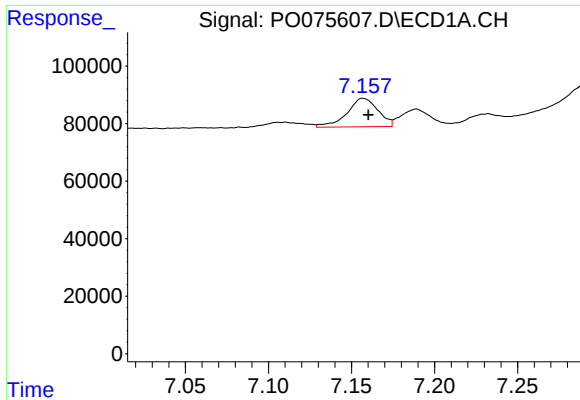


#26 AR-1254-1

R.T.: 7.157 min
Delta R.T.: -0.003 min
Response: 129225
Conc: 29.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TS-1


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:48 PM

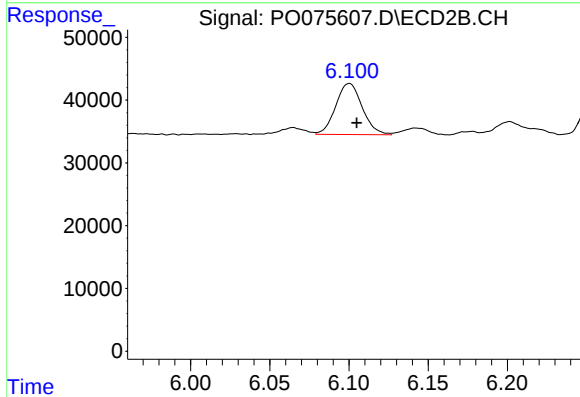


#26 AR-1254-1

R.T.: 6.100 min
Delta R.T.: -0.004 min
Response: 94837
Conc: 30.62 ng/ml

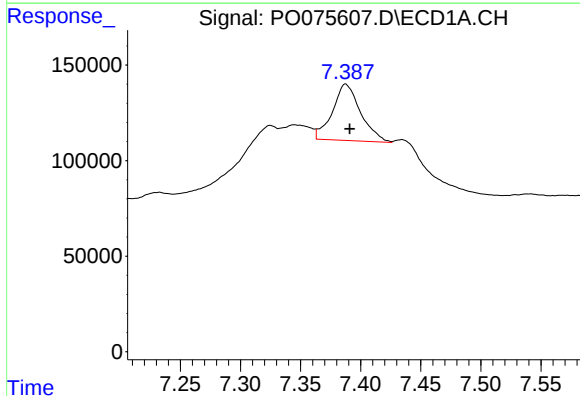


#27 AR-1254-2

R.T.: 7.387 min
Delta R.T.: -0.004 min
Response: 480552
Conc: 71.28 ng/ml m

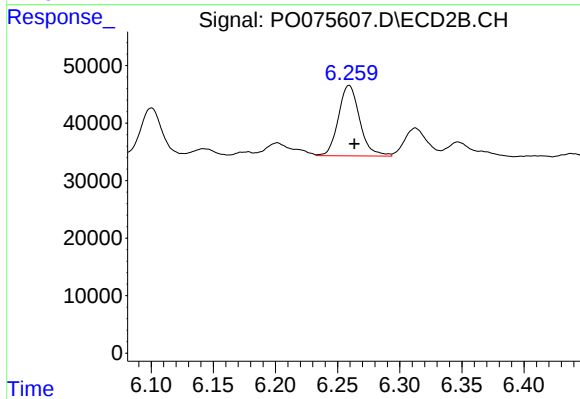

#27 AR-1254-2

R.T.: 6.259 min
Delta R.T.: -0.004 min
Response: 145717
Conc: 54.26 ng/ml

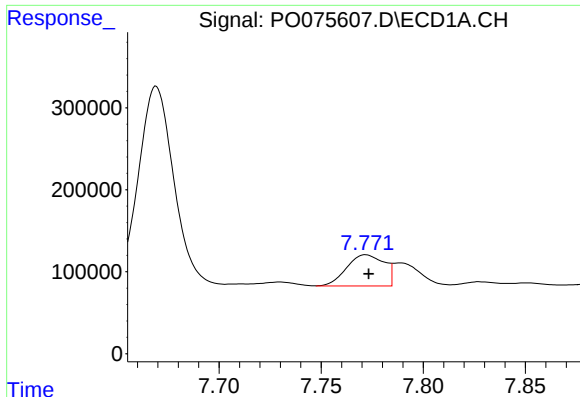


#28 AR-1254-3

R.T.: 7.771 min
Delta R.T.: -0.002 min
Response: 500530
Conc: 72.58 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TS-1


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:48 PM

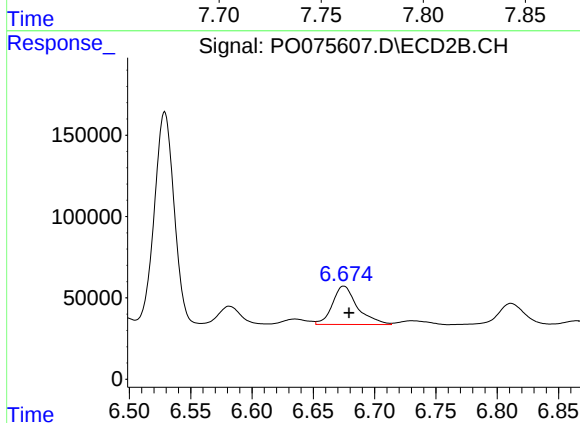


#28 AR-1254-3

R.T.: 6.675 min
Delta R.T.: -0.004 min
Response: 335045
Conc: 78.58 ng/ml

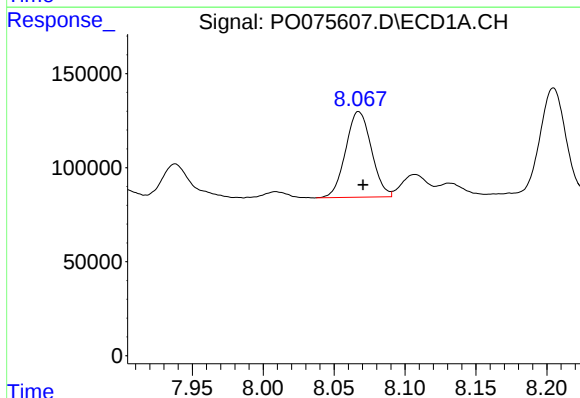


#29 AR-1254-4

R.T.: 8.067 min
Delta R.T.: -0.003 min
Response: 575657
Conc: 95.22 ng/ml

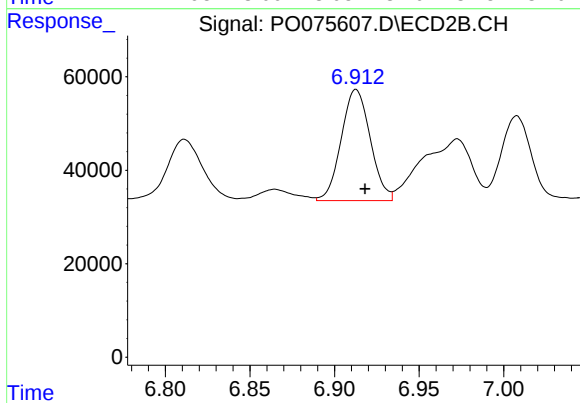

#29 AR-1254-4

R.T.: 6.913 min
Delta R.T.: -0.005 min
Response: 284749
Conc: 97.69 ng/ml

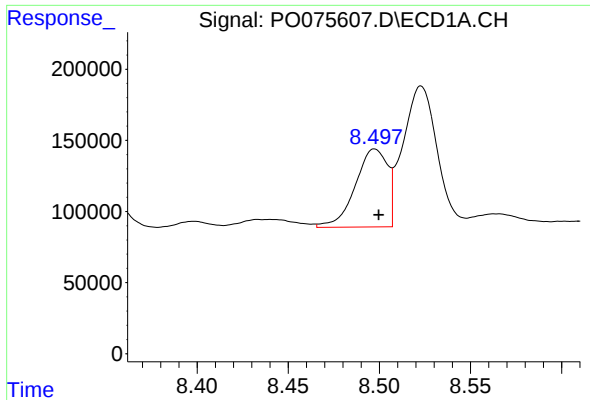


#30 AR-1254-5

R.T.: 8.497 min
Delta R.T.: -0.002 min
Response: 676354
Conc: 121.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
TS-1

Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:48 PM

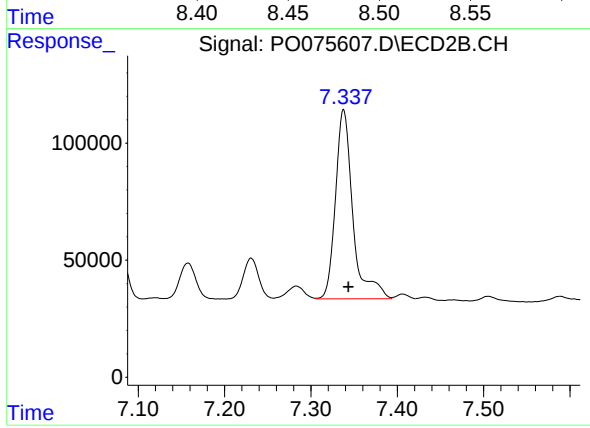

#30 AR-1254-5

R.T.: 7.338 min
Delta R.T.: -0.005 min
Response: 1131868
Conc: 291.63 ng/ml