

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020521\
 Data File : P0075610.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Feb 2021 5:01
 Operator : AJ/MA
 Sample : M1324-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Ankita
 2/8/2021 4:51:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 06:09:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.912	3.996	45559363	1086227	450.182	22.596 #
2) SA Decachlor...	10.943	9.246	122.3E6	26692139	1267.256m	549.882m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020521\
Data File : PO075610.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Feb 2021 5:01
Operator : AJ/MA
Sample : M1324-03
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 06:09:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

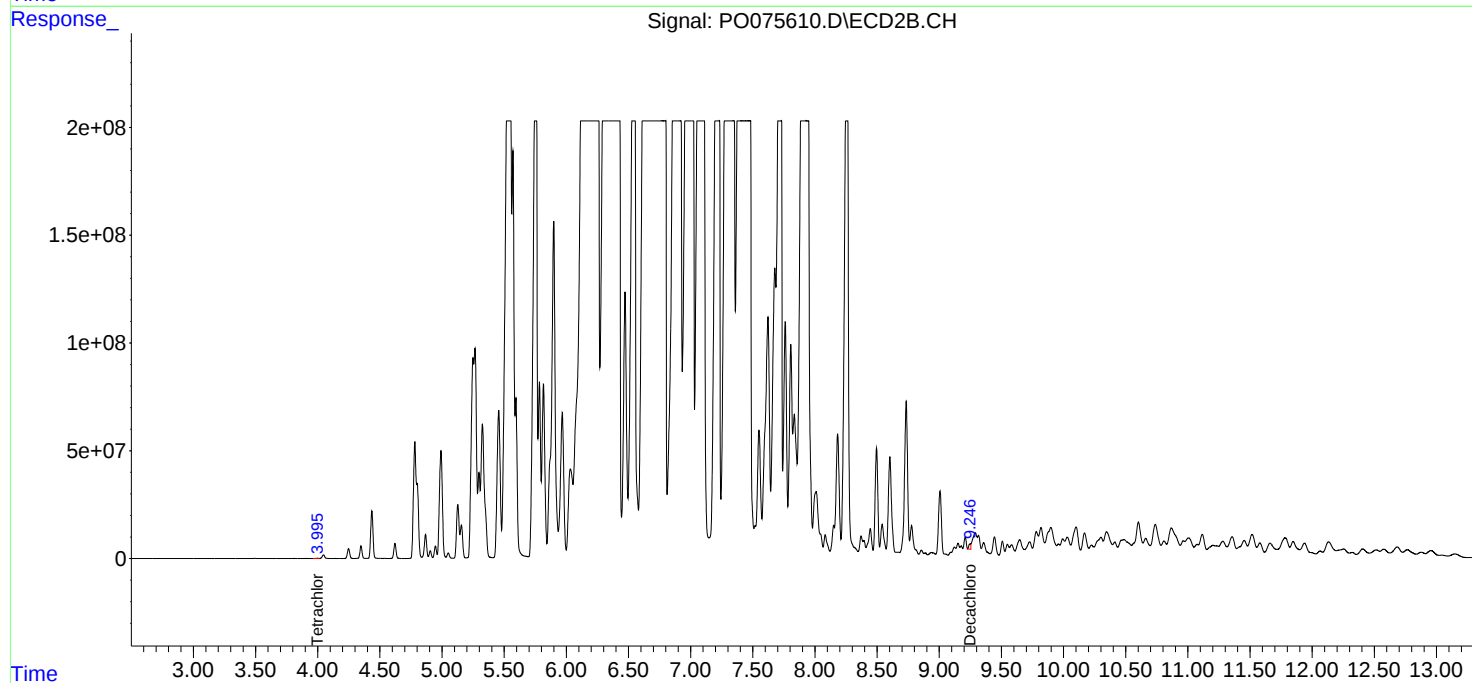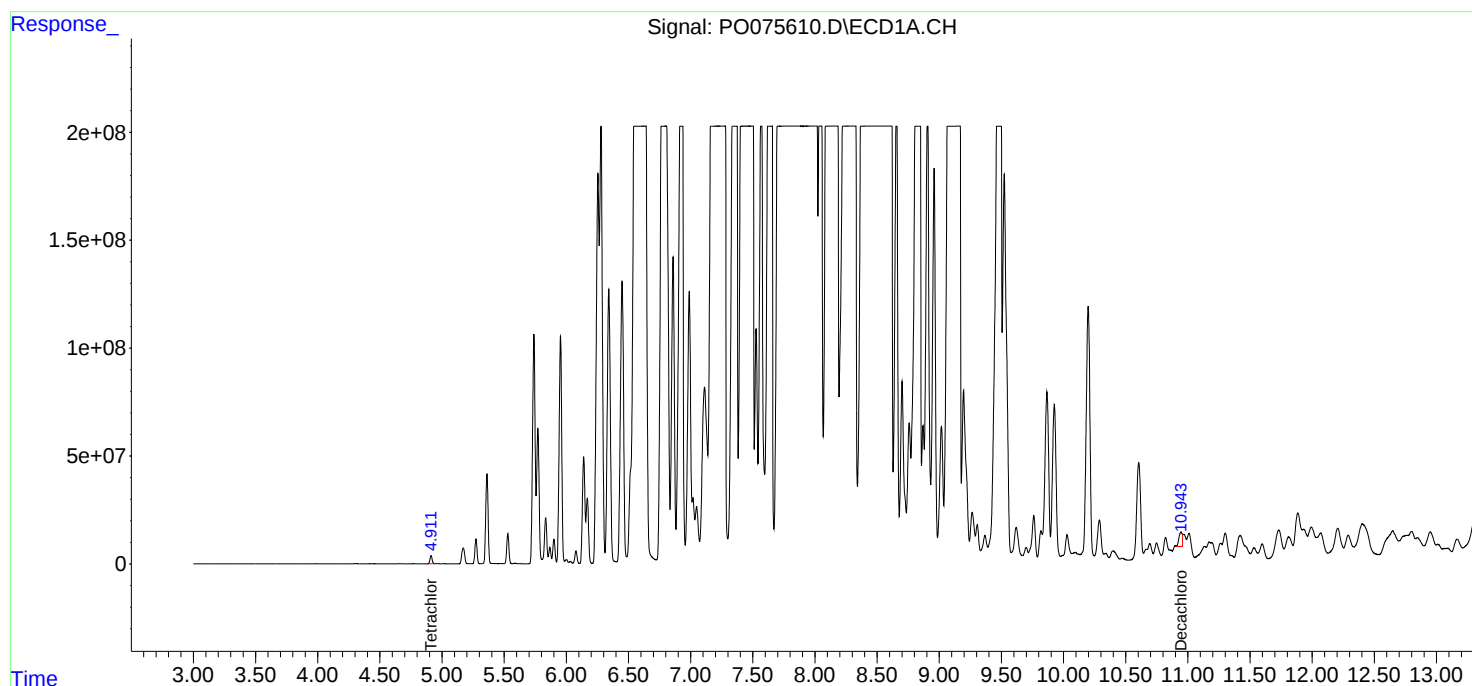

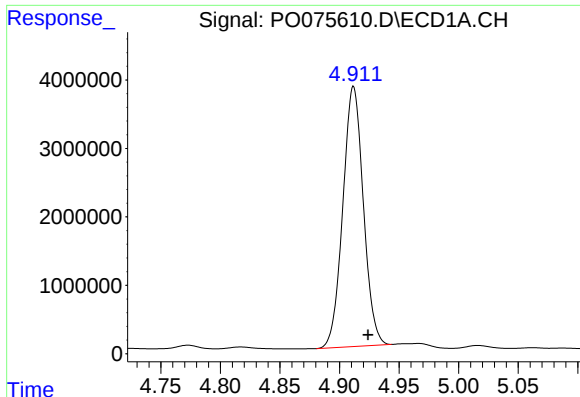


#1 Tetrachloro-m-xylene

R.T.: 4.912 min
Delta R.T.: -0.012 min
Response: 45559363
Conc: 450.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
2/8/2021 4:51:54 PM

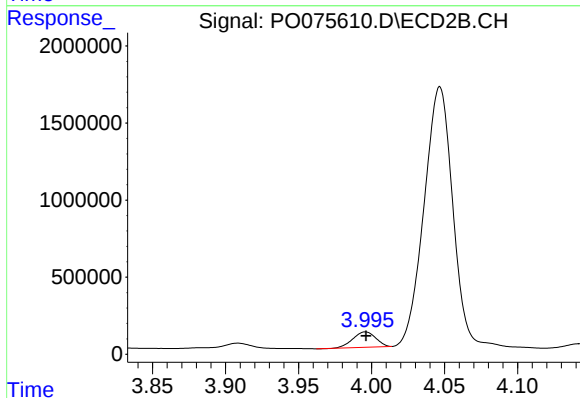


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 1086227
Conc: 22.60 ng/ml

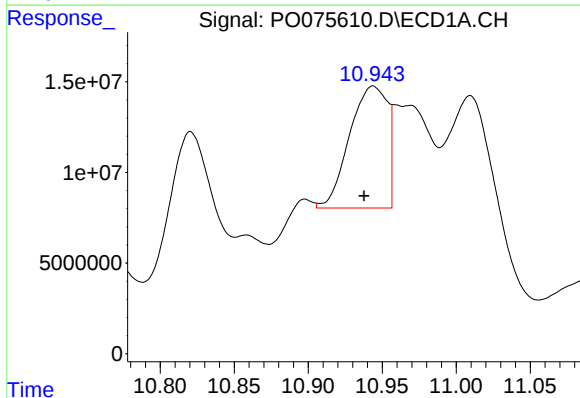

#2 Decachlorobiphenyl

R.T.: 10.943 min
Delta R.T.: 0.006 min
Response: 122267633
Conc: 1267.26 ng/ml m

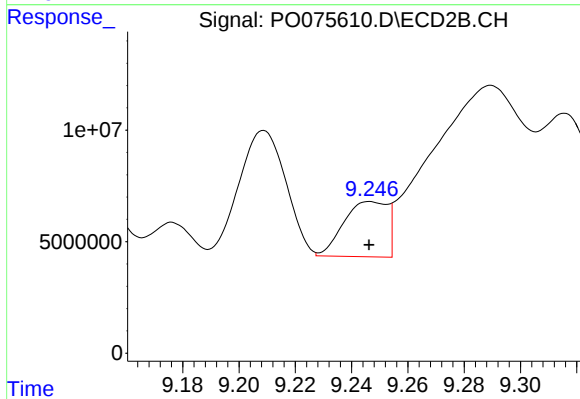

#2 Decachlorobiphenyl

R.T.: 9.246 min
Delta R.T.: 0.000 min
Response: 26692139
Conc: 549.88 ng/ml m