

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020623\
 Data File : P0092380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2023 13:39
 Operator : YP/AJ
 Sample : PB150688BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB150688BL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/07/2023
 Supervised By :mohammad ahmed 02/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 16:28:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.451	3.644	56028395	25146651	19.354	17.909
2) SA Decachlor...	10.388	8.687	46845908	23583696	22.697m	20.891

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020623\
Data File : PO092380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2023 13:39
Operator : YP/AJ
Sample : PB150688BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB150688BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/07/2023
Supervised By :mohammad ahmed 02/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 16:28:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

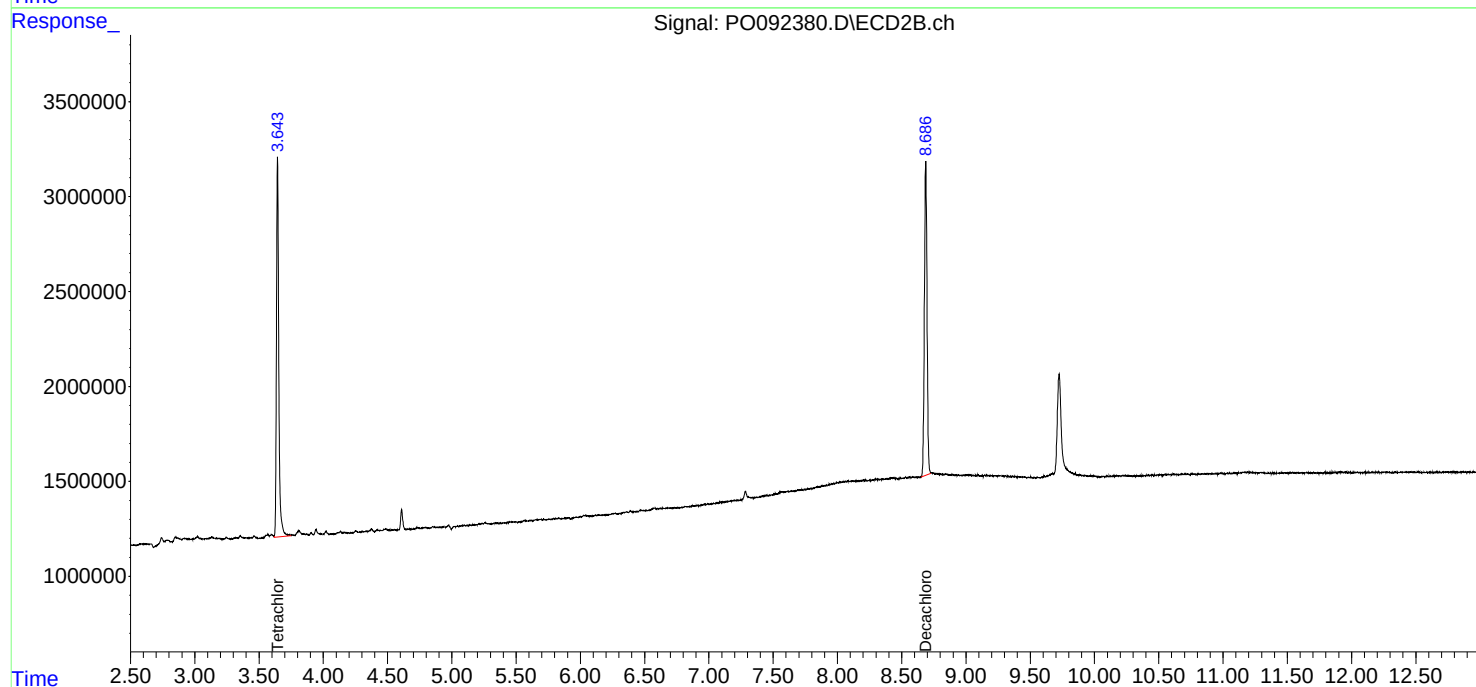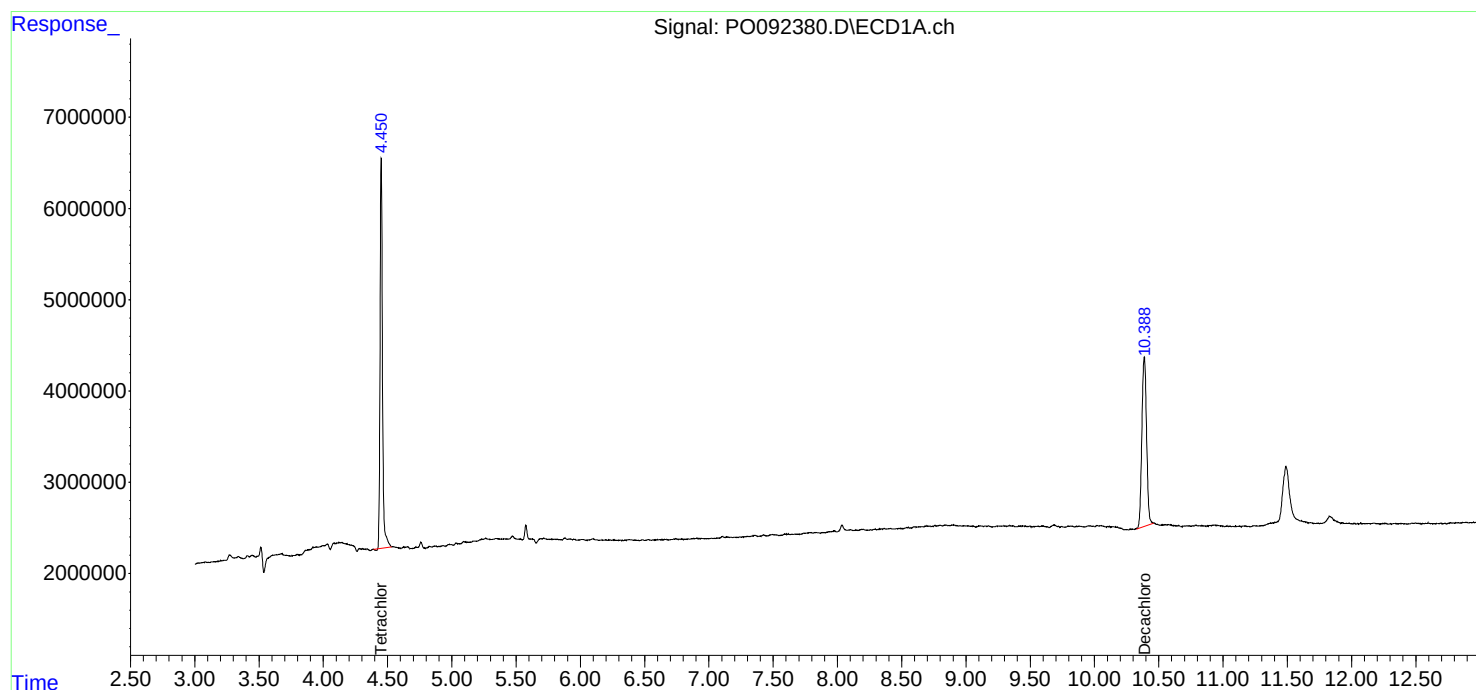

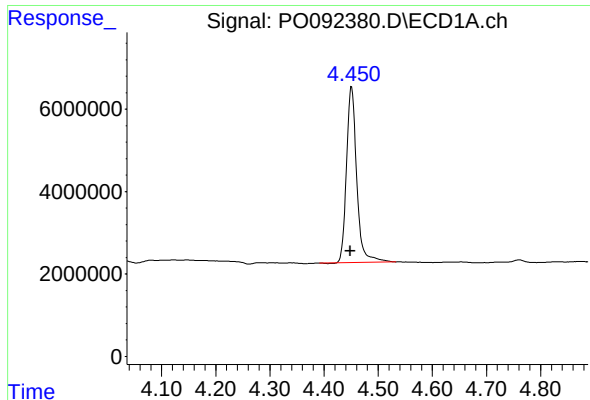

#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: 0.002 min
Response: 56028395
Conc: 19.35 ng/ml

Instrument :


ECD_O

ClientSampleId :

PB150688BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/07/2023
Supervised By :mohammad ahmed 02/07/2023

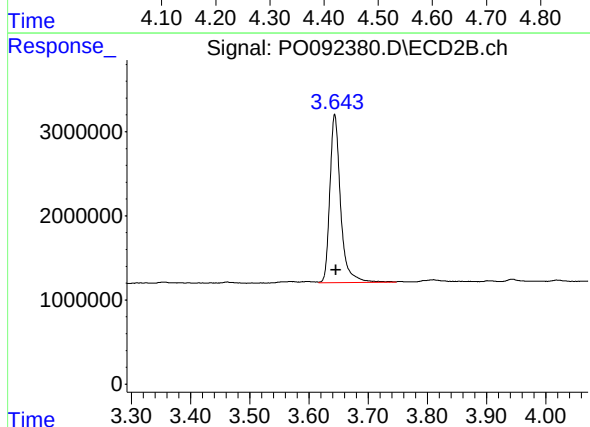


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.002 min
Response: 25146651
Conc: 17.91 ng/ml

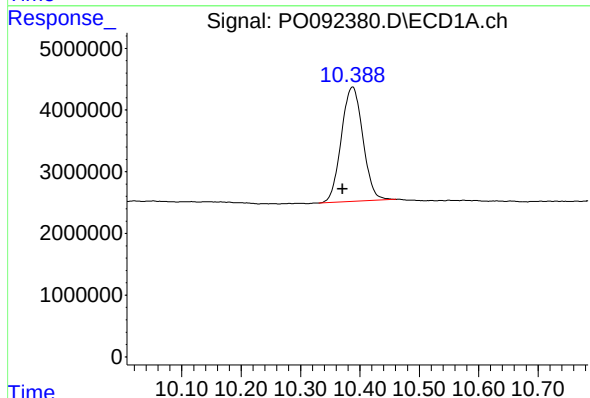

#2 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: 0.016 min
Response: 46845908
Conc: 22.70 ng/ml m

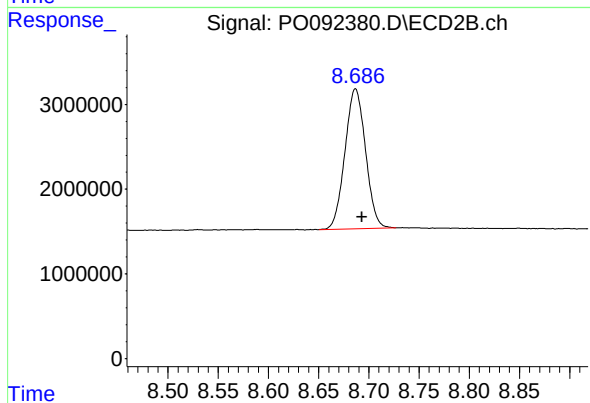

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: -0.006 min
Response: 23583696
Conc: 20.89 ng/ml