

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020922\
 Data File : P0084536.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Feb 2022 13:01
 Operator : YP\AJ
 Sample : N1417-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIT-11-DEWATERING

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/10/2022
 Supervised By :Ankita Jodhani 02/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 16:40:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 09 12:55:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.768	2242557	684130	19.741m	16.377
2) SA Decachlor...	10.446	8.810	1383676	697386	17.275m	18.628

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020922\
Data File : PO084536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Feb 2022 13:01
Operator : YP\AJ
Sample : N1417-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PIT-11-DEWATERING


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/10/2022
Supervised By :Ankita Jodhani 02/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 16:40:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO020822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 09 12:55:28 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

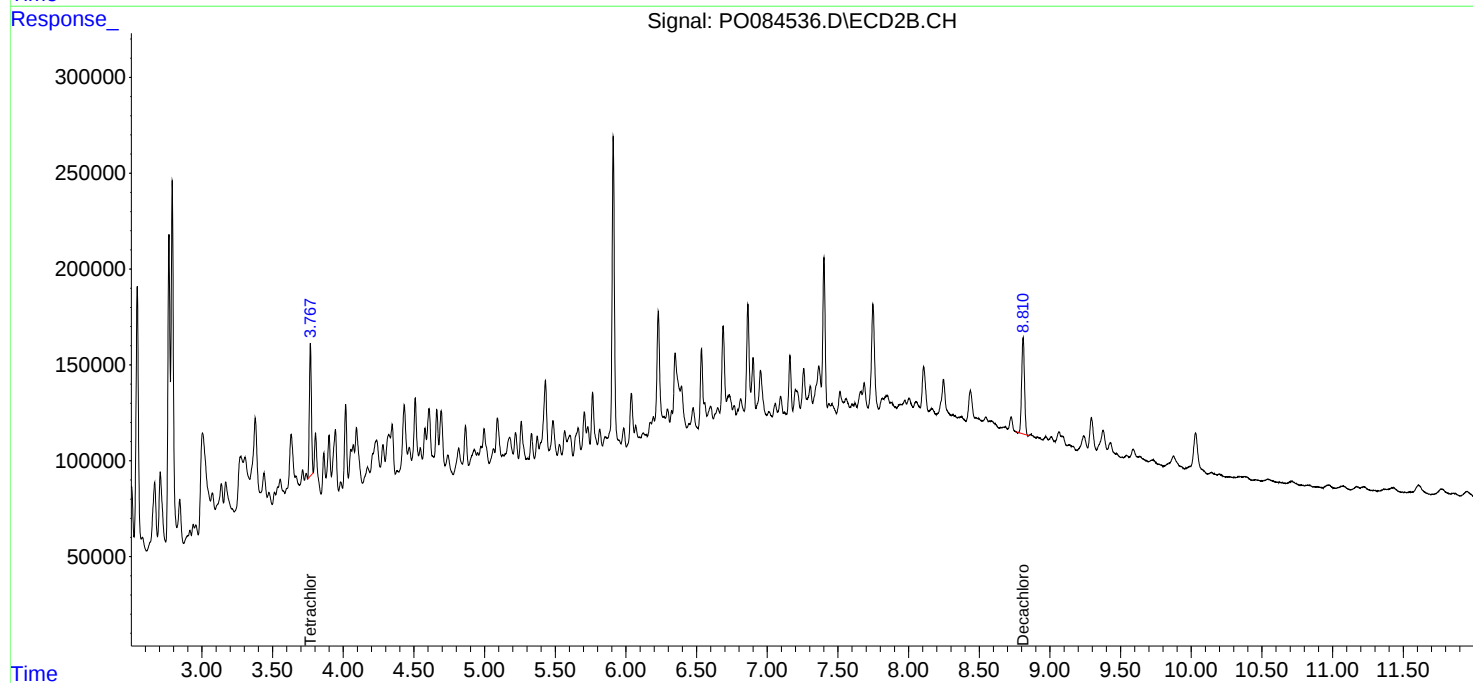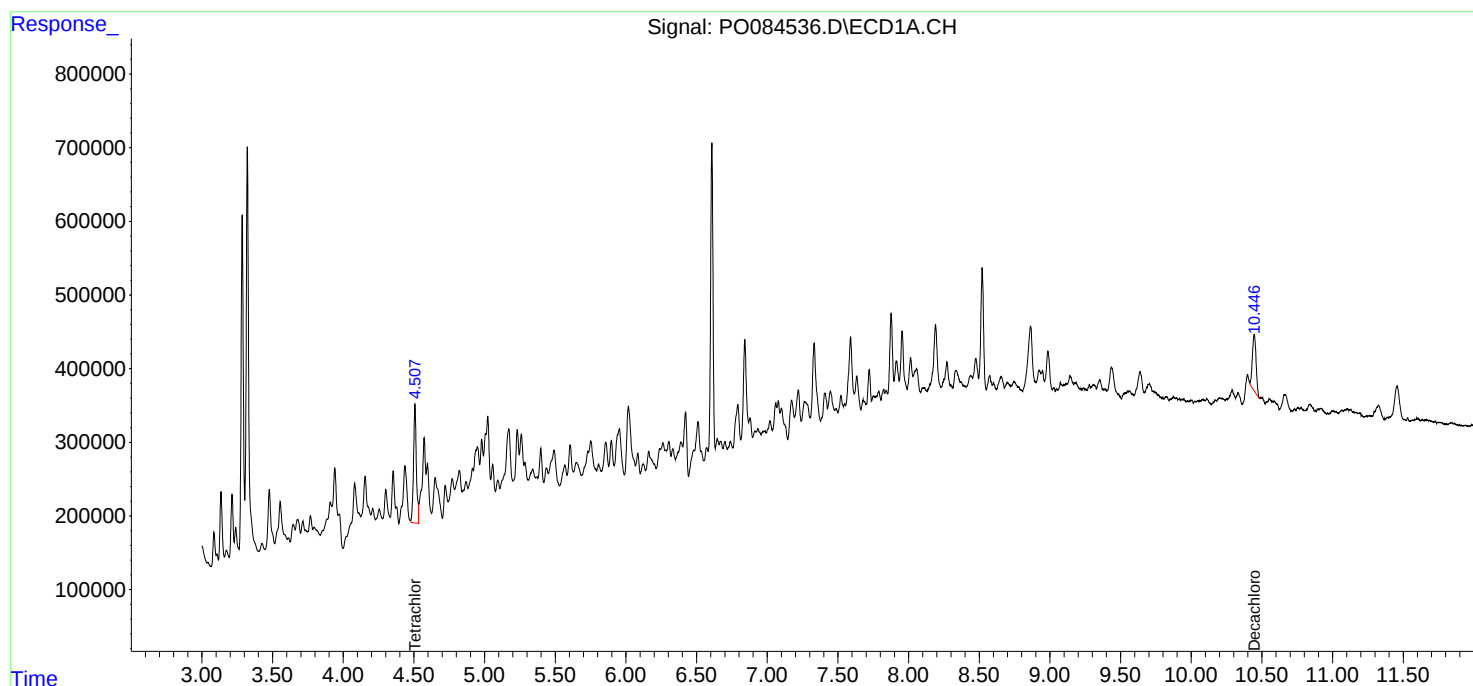

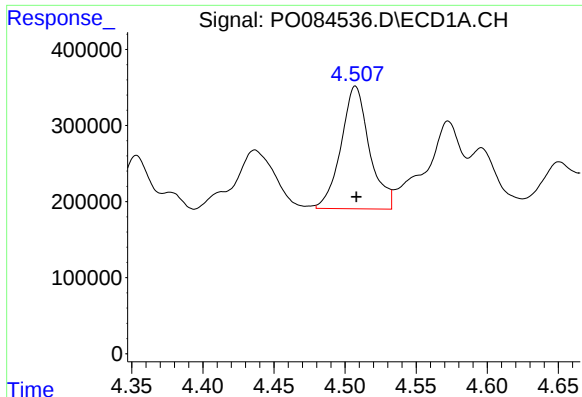


#1 Tetrachloro-m-xylene

R.T.: 4.507 min
Delta R.T.: -0.001 min
Response: 2242557
Conc: 19.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIT-11-DEWATERING


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/10/2022
Supervised By :Ankita Jodhani 02/10/2022

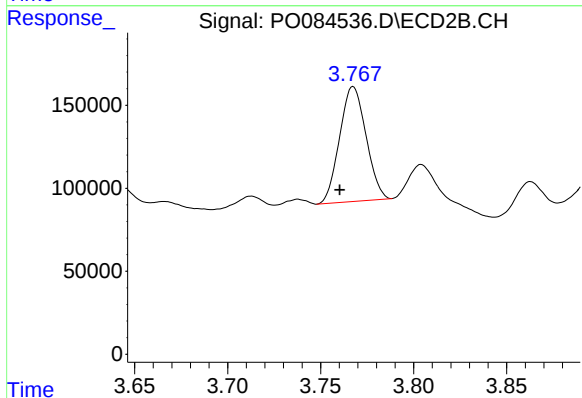


#1 Tetrachloro-m-xylene

R.T.: 3.768 min
Delta R.T.: 0.007 min
Response: 684130
Conc: 16.38 ng/ml

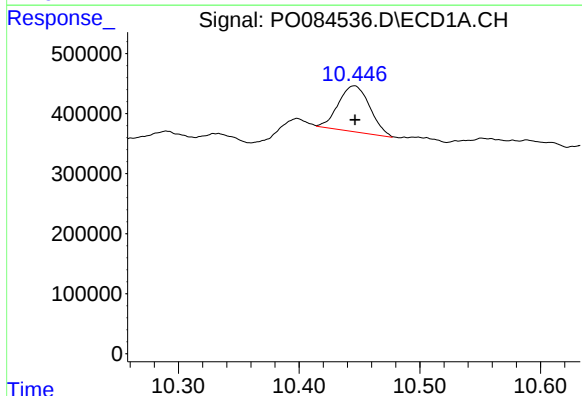

#2 Decachlorobiphenyl

R.T.: 10.446 min
Delta R.T.: 0.000 min
Response: 1383676
Conc: 17.28 ng/ml m

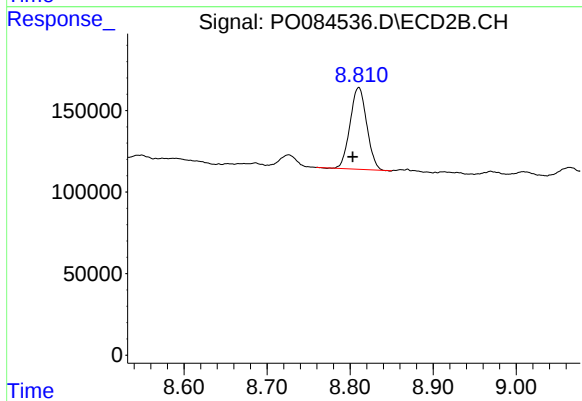

#2 Decachlorobiphenyl

R.T.: 8.810 min
Delta R.T.: 0.007 min
Response: 697386
Conc: 18.63 ng/ml