

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020922\
Data File : P0084562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Feb 2022 20:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 07:35:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 10 07:10:18 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.775	2345865	862241	20.631	18.767
2) SA Decachlor...	10.446	8.819	1683272	779278	21.015	20.808

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020922\
Data File : P0084562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Feb 2022 20:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 07:35:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 10 07:10:18 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

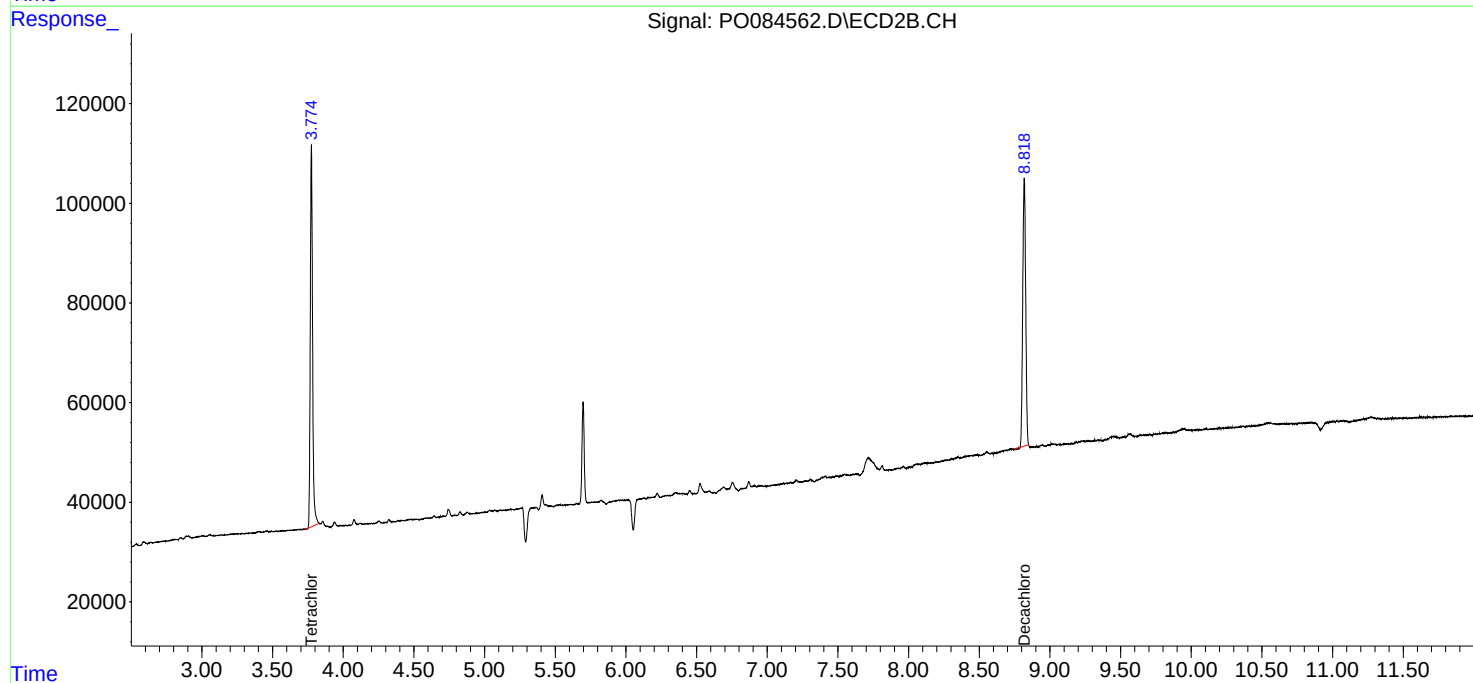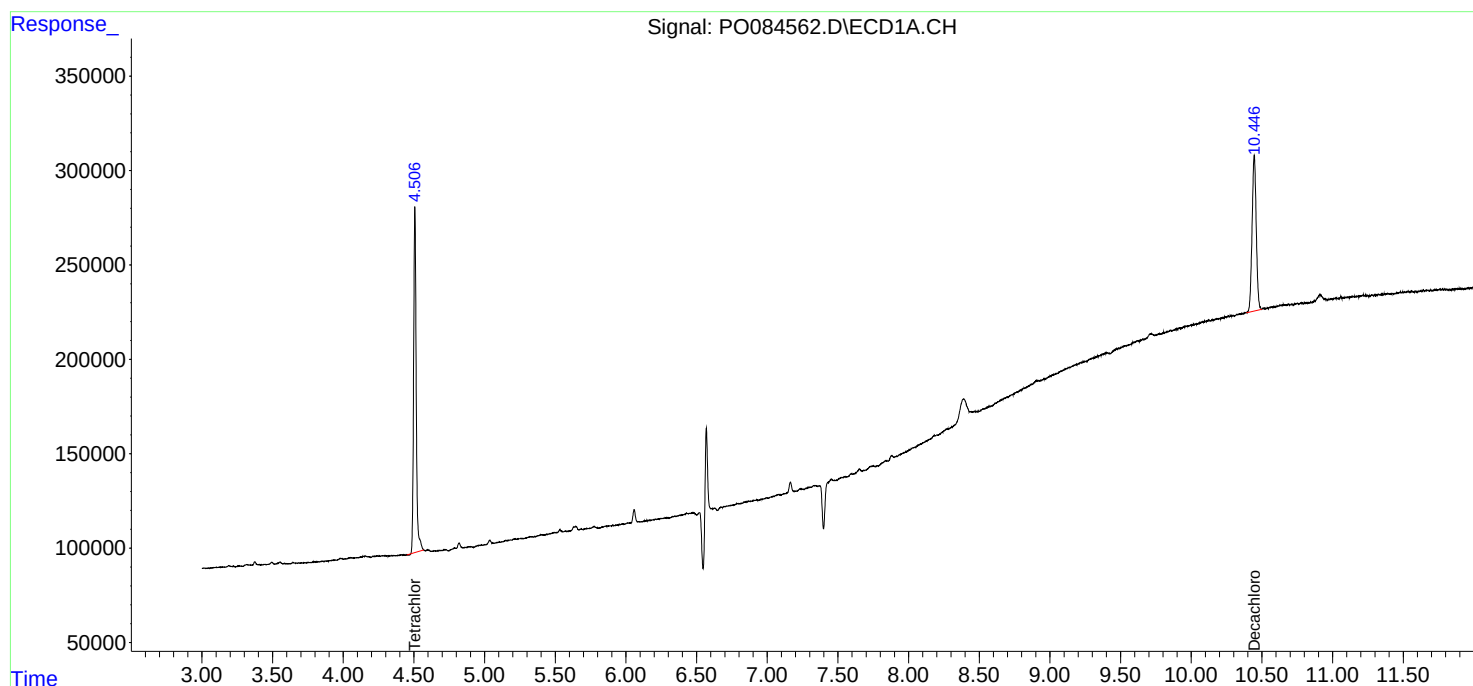


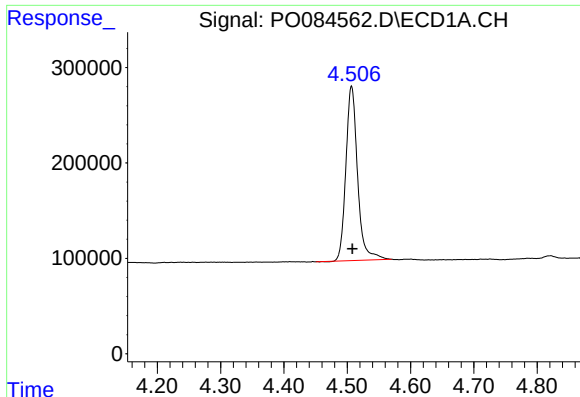

#1 Tetrachloro-m-xylene


R.T.: 4.507 min
Delta R.T.: -0.001 min
Response: 2345865
Conc: 20.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

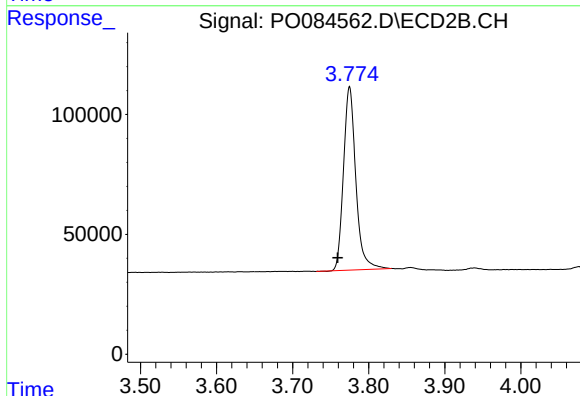


#1 Tetrachloro-m-xylene

R.T.: 3.775 min
Delta R.T.: 0.015 min
Response: 862241
Conc: 18.77 ng/ml

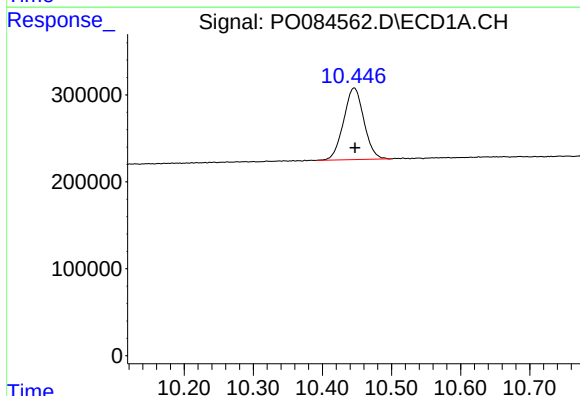

#2 Decachlorobiphenyl

R.T.: 10.446 min
Delta R.T.: -0.001 min
Response: 1683272
Conc: 21.02 ng/ml

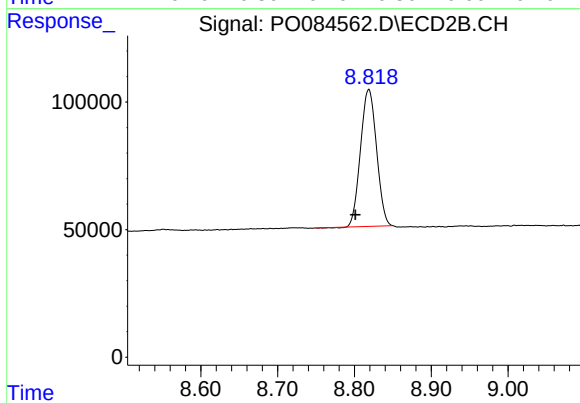

#2 Decachlorobiphenyl

R.T.: 8.819 min
Delta R.T.: 0.017 min
Response: 779278
Conc: 20.81 ng/ml