

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020923\
 Data File : P0092439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2023 13:33
 Operator : YP/AJ
 Sample : 01490-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2023-1A

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
 Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 21:32:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.445	3.643	4157342	2131871	1.436m	1.518
2) SA Decachlor...	10.366	8.680	6359049	1606458	3.081	1.423m#
Target Compounds						
26) L6 AR-1254-1	6.504	5.534	5351380	2916188	48.335	37.201
27) L6 AR-1254-2	6.729	5.682	9083010	3867983	55.877	55.903
28) L6 AR-1254-3	7.101	6.087	7472272	4016461	45.306	37.630
29) L6 AR-1254-4	7.393	6.317	5518339	2283006	50.449	38.764
30) L6 AR-1254-5	7.823	6.738	6625194	3727724	47.088	40.957

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020923\
Data File : PO092439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2023 13:33
Operator : YP/AJ
Sample : 01490-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CLI-2023-1A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 21:32:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

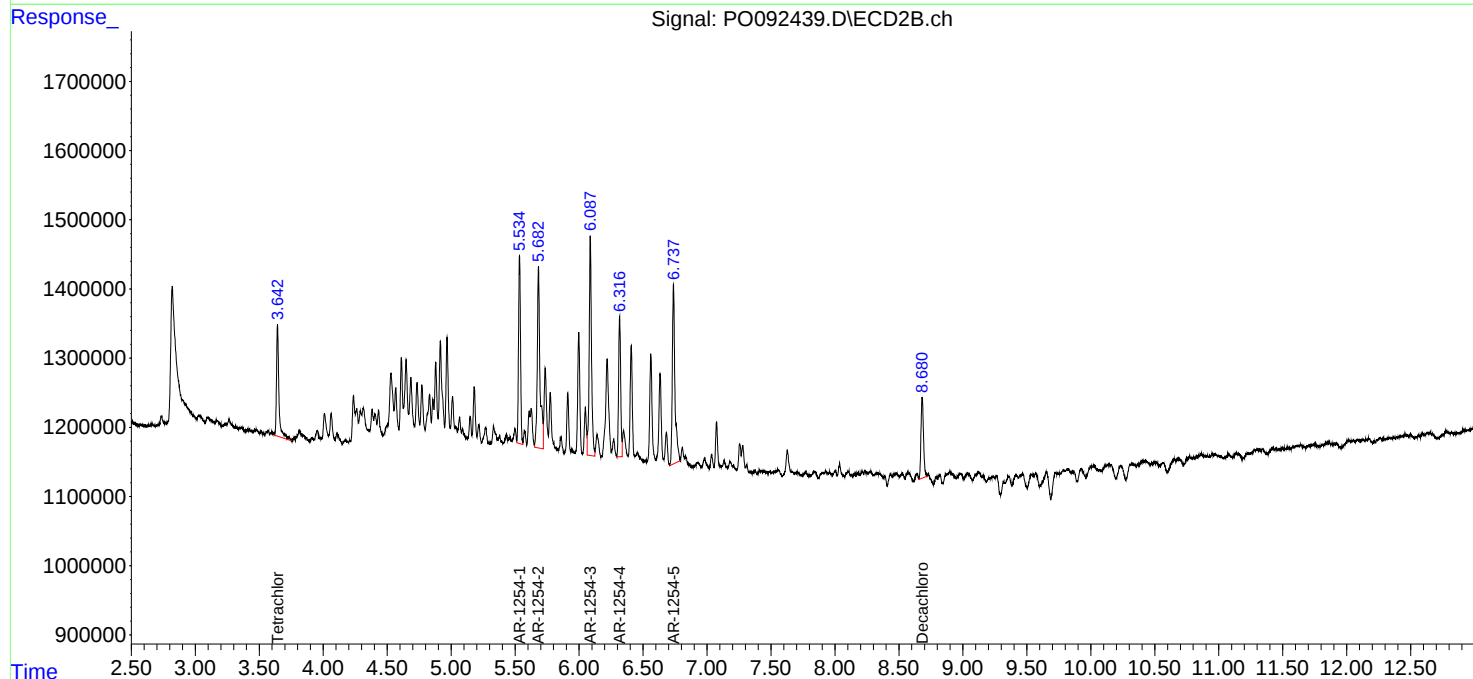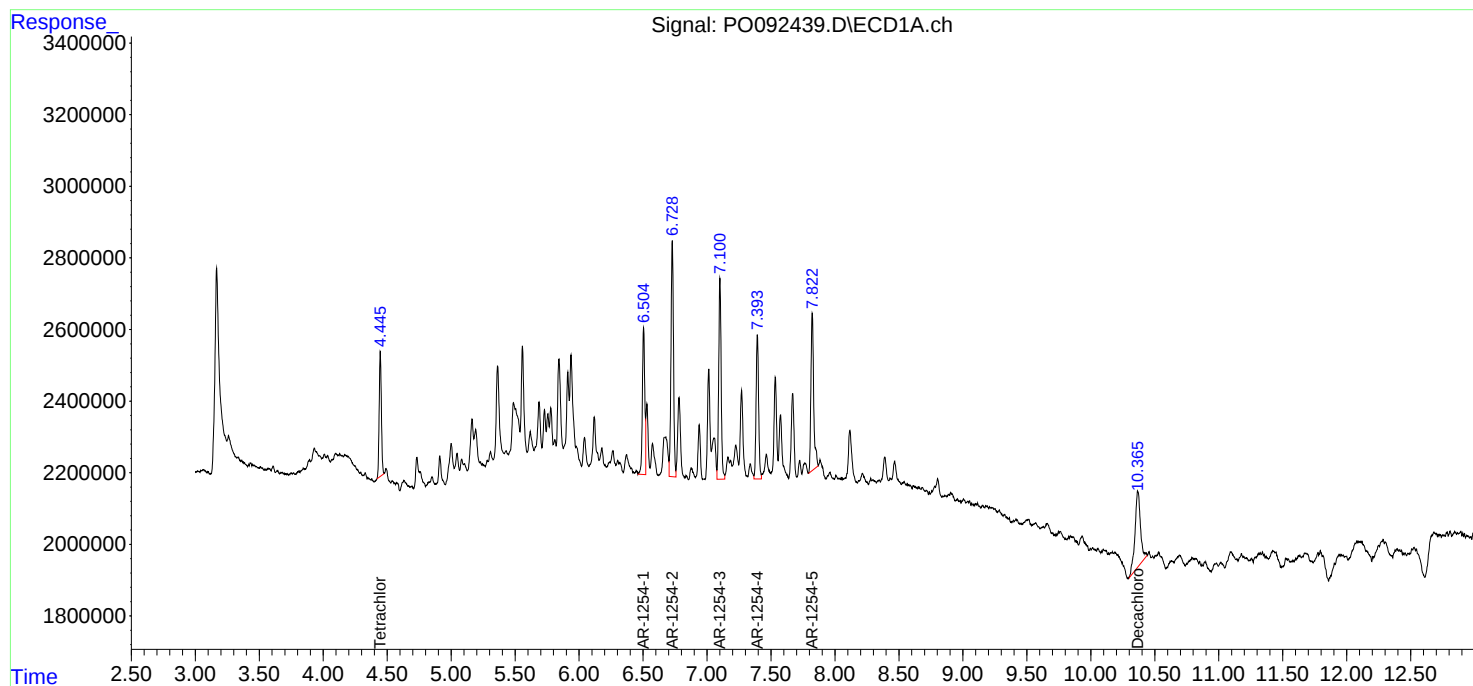

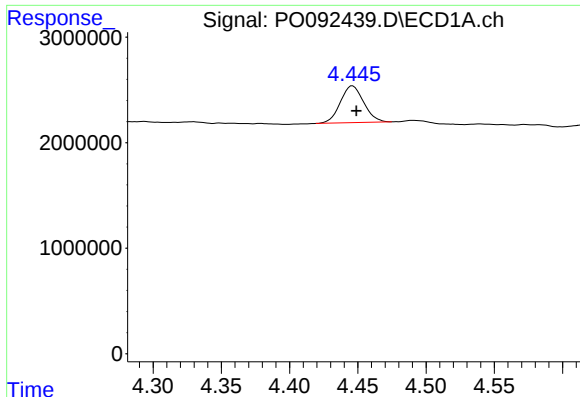


#1 Tetrachloro-m-xylene

R.T.: 4.445 min
Delta R.T.: -0.004 min
Response: 4157342
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2023-1A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

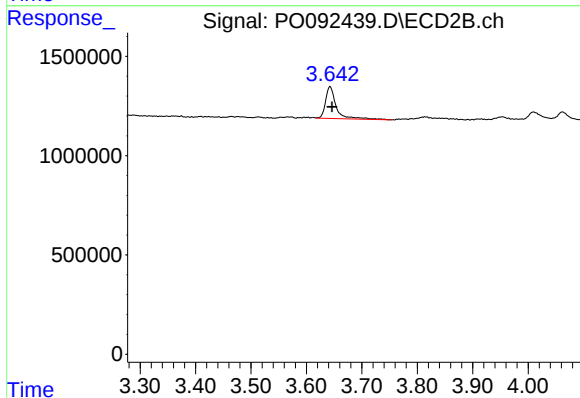


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.003 min
Response: 2131871
Conc: 1.52 ng/ml

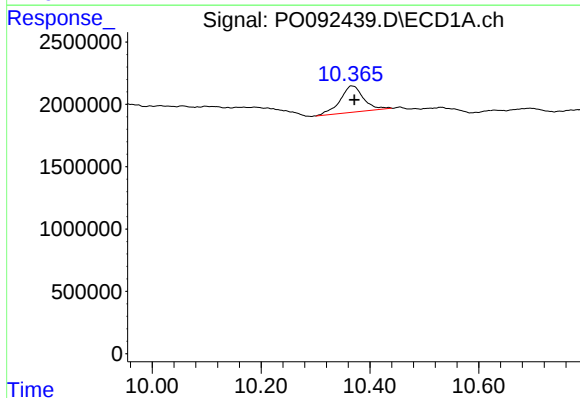


#2 Decachlorobiphenyl

R.T.: 10.366 min
Delta R.T.: -0.005 min
Response: 6359049
Conc: 3.08 ng/ml

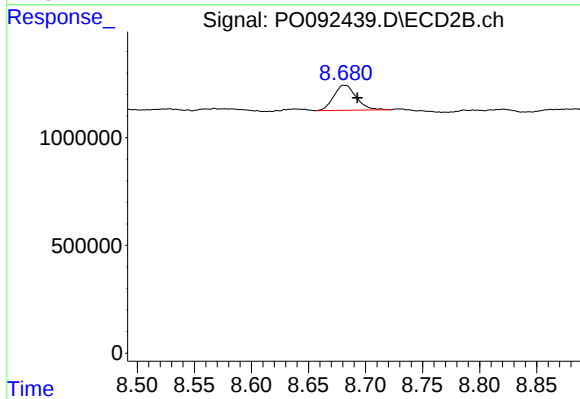

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.013 min
Response: 1606458
Conc: 1.42 ng/ml m

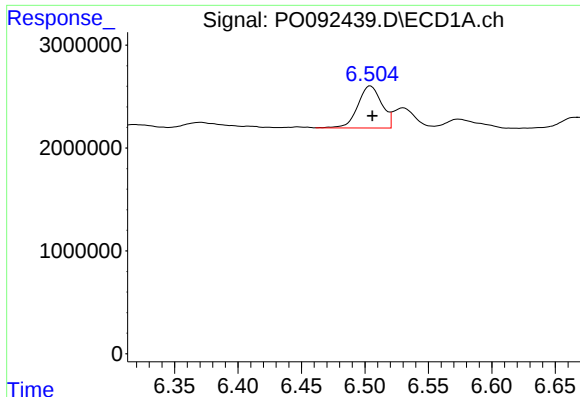


#26 AR-1254-1

R.T.: 6.504 min
Delta R.T.: -0.002 min
Response: 5351380
Conc: 48.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2023-1A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

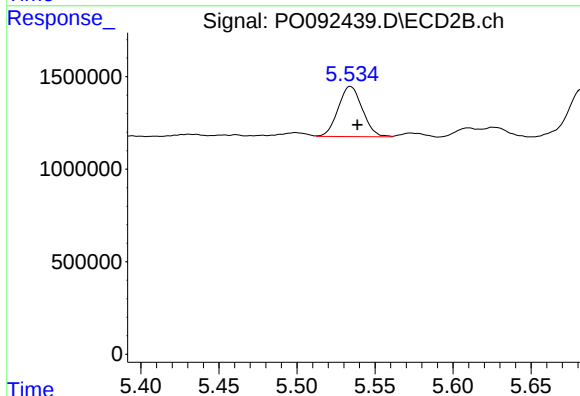


#26 AR-1254-1

R.T.: 5.534 min
Delta R.T.: -0.005 min
Response: 2916188
Conc: 37.20 ng/ml

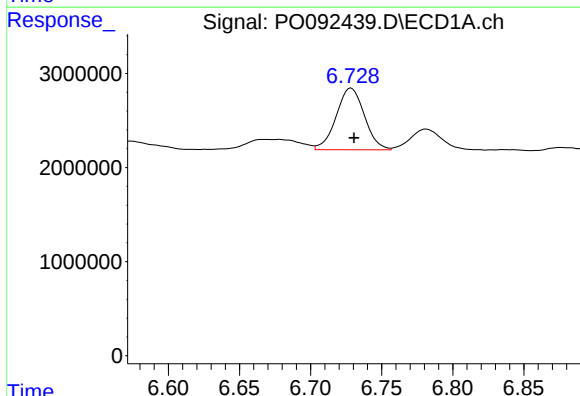


#27 AR-1254-2

R.T.: 6.729 min
Delta R.T.: -0.002 min
Response: 9083010
Conc: 55.88 ng/ml

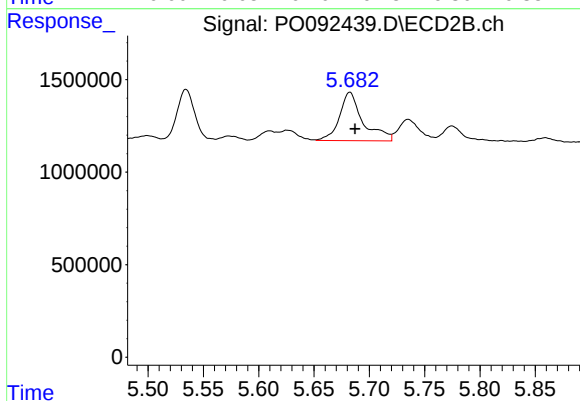

#27 AR-1254-2

R.T.: 5.682 min
Delta R.T.: -0.005 min
Response: 3867983
Conc: 55.90 ng/ml

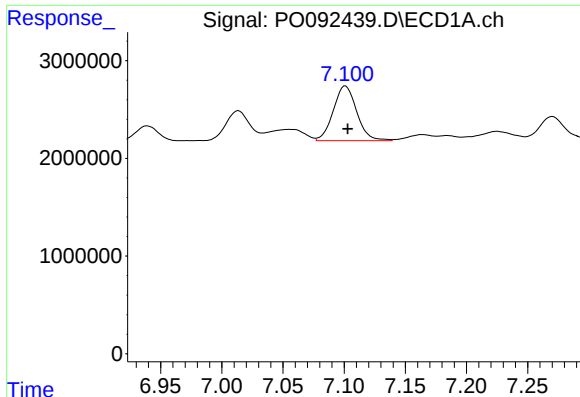


#28 AR-1254-3

R.T.: 7.101 min
Delta R.T.: -0.002 min
Response: 7472272
Conc: 45.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2023-1A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

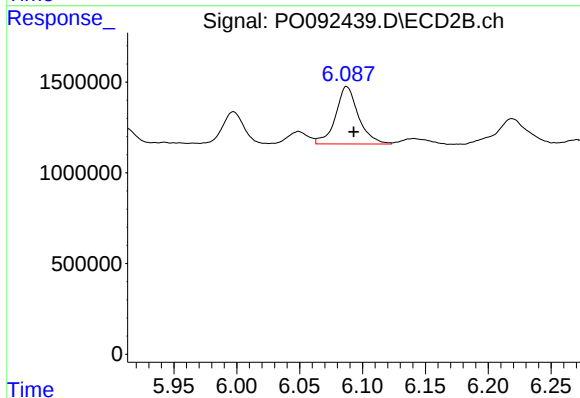


#28 AR-1254-3

R.T.: 6.087 min
Delta R.T.: -0.006 min
Response: 4016461
Conc: 37.63 ng/ml

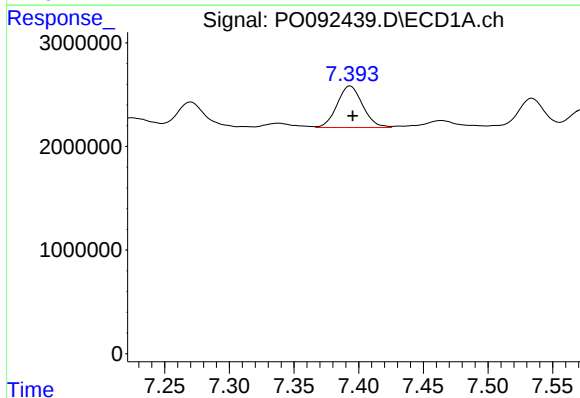


#29 AR-1254-4

R.T.: 7.393 min
Delta R.T.: -0.002 min
Response: 5518339
Conc: 50.45 ng/ml

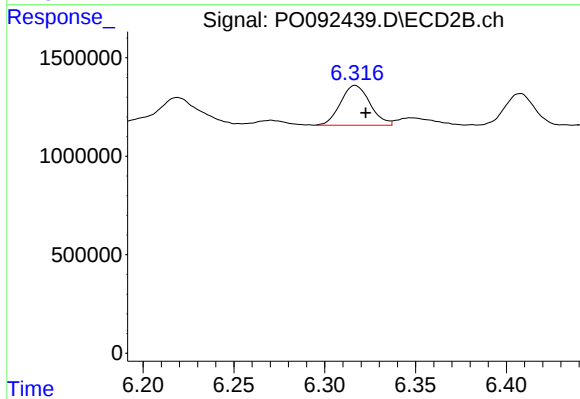

#29 AR-1254-4

R.T.: 6.317 min
Delta R.T.: -0.006 min
Response: 2283006
Conc: 38.76 ng/ml

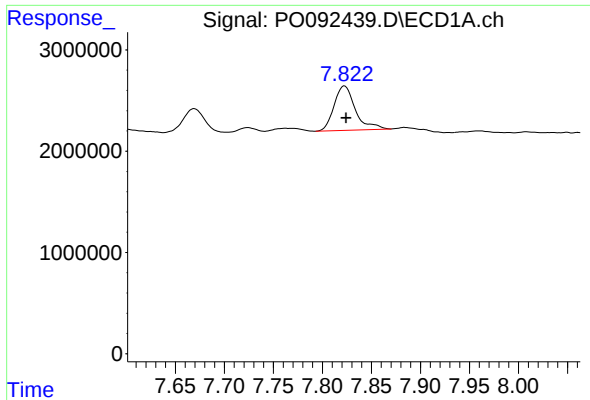


#30 AR-1254-5

R.T.: 7.823 min
Delta R.T.: -0.002 min
Response: 6625194
Conc: 47.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2023-1A

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

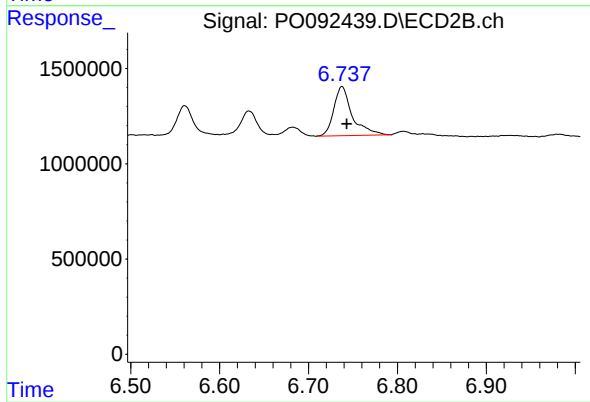

#30 AR-1254-5

R.T.: 6.738 min
Delta R.T.: -0.005 min
Response: 3727724
Conc: 40.96 ng/ml