

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020923\
 Data File : P0092453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2023 17:48
 Operator : YP/AJ
 Sample : 01502-04 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA652M-2-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
 Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 21:52:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.642	4438436	1635758	1.533	1.165m
2) SA Decachlor...	10.372	8.683	4757513	1806886	2.305	1.601m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020923\
Data File : PO092453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2023 17:48
Operator : YP/AJ
Sample : 01502-04 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA652M-2-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 21:52:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

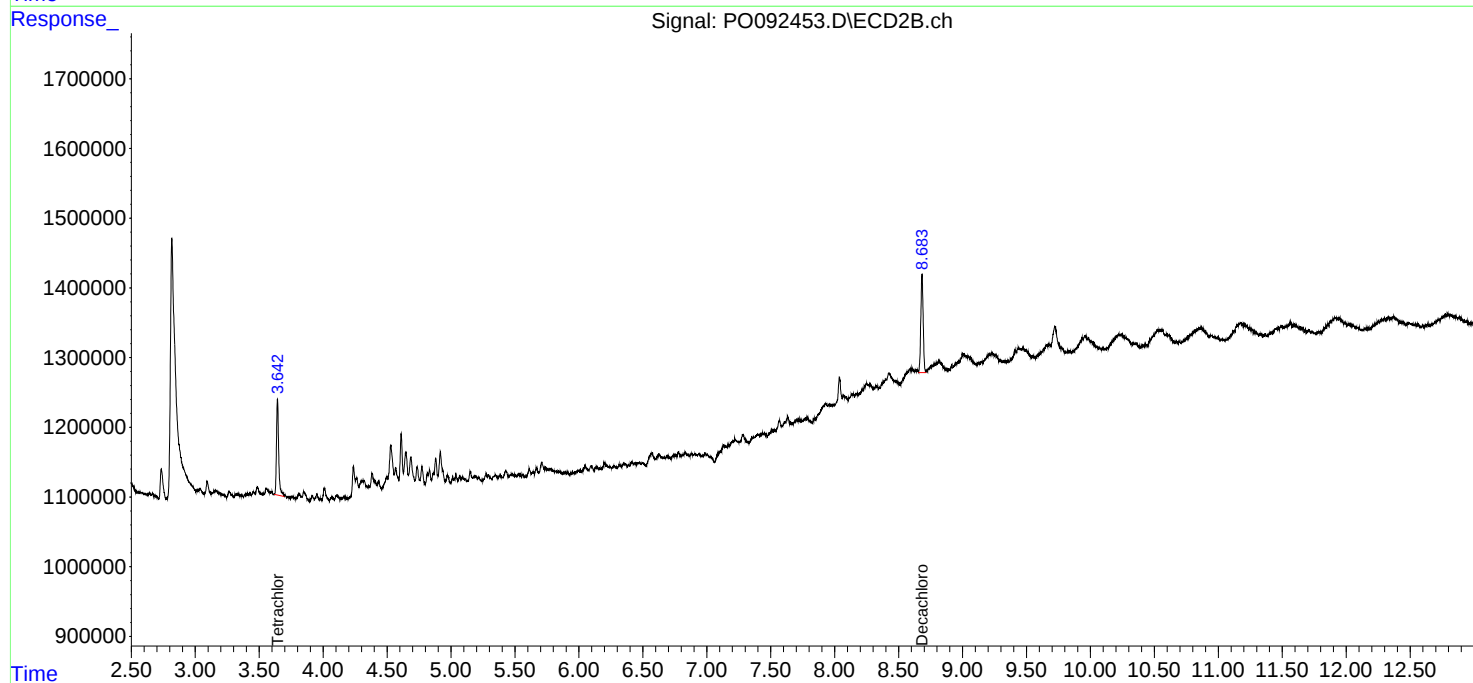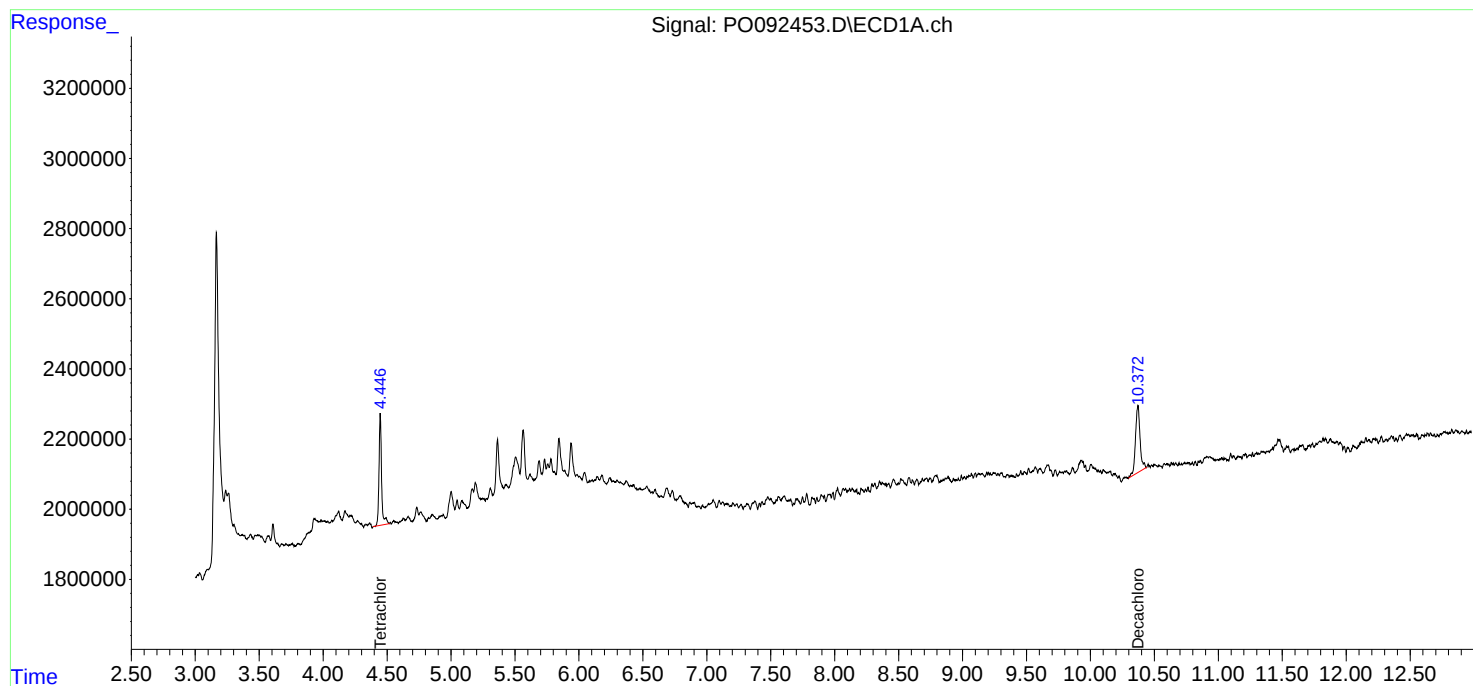

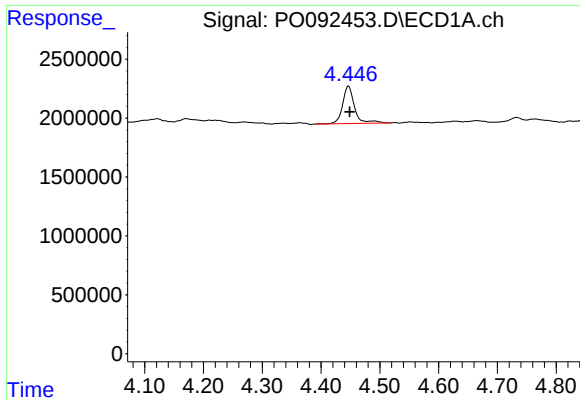


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: -0.002 min
Response: 4438436
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA652M-2-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

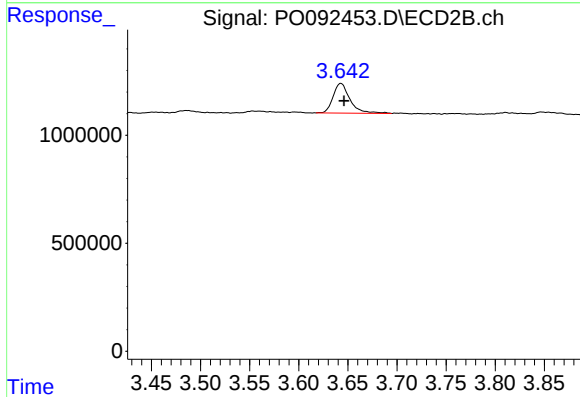


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.004 min
Response: 1635758
Conc: 1.16 ng/ml m

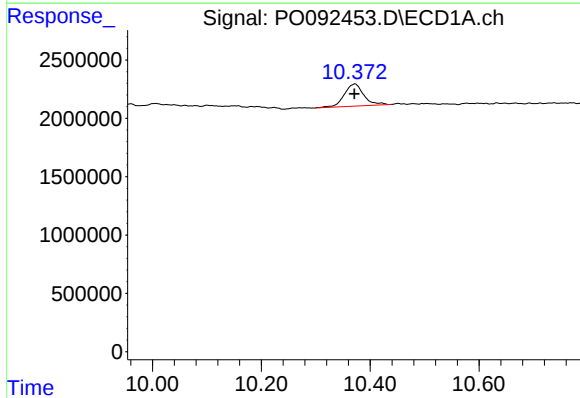

#2 Decachlorobiphenyl

R.T.: 10.372 min
Delta R.T.: 0.000 min
Response: 4757513
Conc: 2.31 ng/ml

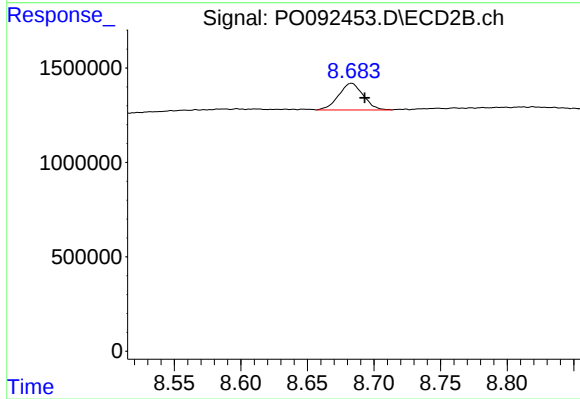

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.010 min
Response: 1806886
Conc: 1.60 ng/ml m