

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020923\
 Data File : P0092457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2023 18:56
 Operator : YP/AJ
 Sample : 01502-08 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEH655I-1-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
 Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 21:55:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.642	3359045	1699456	1.160m	1.210
2) SA Decachlor...	10.371	8.683	4479991	1919664	2.171	1.700

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020923\
Data File : PO092457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2023 18:56
Operator : YP/AJ
Sample : 01502-08 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEH655I-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 21:55:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

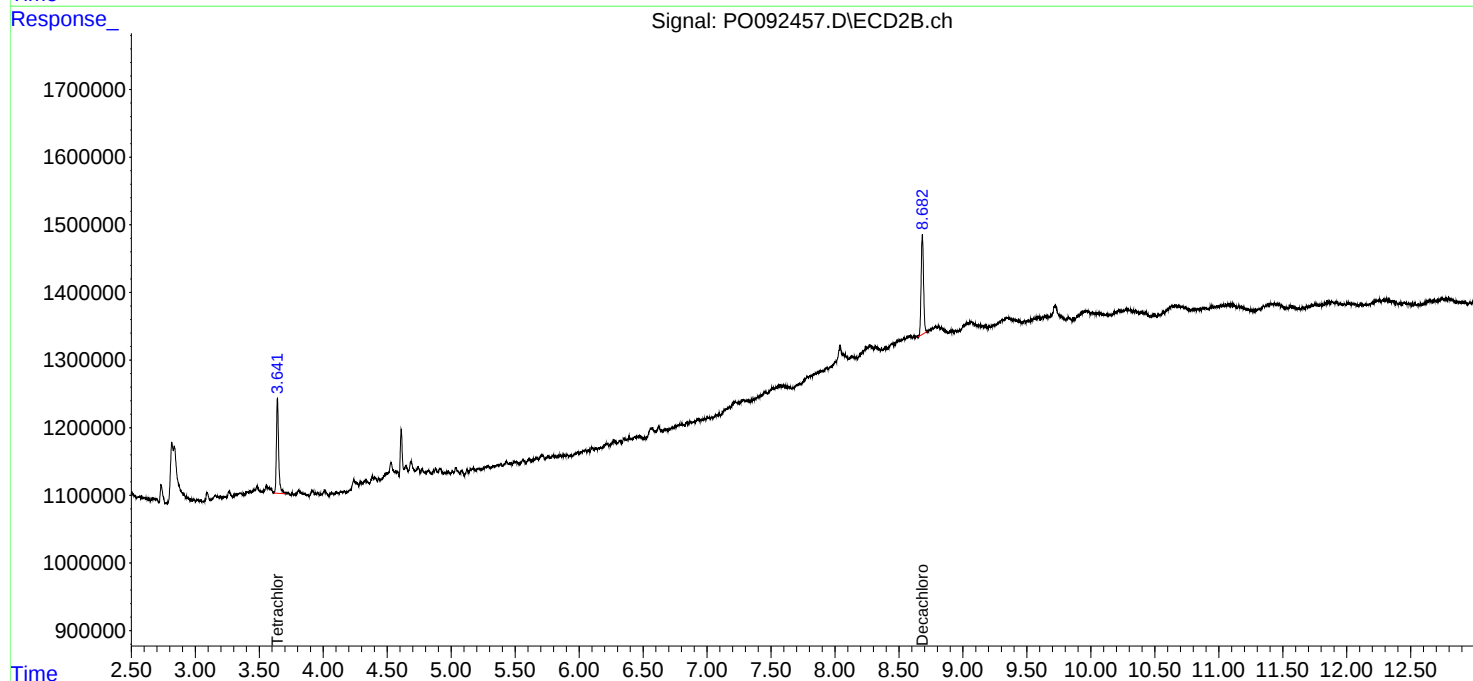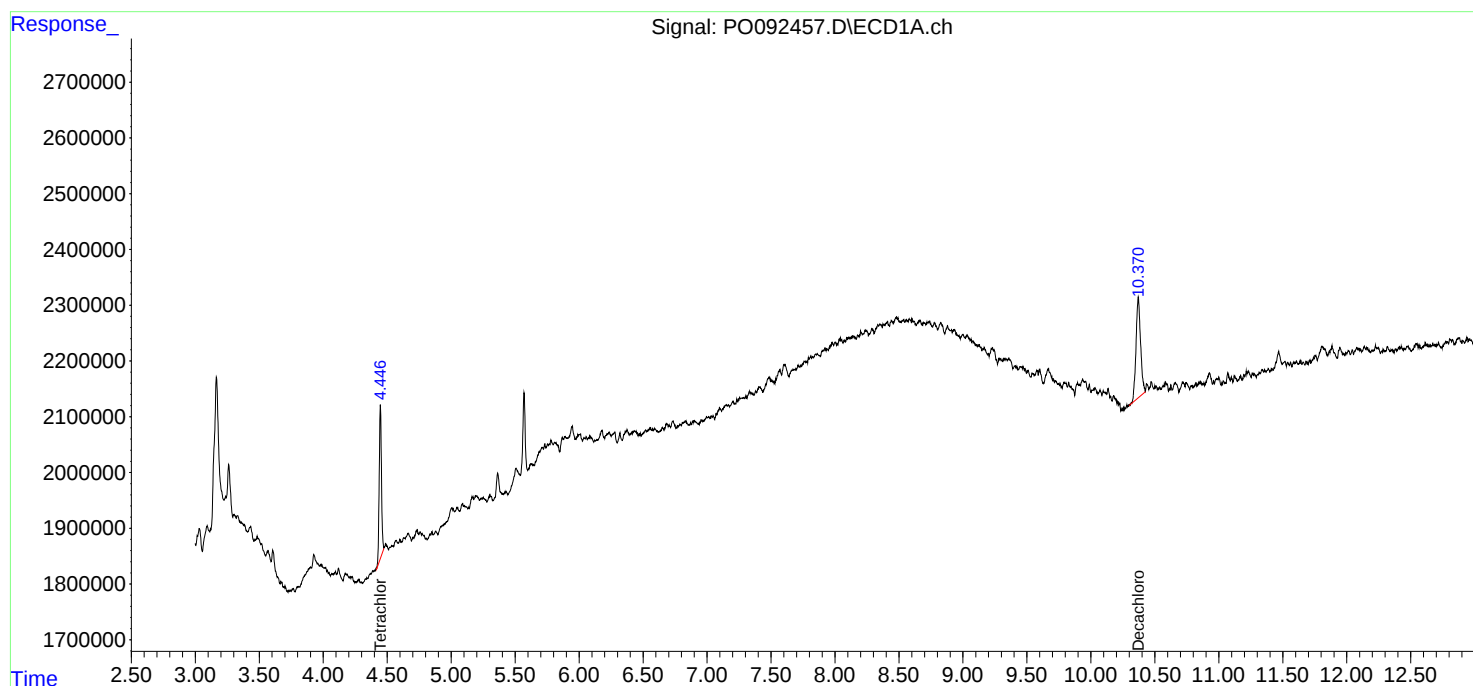

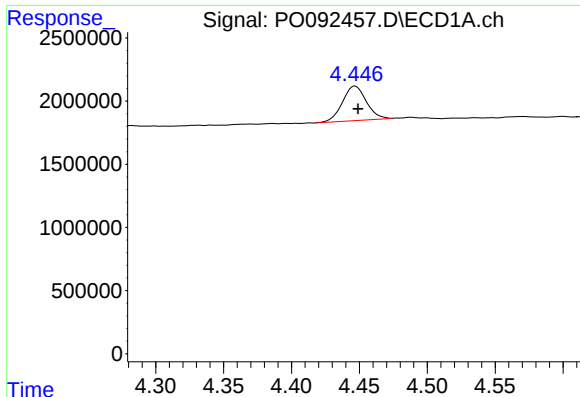


#1 Tetrachloro-m-xylene

R.T.: 4.446 min
Delta R.T.: -0.003 min
Response: 3359045
Conc: 1.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
JEH655I-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/10/2023
Supervised By :Sohil Jodhani 02/10/2023

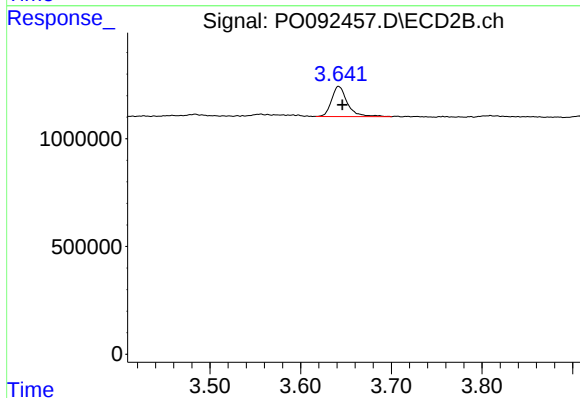


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.004 min
Response: 1699456
Conc: 1.21 ng/ml

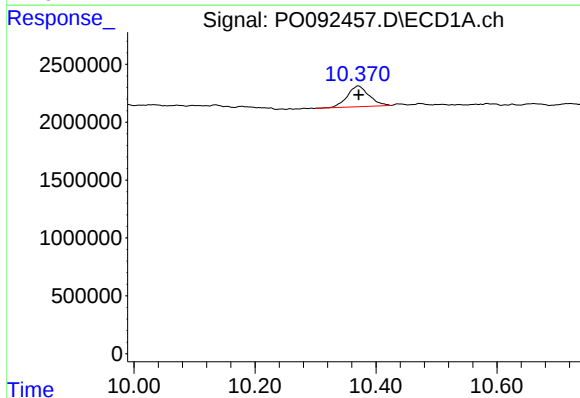

#2 Decachlorobiphenyl

R.T.: 10.371 min
Delta R.T.: 0.000 min
Response: 4479991
Conc: 2.17 ng/ml

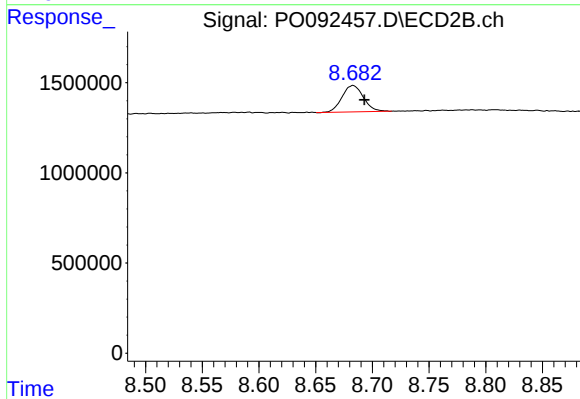

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.010 min
Response: 1919664
Conc: 1.70 ng/ml