

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021022\
 Data File : P0084574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Feb 2022 13:19
 Operator : YP\AJ
 Sample : N1449-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220042-AMENDED-NACOTE-2-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 05:43:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 10 07:10:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.780	2088662	787041	18.369	17.130
2) SA Decachlor...	10.449	8.824	808426	380408	10.093	10.157

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021022\
Data File : P0084574.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Feb 2022 13:19
Operator : YP\AJ
Sample : N1449-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220042-AMENDED-NACOTE-2-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 05:43:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 10 07:10:18 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

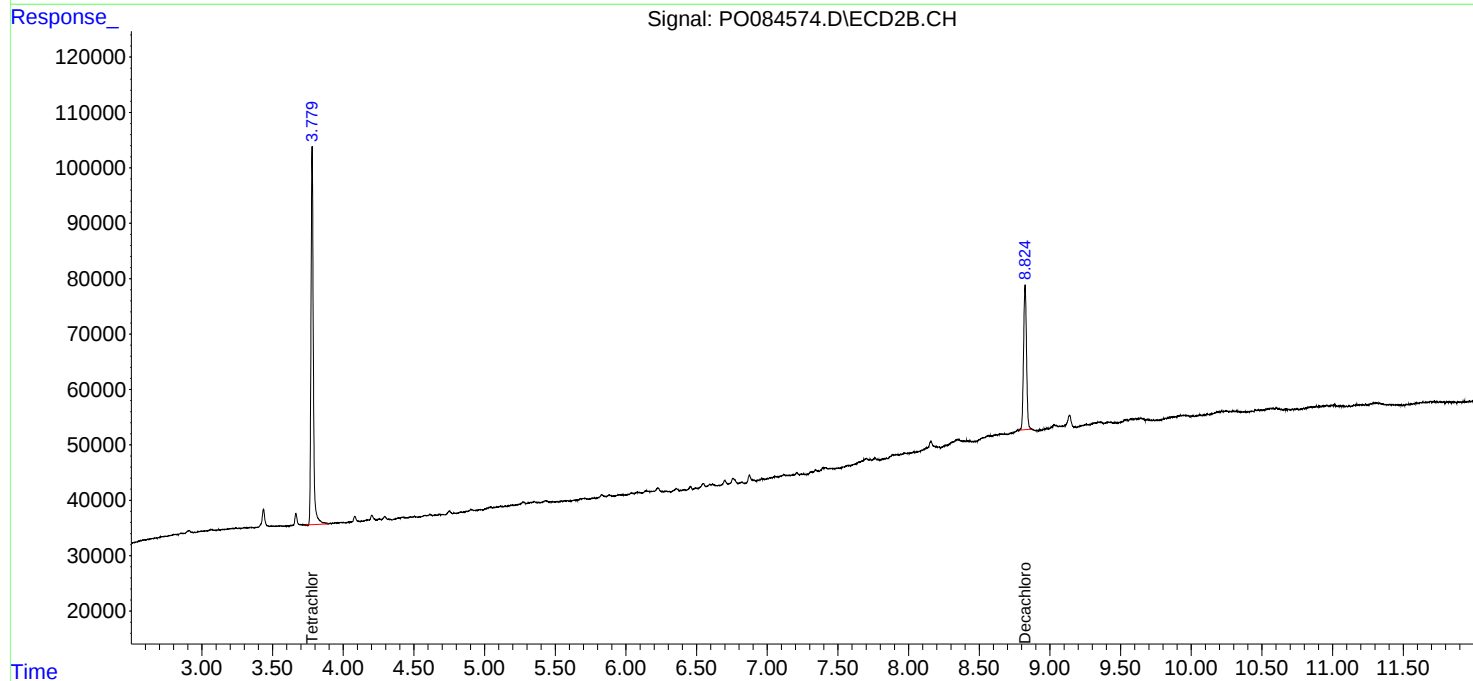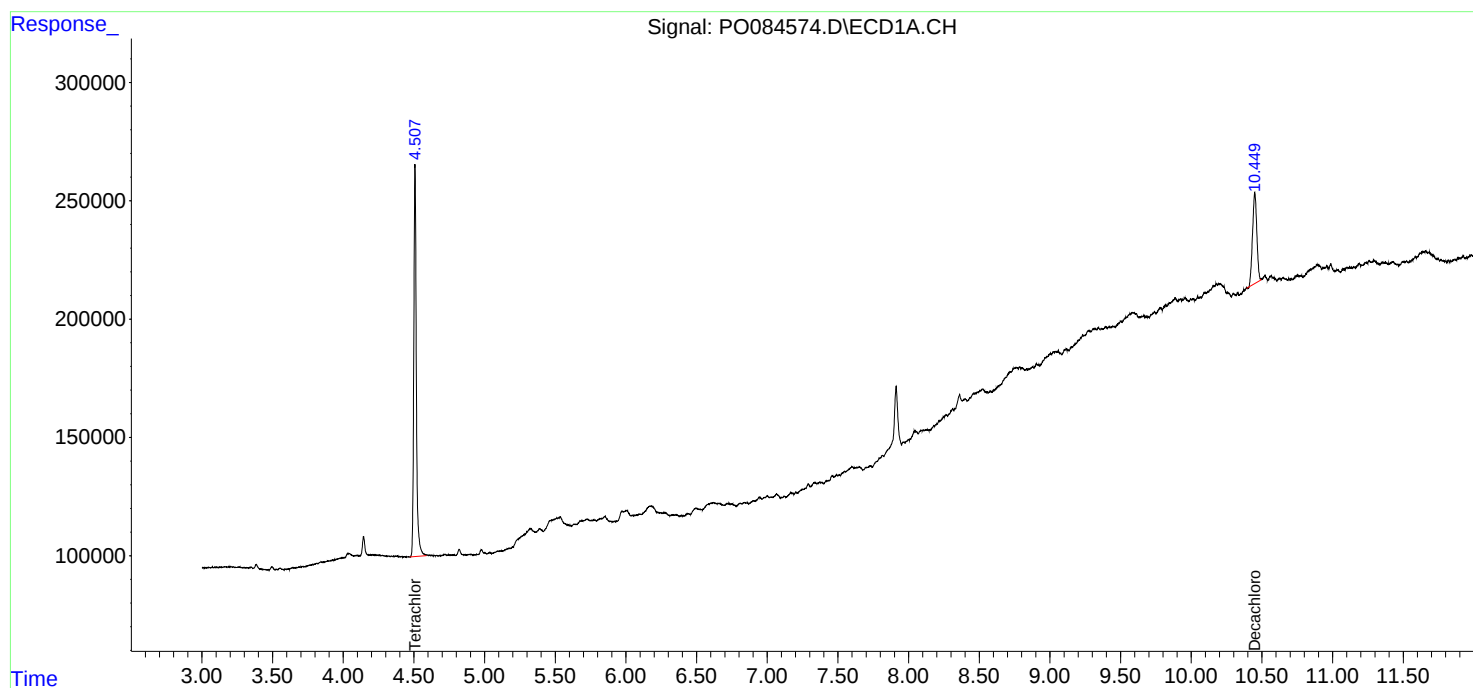

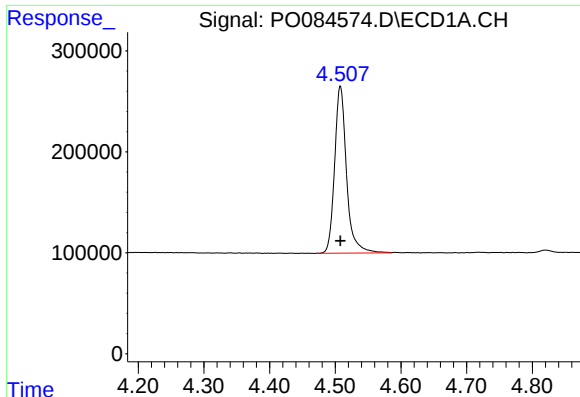

#1 Tetrachloro-m-xylene


R.T.: 4.508 min
Delta R.T.: 0.000 min
Response: 2088662
Conc: 18.37 ng/ml

Instrument :

ECD_O


ClientSampleId :

20220042-AMENDED-NACOTE-2-COMP

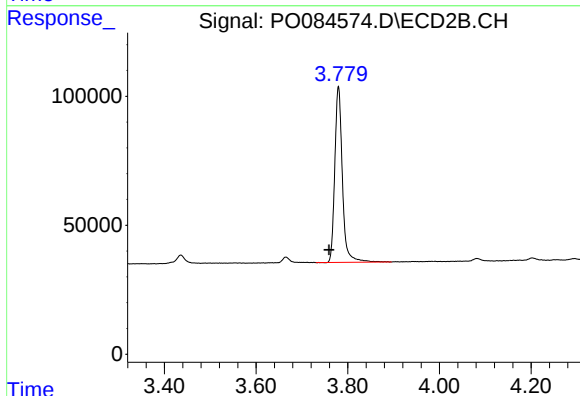


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: 0.020 min
Response: 787041
Conc: 17.13 ng/ml

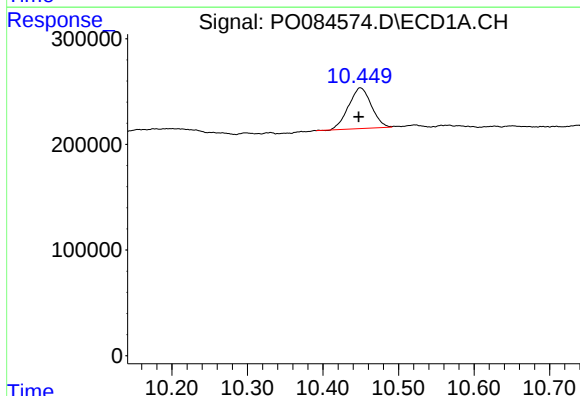

#2 Decachlorobiphenyl

R.T.: 10.449 min
Delta R.T.: 0.002 min
Response: 808426
Conc: 10.09 ng/ml

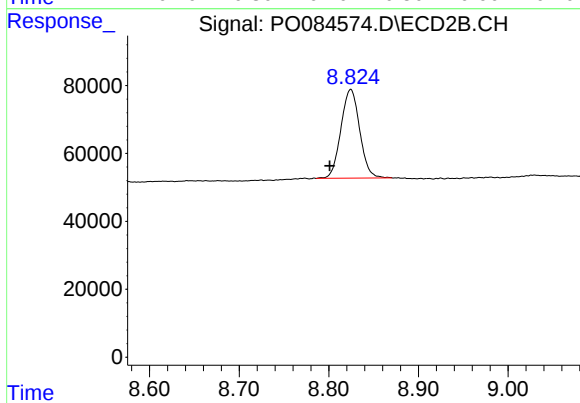

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.023 min
Response: 380408
Conc: 10.16 ng/ml