

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0021022\
 Data File : P0084599.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Feb 2022 20:28
 Operator : YP\AJ
 Sample : N1460-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 PIPE-AUD-1257

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/11/2022
 Supervised By :Ankita Jodhani 02/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 05:53:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0020822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 10 07:10:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.784	2140335	756835	18.824	16.473
2) SA Decachlor...	10.448	8.827	1418706	652323	17.712	17.418
Target Compounds						
26) L6 AR-1254-1	6.571	5.680	97244	29876	22.016m	10.872m#
27) L6 AR-1254-2	6.793	5.828	79425	25530	12.020	10.650m
28) L6 AR-1254-3	7.165	6.230	130854	53110	19.278	14.263m#
29) L6 AR-1254-4	7.454	6.458	77232	31140	16.391m	13.687m
30) L6 AR-1254-5	7.880	6.877	170926	84939	32.200	26.040m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021022\
Data File : P0084599.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Feb 2022 20:28
Operator : YP\AJ
Sample : N1460-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PIPE-AUD-1257


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/11/2022
Supervised By :Ankita Jodhani 02/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 05:53:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 10 07:10:18 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

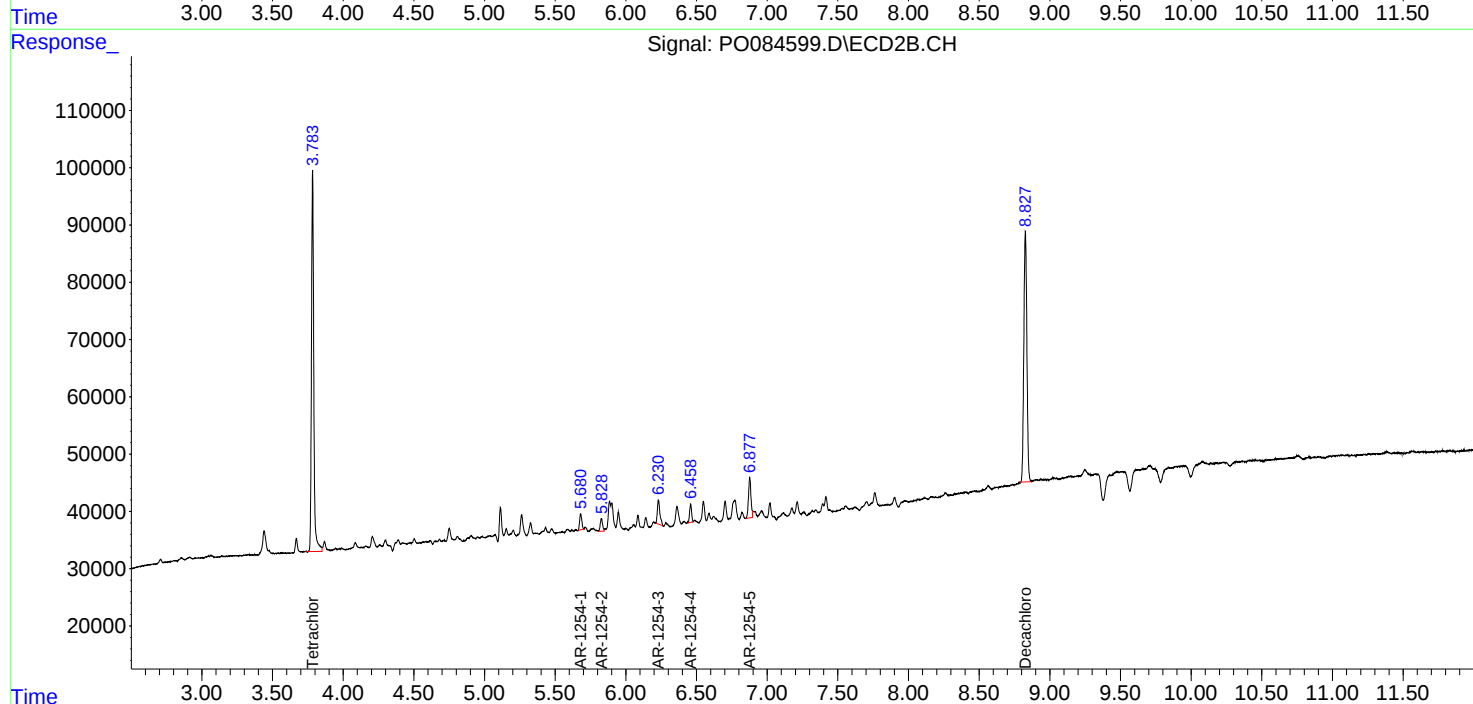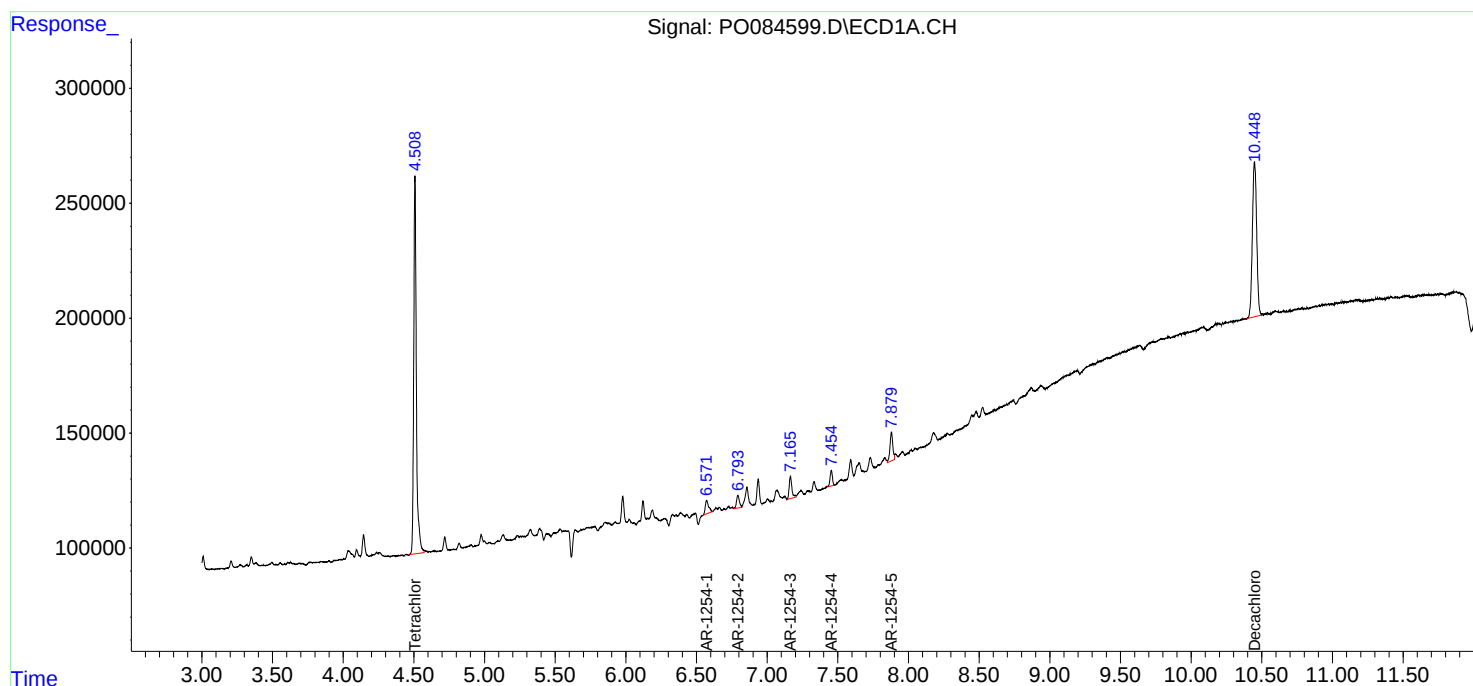

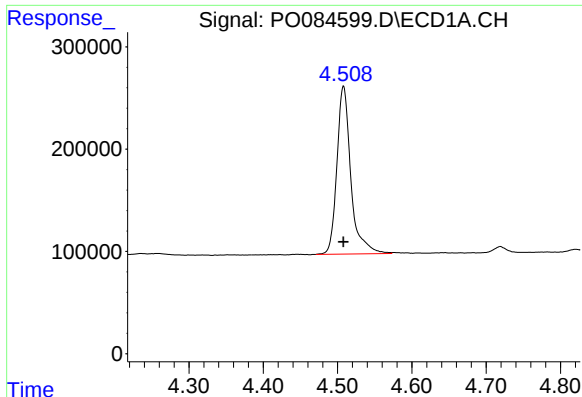


#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: 0.000 min
Response: 2140335
Conc: 18.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-AUD-1257


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/11/2022
Supervised By :Ankita Jodhani 02/11/2022

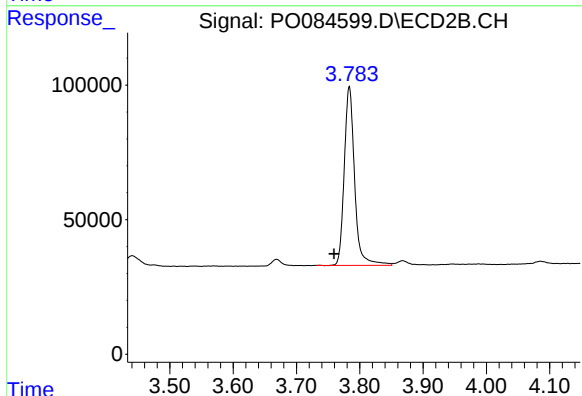


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: 0.024 min
Response: 756835
Conc: 16.47 ng/ml

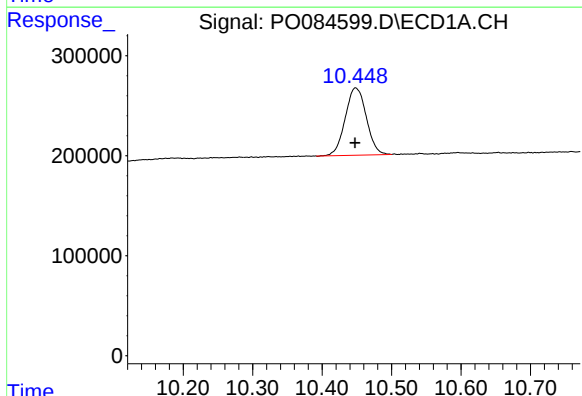


#2 Decachlorobiphenyl

R.T.: 10.448 min
Delta R.T.: 0.000 min
Response: 1418706
Conc: 17.71 ng/ml

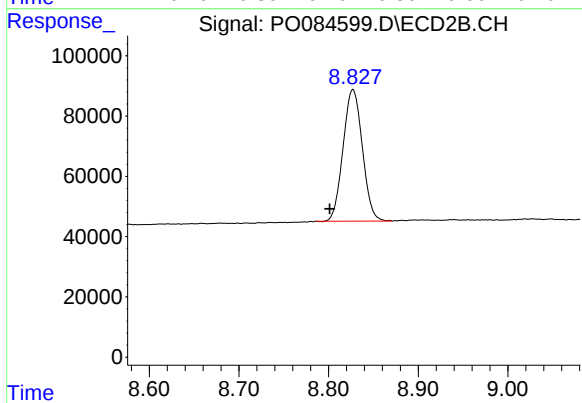

#2 Decachlorobiphenyl

R.T.: 8.827 min
Delta R.T.: 0.026 min
Response: 652323
Conc: 17.42 ng/ml

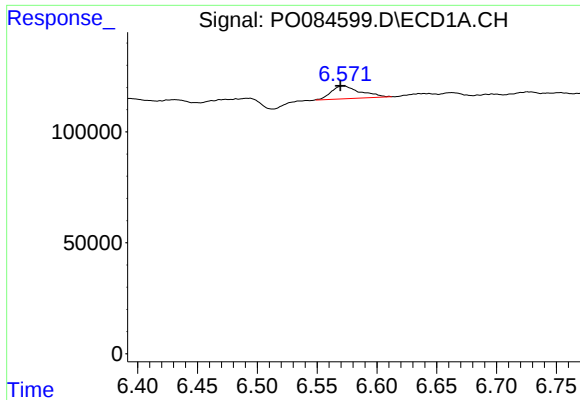


#26 AR-1254-1

R.T.: 6.571 min
Delta R.T.: 0.002 min
Response: 97244
Conc: 22.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-AUD-1257


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/11/2022
Supervised By :Ankita Jodhani 02/11/2022

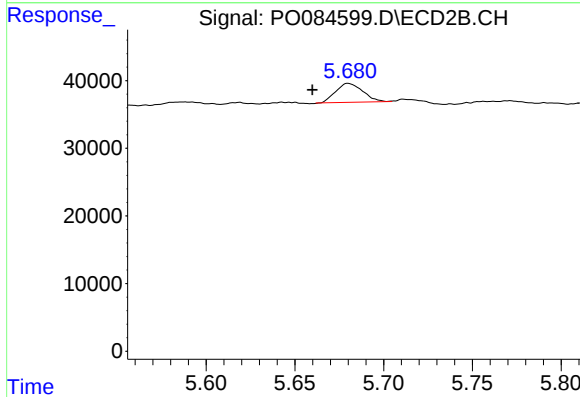


#26 AR-1254-1

R.T.: 5.680 min
Delta R.T.: 0.020 min
Response: 29876
Conc: 10.87 ng/ml m

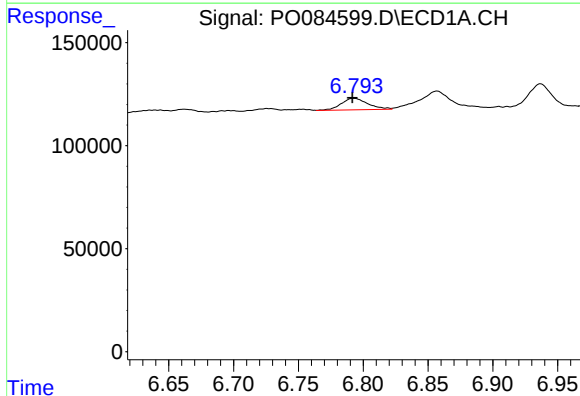


#27 AR-1254-2

R.T.: 6.793 min
Delta R.T.: 0.001 min
Response: 79425
Conc: 12.02 ng/ml

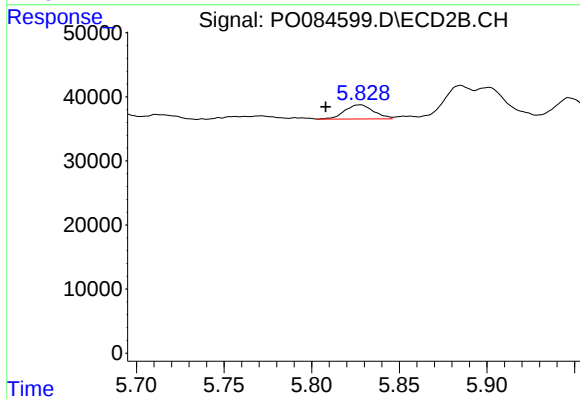

#27 AR-1254-2

R.T.: 5.828 min
Delta R.T.: 0.020 min
Response: 25530
Conc: 10.65 ng/ml m

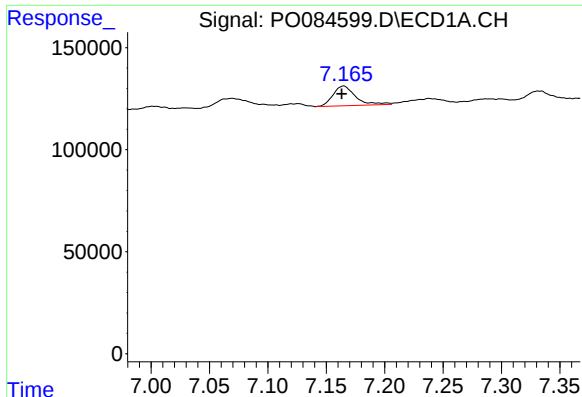


#28 AR-1254-3

R.T.: 7.165 min
Delta R.T.: 0.002 min
Response: 130854
Conc: 19.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-AUD-1257


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/11/2022
Supervised By :Ankita Jodhani 02/11/2022

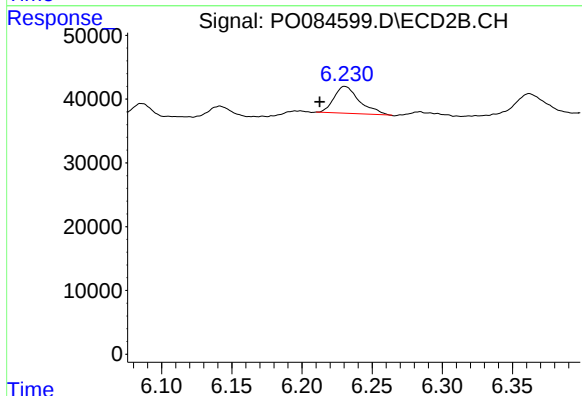


#28 AR-1254-3

R.T.: 6.230 min
Delta R.T.: 0.017 min
Response: 53110
Conc: 14.26 ng/ml m

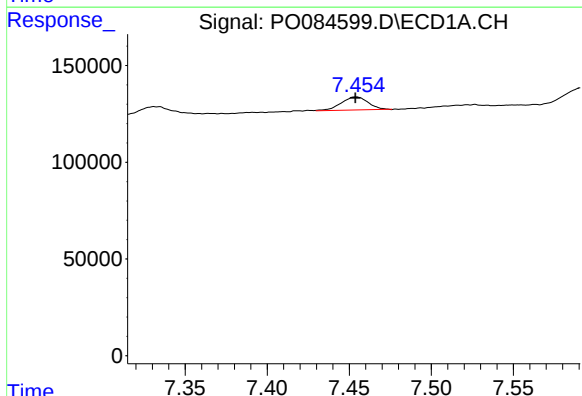


#29 AR-1254-4

R.T.: 7.454 min
Delta R.T.: 0.000 min
Response: 77232
Conc: 16.39 ng/ml m

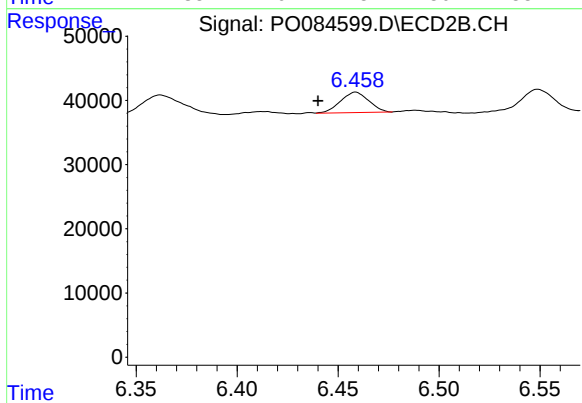

#29 AR-1254-4

R.T.: 6.458 min
Delta R.T.: 0.018 min
Response: 31140
Conc: 13.69 ng/ml m

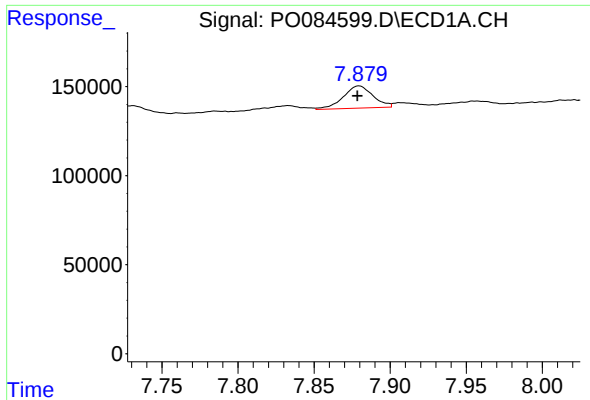


#30 AR-1254-5

R.T.: 7.880 min
Delta R.T.: 0.000 min
Response: 170926
Conc: 32.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-AUD-1257

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/11/2022
Supervised By :Ankita Jodhani 02/11/2022

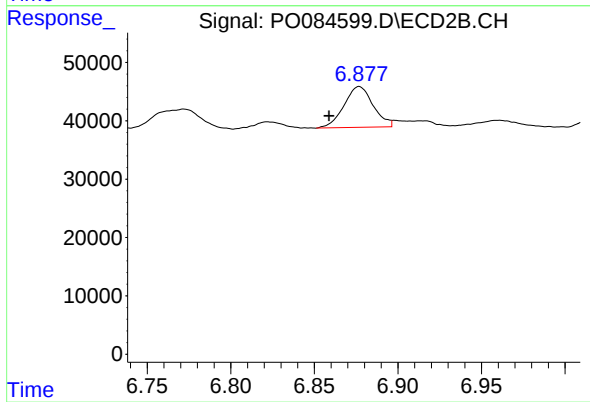

#30 AR-1254-5

R.T.: 6.877 min
Delta R.T.: 0.018 min
Response: 84939
Conc: 26.04 ng/ml m