

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021022\
 Data File : P0084603.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Feb 2022 21:32
 Operator : YP\AJ
 Sample : N1449-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220040-NACOTE-2-COMPOSITE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 05:55:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 10 07:10:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.783	1797827	656733	15.811	14.294
2) SA Decachlor...	10.447	8.827	674012	319603	8.415	8.534

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021022\
Data File : P0084603.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Feb 2022 21:32
Operator : YP\AJ
Sample : N1449-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220040-NACOTE-2-COMPOSITE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 05:55:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020822.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 10 07:10:18 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

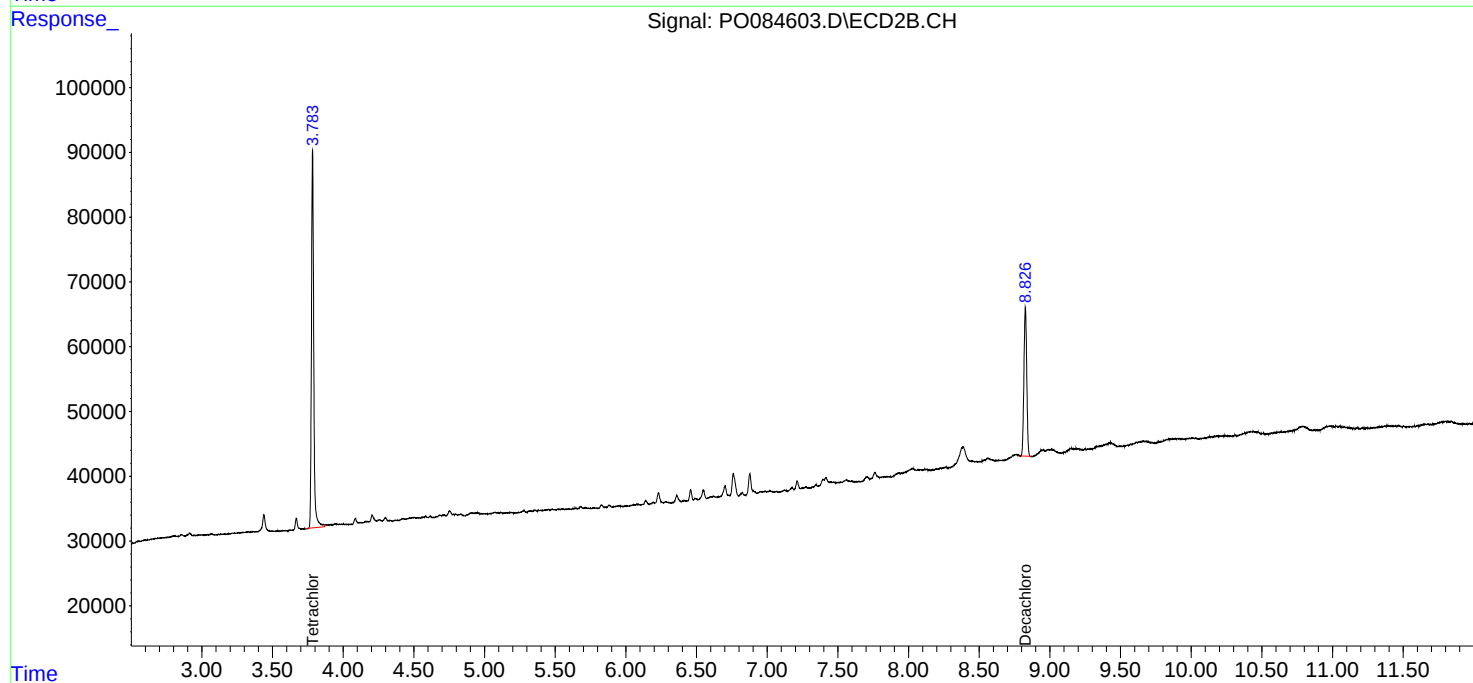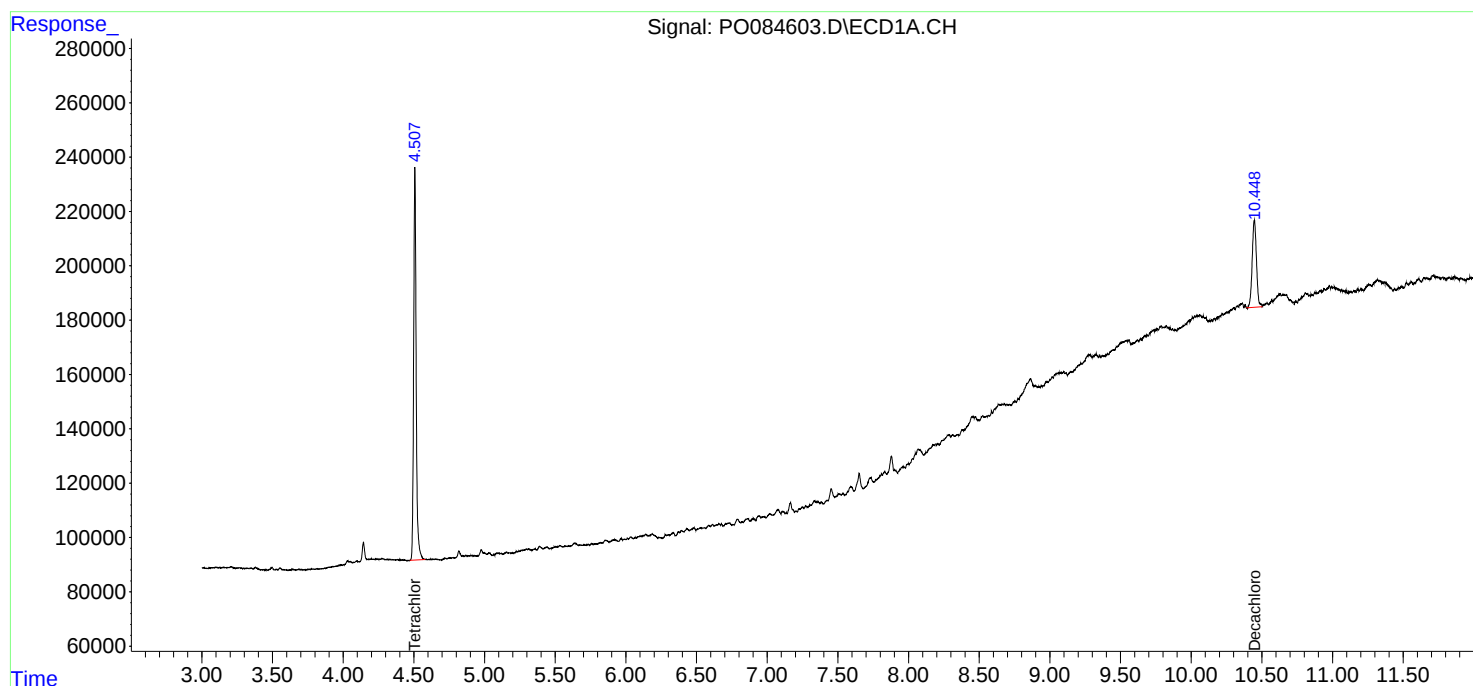


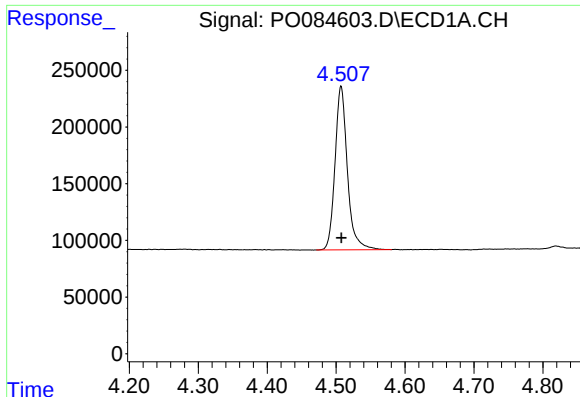

#1 Tetrachloro-m-xylene


R.T.: 4.507 min
Delta R.T.: 0.000 min
Response: 1797827
Conc: 15.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220040-NACOTE-2-COMPOSITE

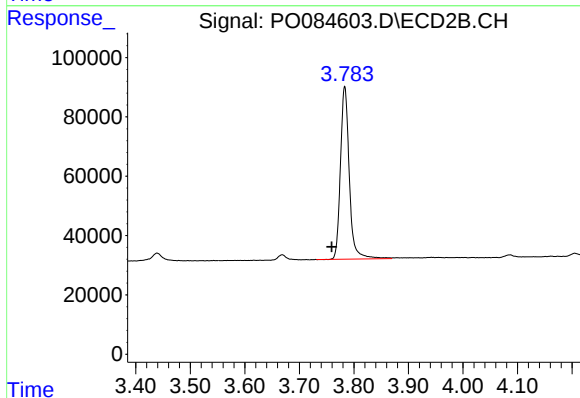


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: 0.024 min
Response: 656733
Conc: 14.29 ng/ml

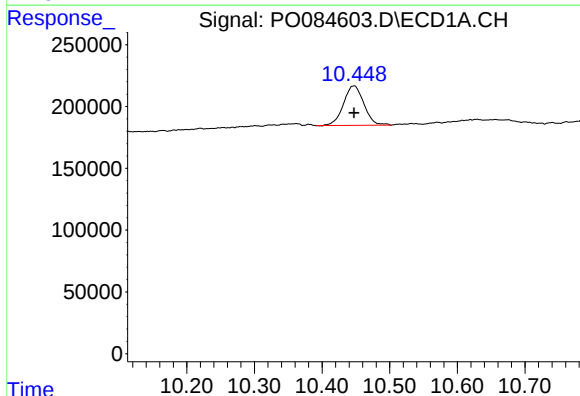

#2 Decachlorobiphenyl

R.T.: 10.447 min
Delta R.T.: 0.000 min
Response: 674012
Conc: 8.41 ng/ml

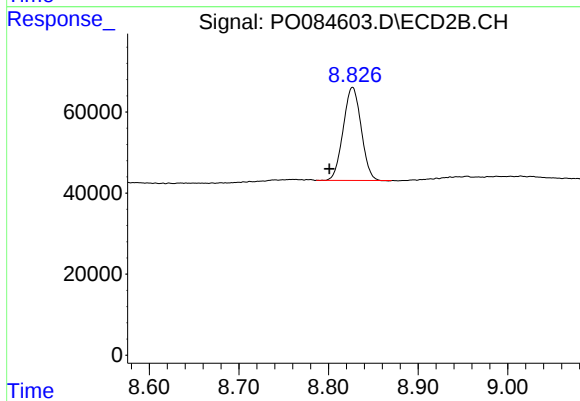

#2 Decachlorobiphenyl

R.T.: 8.827 min
Delta R.T.: 0.026 min
Response: 319603
Conc: 8.53 ng/ml