

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021120\
 Data File : P0066450.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Feb 2020 18:15
 Operator : DD\AJ
 Sample : L1478-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 330

Manual Integrations
 APPROVED

mohammad
 2/12/2020 4:47:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 05:53:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 06 18:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.139	3.417	813839	995692	28.852m	25.355
2) SA Decachlor...	9.626	8.310	1021157	1500256	24.727	25.785m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021120\
Data File : P0066450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Feb 2020 18:15
Operator : DD\AJ
Sample : L1478-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
330


Manual Integrations
APPROVED

mohammad
2/12/2020 4:47:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 05:53:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

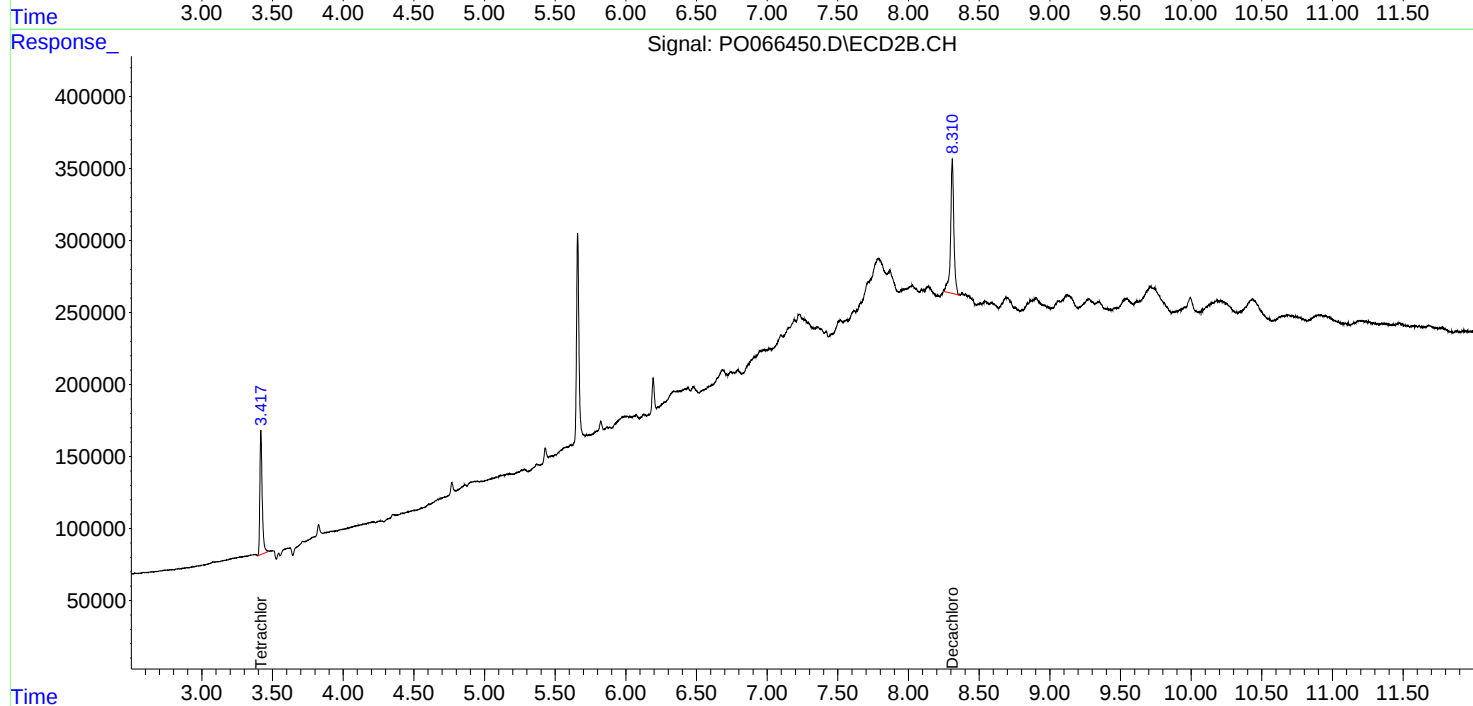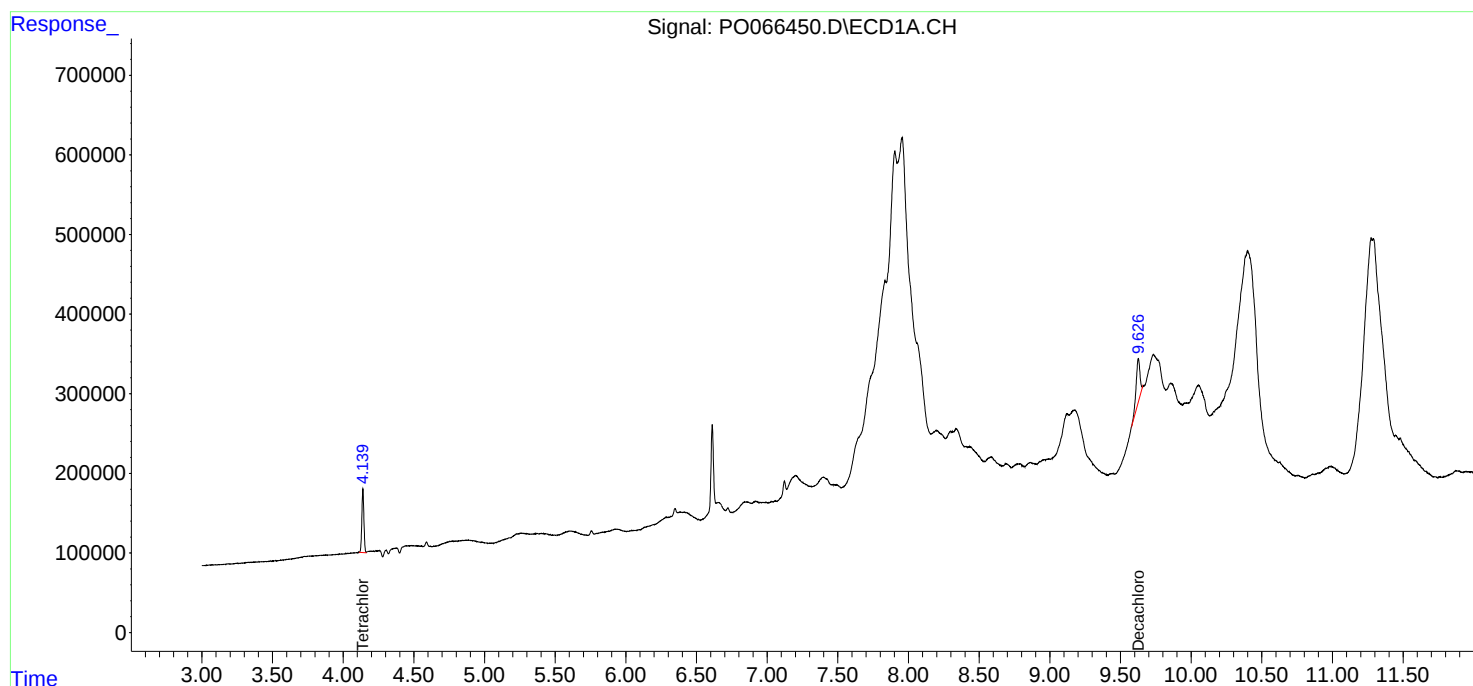

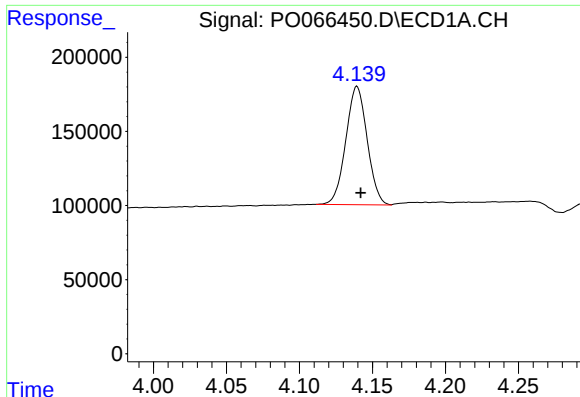


#1 Tetrachloro-m-xylene

R.T.: 4.139 min
Delta R.T.: -0.003 min
Response: 813839
Conc: 28.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
330


Manual Integrations
APPROVED

mohammad
2/12/2020 4:47:18 PM

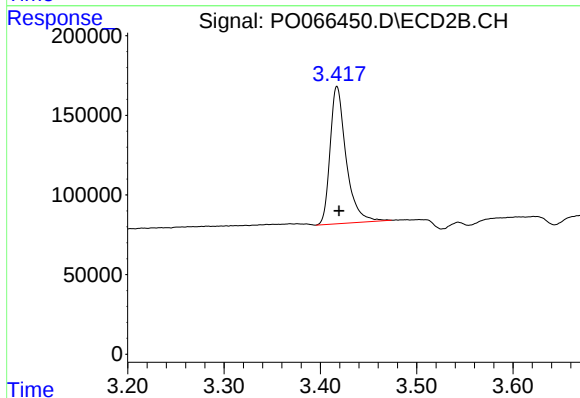


#1 Tetrachloro-m-xylene

R.T.: 3.417 min
Delta R.T.: -0.002 min
Response: 995692
Conc: 25.36 ng/ml

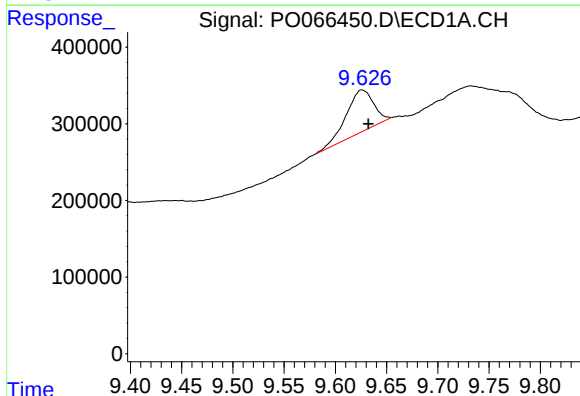

#2 Decachlorobiphenyl

R.T.: 9.626 min
Delta R.T.: -0.006 min
Response: 1021157
Conc: 24.73 ng/ml

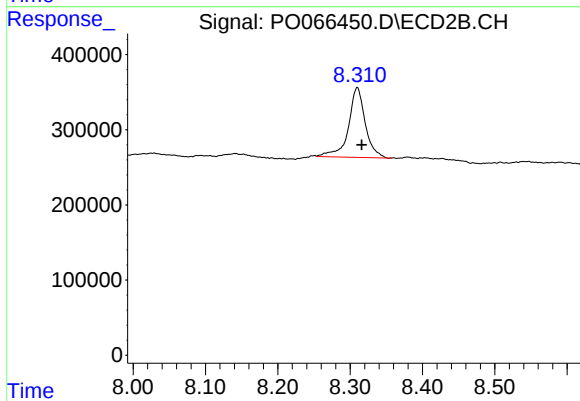

#2 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: -0.007 min
Response: 1500256
Conc: 25.79 ng/ml m