

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021120\
 Data File : P0066454.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Feb 2020 19:22
 Operator : DD\AJ
 Sample : L1372-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-01-021020

Manual Integrations
 APPROVED

mohammad
 2/12/2020 4:47:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 05:55:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 06 18:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.140	3.419	754618	1052984	26.752m	26.814
2) SA Decachlor...	9.626	8.310	576103	742088	13.950	12.754

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021120\
Data File : P0066454.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Feb 2020 19:22
Operator : DD\AJ
Sample : L1372-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-01-021020


Manual Integrations
APPROVED

mohammad
2/12/2020 4:47:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 05:55:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

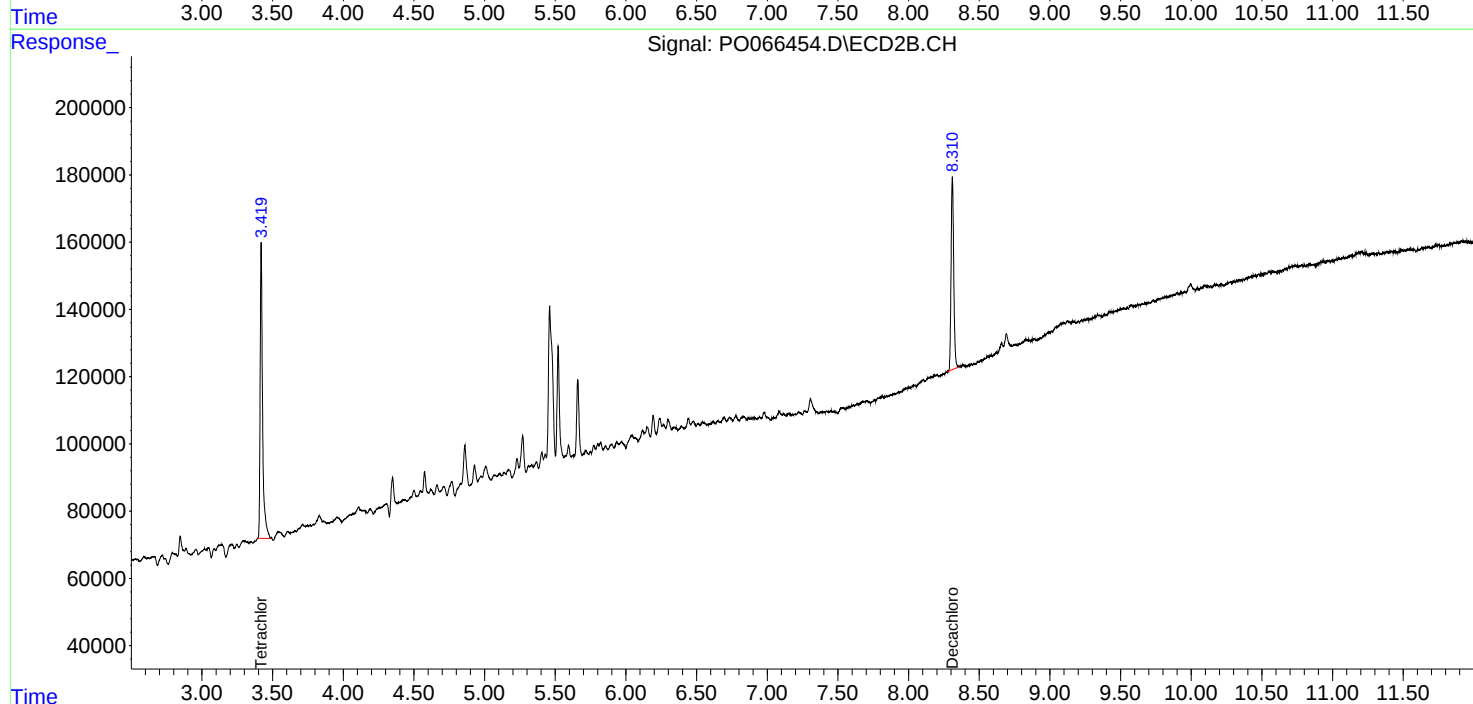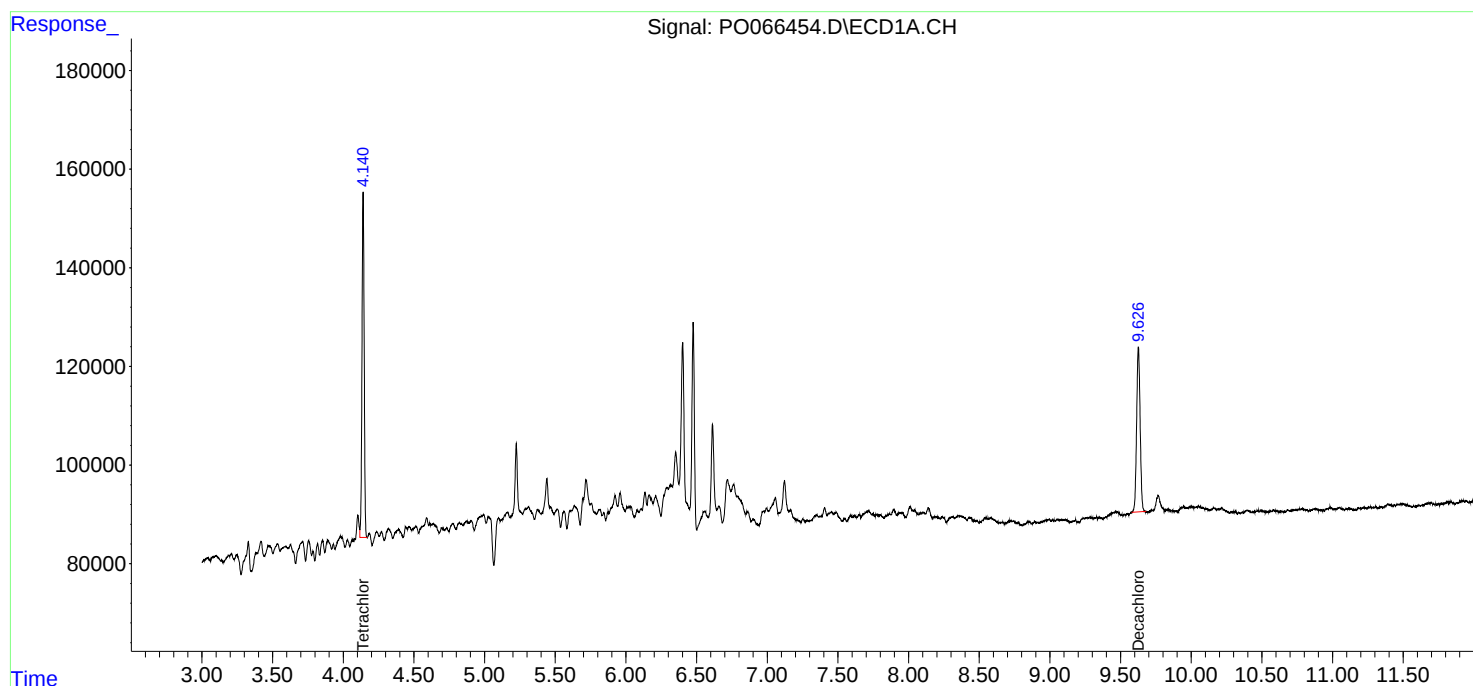

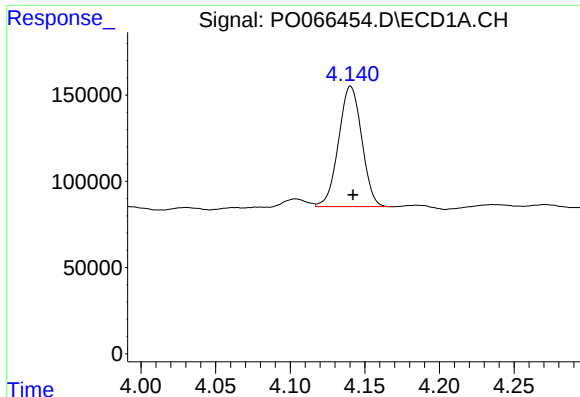


#1 Tetrachloro-m-xylene

R.T.: 4.140 min
Delta R.T.: -0.002 min
Response: 754618
Conc: 26.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU-01-021020


Manual Integrations
APPROVED

mohammad
2/12/2020 4:47:25 PM

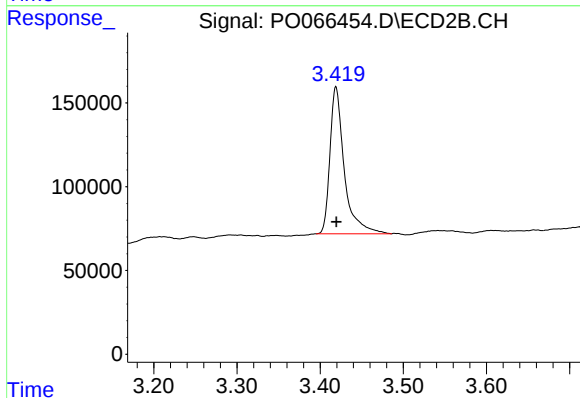


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 1052984
Conc: 26.81 ng/ml

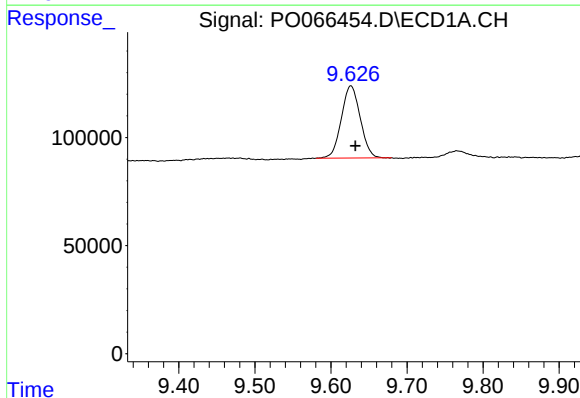

#2 Decachlorobiphenyl

R.T.: 9.626 min
Delta R.T.: -0.006 min
Response: 576103
Conc: 13.95 ng/ml

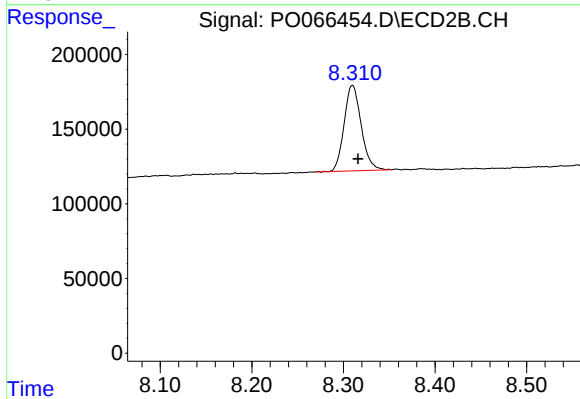

#2 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: -0.006 min
Response: 742088
Conc: 12.75 ng/ml