

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021224\
 Data File : P0101688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2024 12:22
 Operator : YP/AJ
 Sample : P1424-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1281

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/13/2024
 Supervised By :Ankita Jodhani 02/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 23:37:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.290	3.398	13826841	7428521	4.484	2.795m#
2) SA Decachlor...	9.848	8.280	5325199	3883045	2.540m	2.044

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO021224\
Data File : PO101688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2024 12:22
Operator : YP/AJ
Sample : P1424-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
1281


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :Ankita Jodhani 02/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 23:37:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

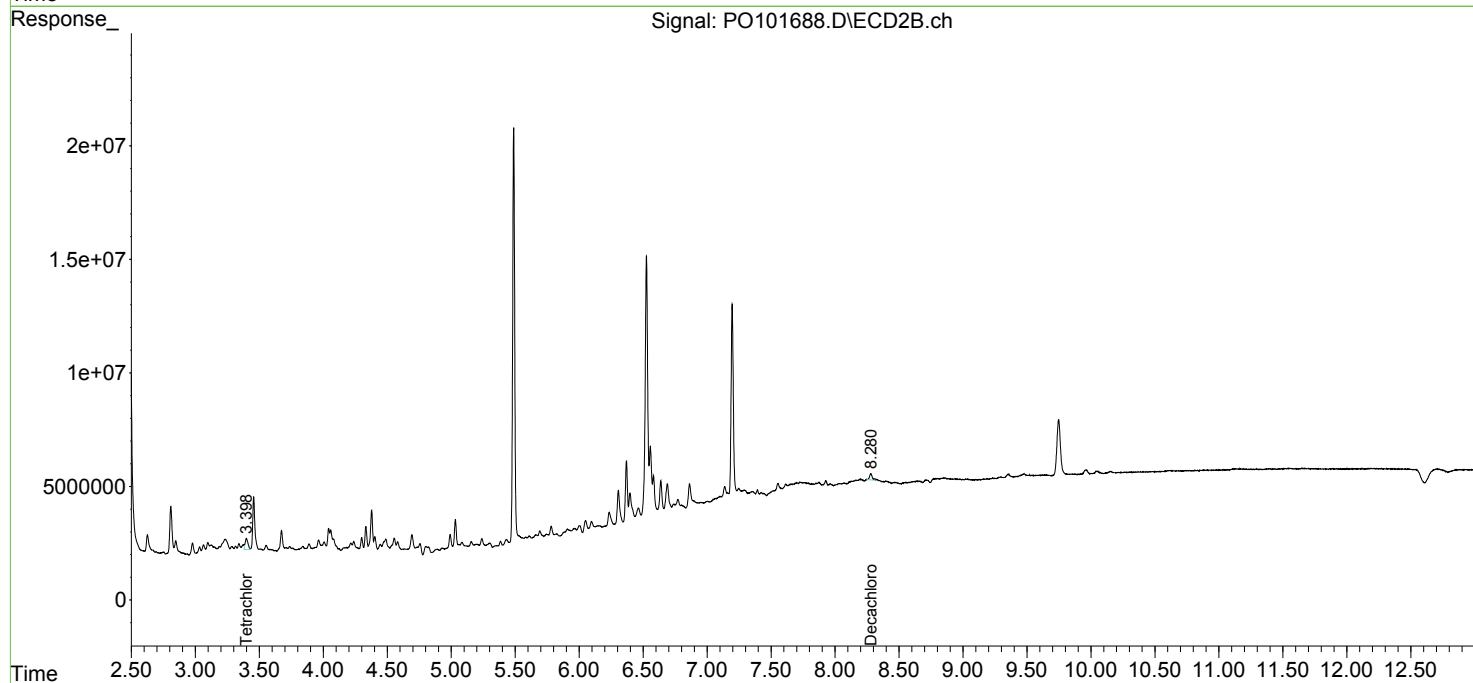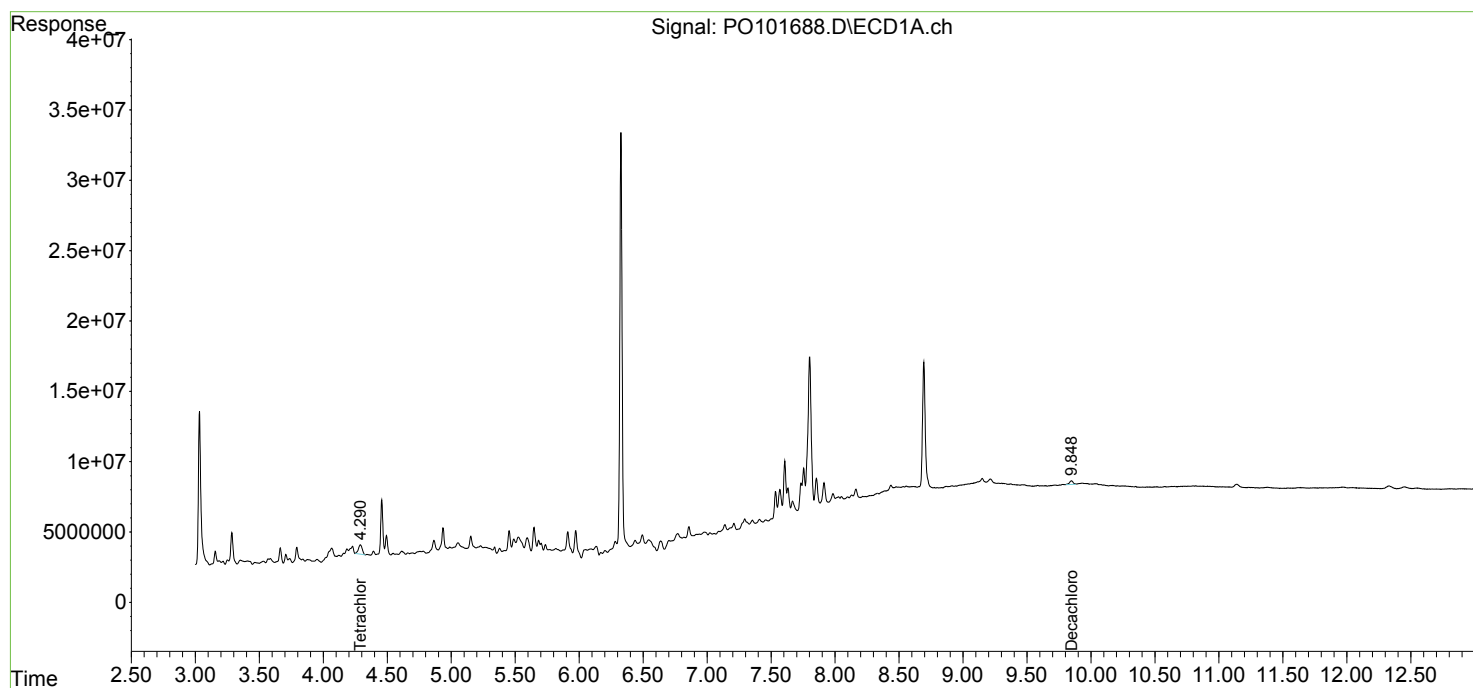

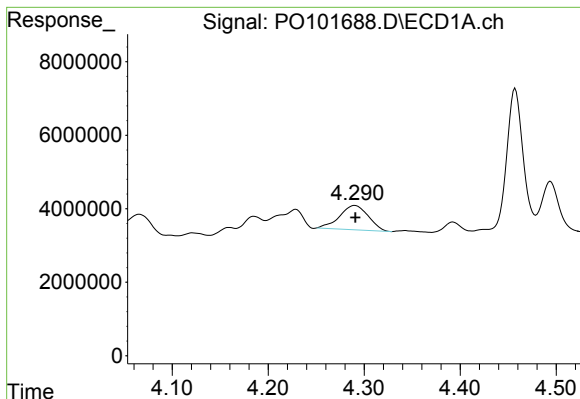

#1 Tetrachloro-m-xylene

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 13826841
Conc: 4.48 ng/ml


Instrument :

ECD_O

ClientSampleId :
1281


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :Ankita Jodhani 02/14/2024

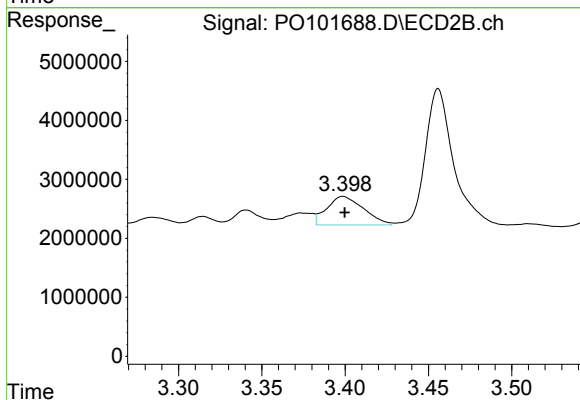


#1 Tetrachloro-m-xylene

R.T.: 3.398 min
Delta R.T.: -0.001 min
Response: 7428521
Conc: 2.79 ng/ml m

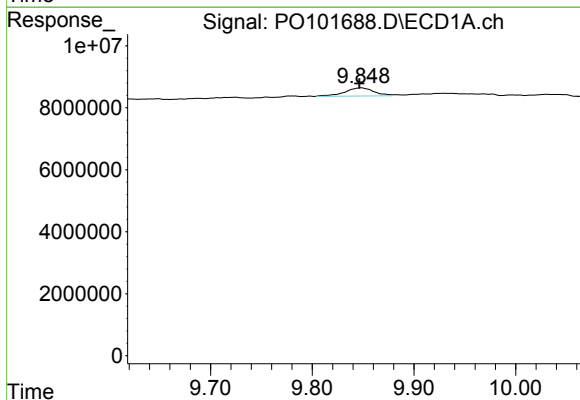

#2 Decachlorobiphenyl

R.T.: 9.848 min
Delta R.T.: 0.001 min
Response: 5325199
Conc: 2.54 ng/ml m

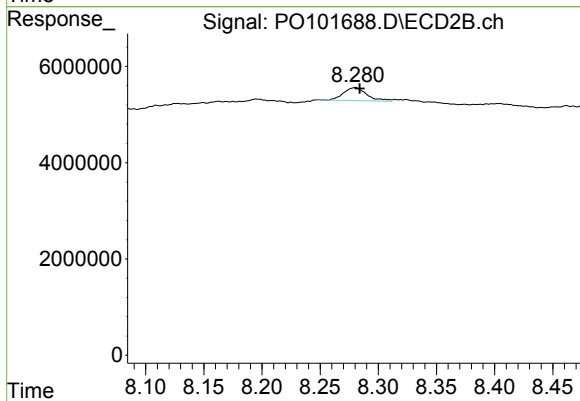

#2 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: -0.004 min
Response: 3883045
Conc: 2.04 ng/ml