

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021224\
 Data File : P0101716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2024 20:56
 Operator : YP/AJ
 Sample : P1449-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-362

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/13/2024
 Supervised By :Ankita Jodhani 02/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 23:47:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.288	3.398	79689730	54483109	25.844	20.497
2) SA Decachlor...	9.847	8.280	39573564	31804619	18.872	16.740m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021224\
Data File : PO101716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2024 20:56
Operator : YP/AJ
Sample : P1449-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-362


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :Ankita Jodhani 02/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 23:47:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

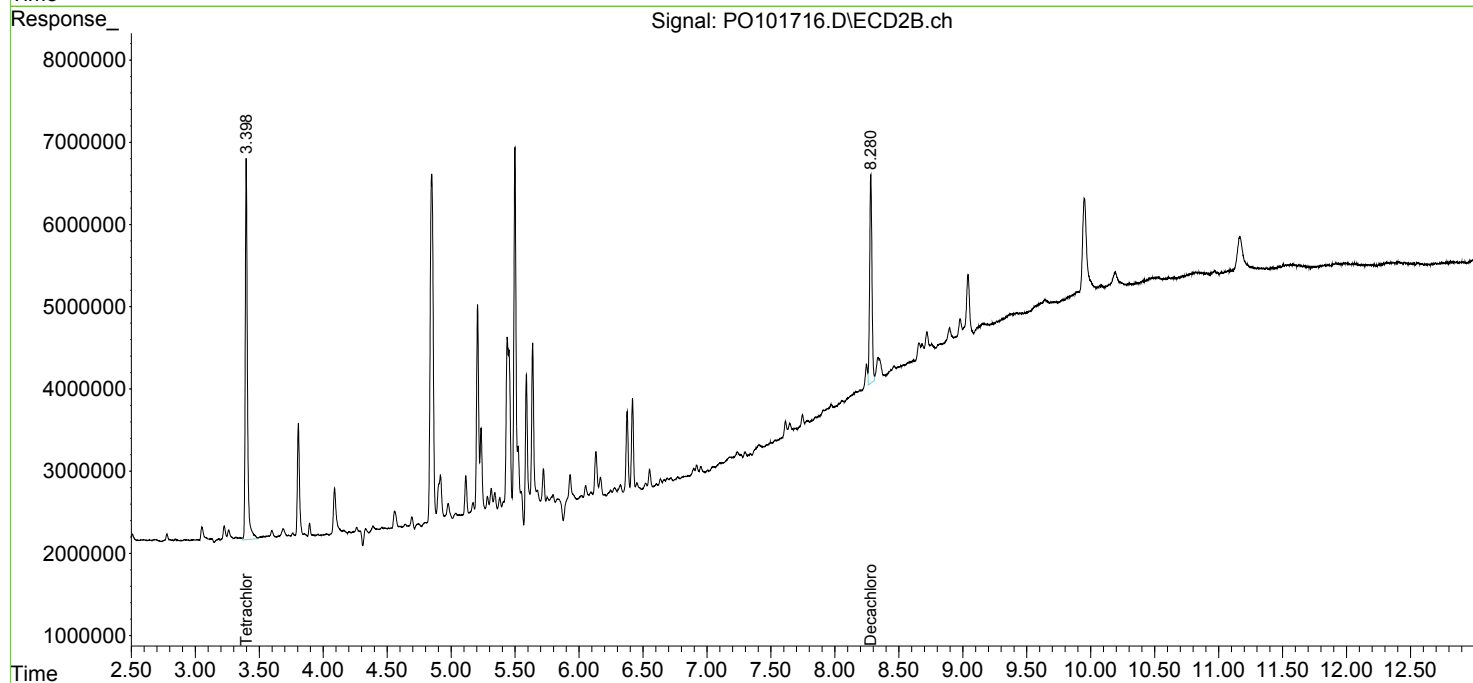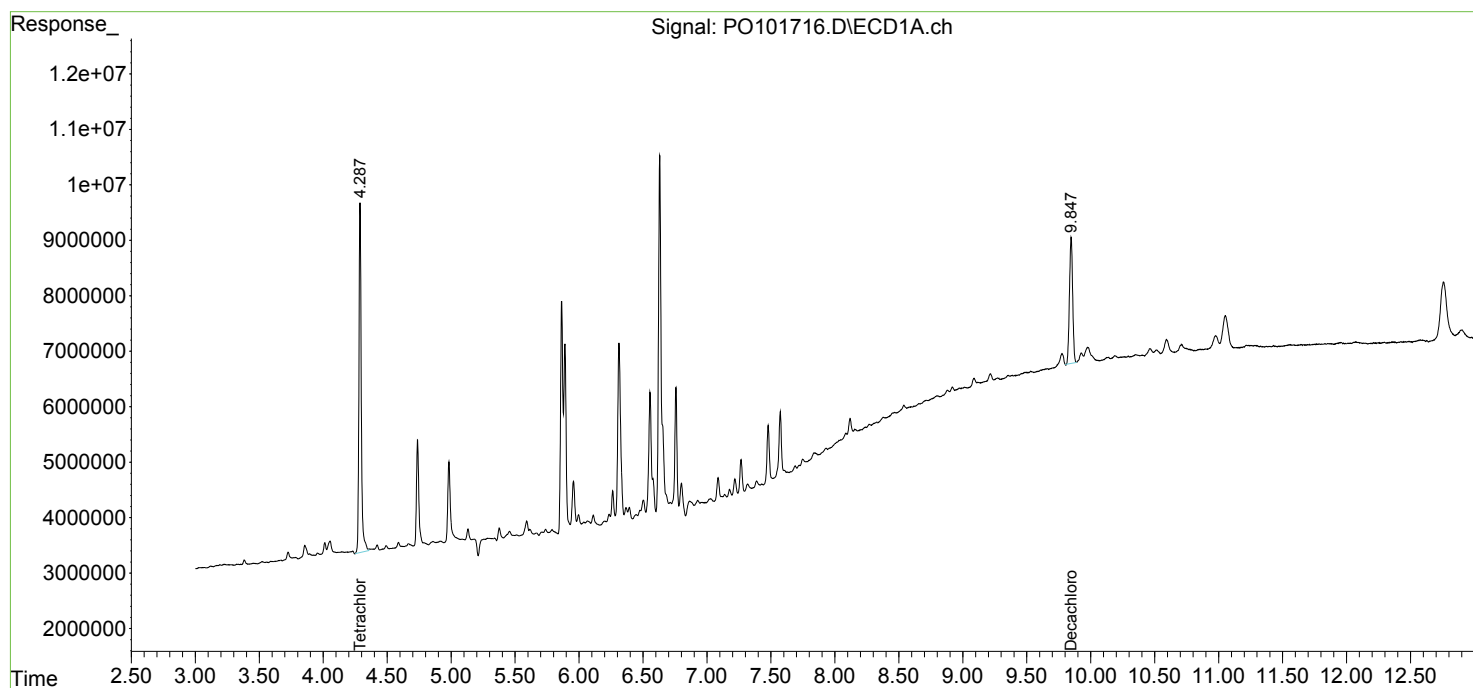

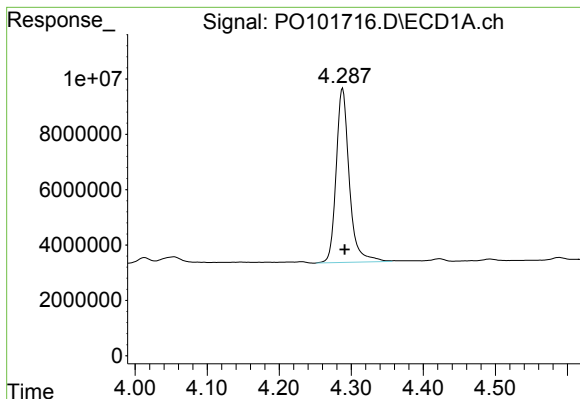


#1 Tetrachloro-m-xylene

R.T.: 4.288 min
Delta R.T.: -0.003 min
Response: 79689730
Conc: 25.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-362


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :Ankita Jodhani 02/14/2024

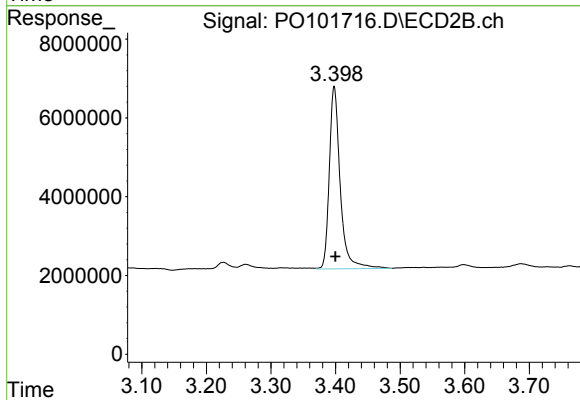


#1 Tetrachloro-m-xylene

R.T.: 3.398 min
Delta R.T.: -0.002 min
Response: 54483109
Conc: 20.50 ng/ml

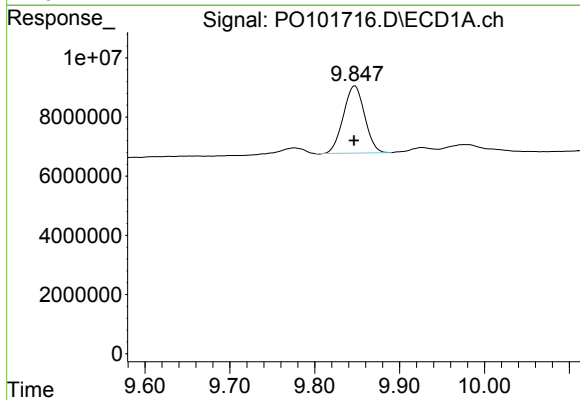

#2 Decachlorobiphenyl

R.T.: 9.847 min
Delta R.T.: 0.000 min
Response: 39573564
Conc: 18.87 ng/ml

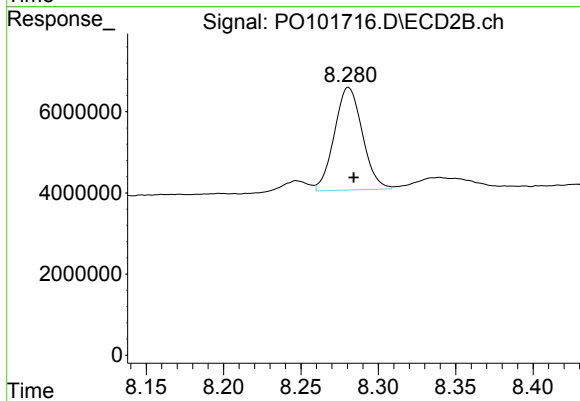

#2 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: -0.004 min
Response: 31804619
Conc: 16.74 ng/ml m