

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021224\
 Data File : P0101718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Feb 2024 21:30
 Operator : YP/AJ
 Sample : P1451-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-02092024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/13/2024
 Supervised By :Ankita Jodhani 02/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 23:47:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.288	3.398	81028186	53725095	26.278	20.212m
2) SA Decachlor...	9.847	8.282	52163924	35677083	24.876	18.779

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021224\
Data File : PO101718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Feb 2024 21:30
Operator : YP/AJ
Sample : P1451-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-01-02092024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :Ankita Jodhani 02/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 23:47:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

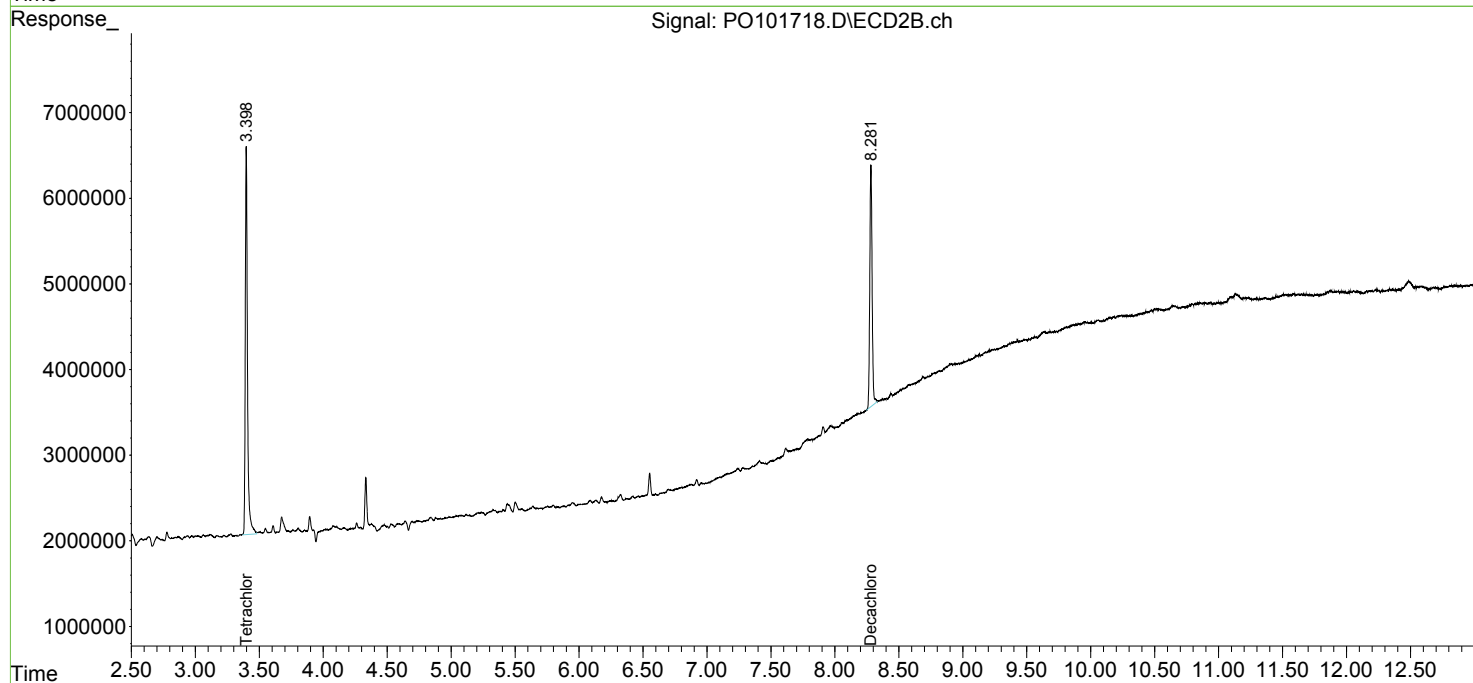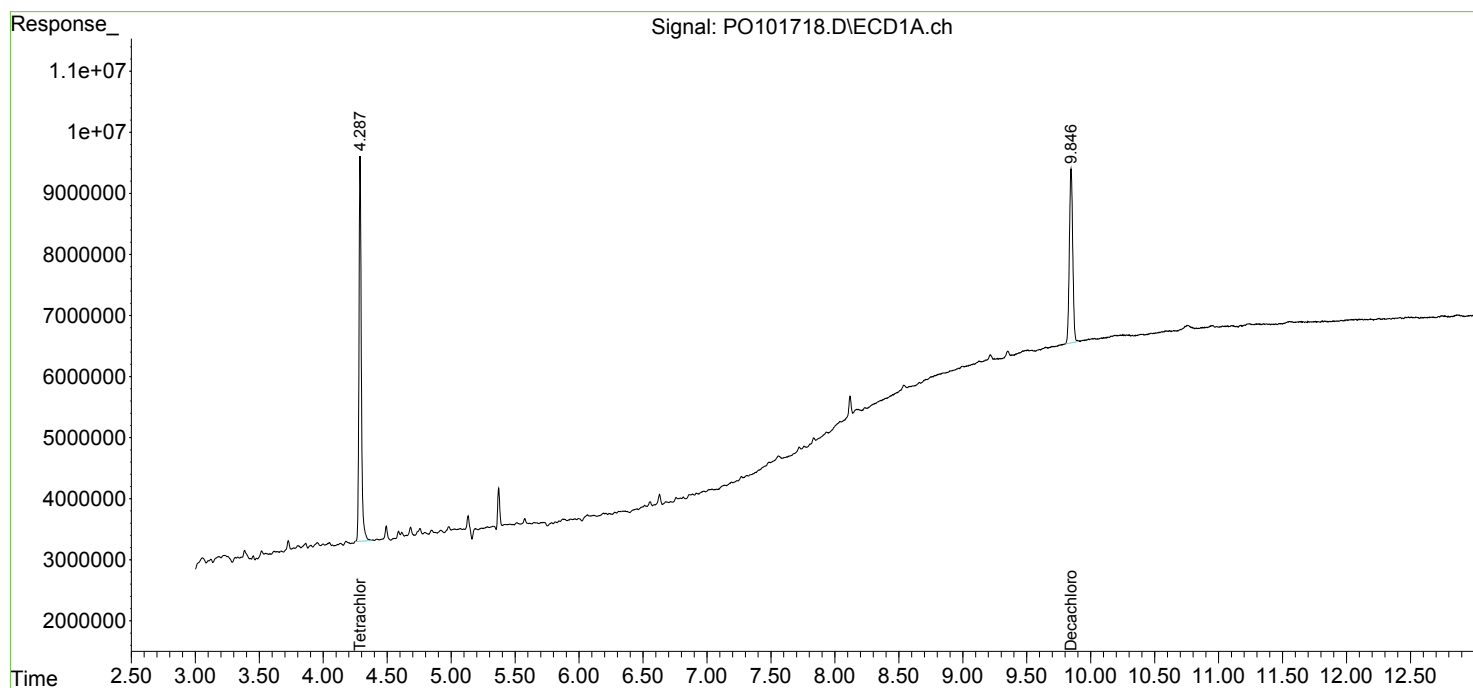

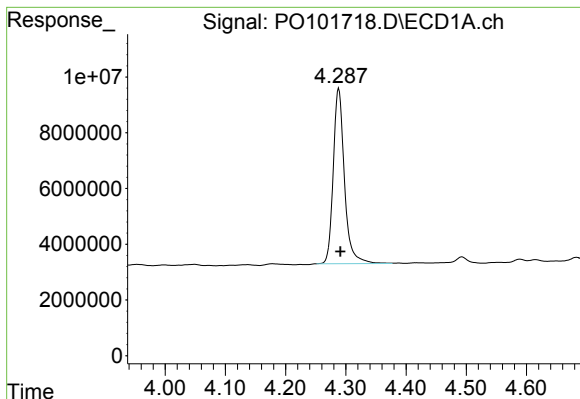


#1 Tetrachloro-m-xylene

R.T.: 4.288 min
Delta R.T.: -0.003 min
Response: 81028186
Conc: 26.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-02092024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :Ankita Jodhani 02/14/2024

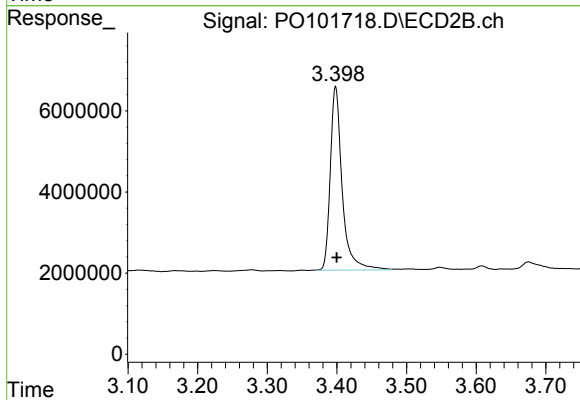


#1 Tetrachloro-m-xylene

R.T.: 3.398 min
Delta R.T.: -0.002 min
Response: 53725095
Conc: 20.21 ng/ml m

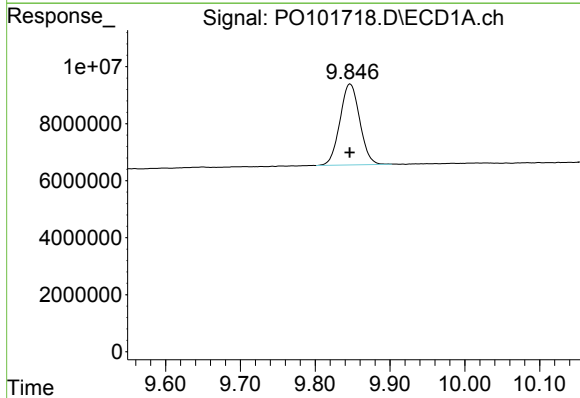

#2 Decachlorobiphenyl

R.T.: 9.847 min
Delta R.T.: 0.000 min
Response: 52163924
Conc: 24.88 ng/ml

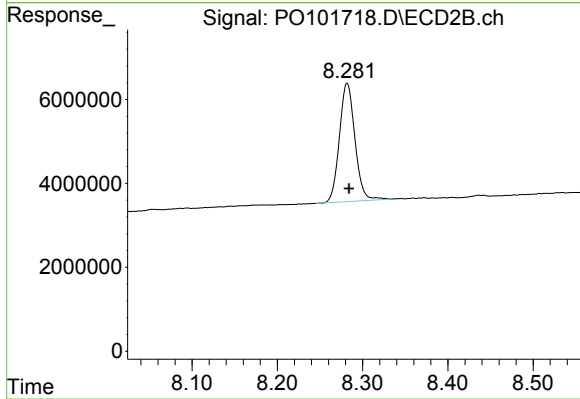

#2 Decachlorobiphenyl

R.T.: 8.282 min
Delta R.T.: -0.002 min
Response: 35677083
Conc: 18.78 ng/ml