

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021419\
 Data File : P0053878.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Feb 2019 8:04
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 15:40:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 11 14:15:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.073	3.142	86333106	6441799	24.287	23.598
2) SA Decachlor...	9.434	7.735	29978623	6639520	23.875	23.757

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO0211419\
Data File : PO053878.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Feb 2019 8:04
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 15:40:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 11 14:15:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

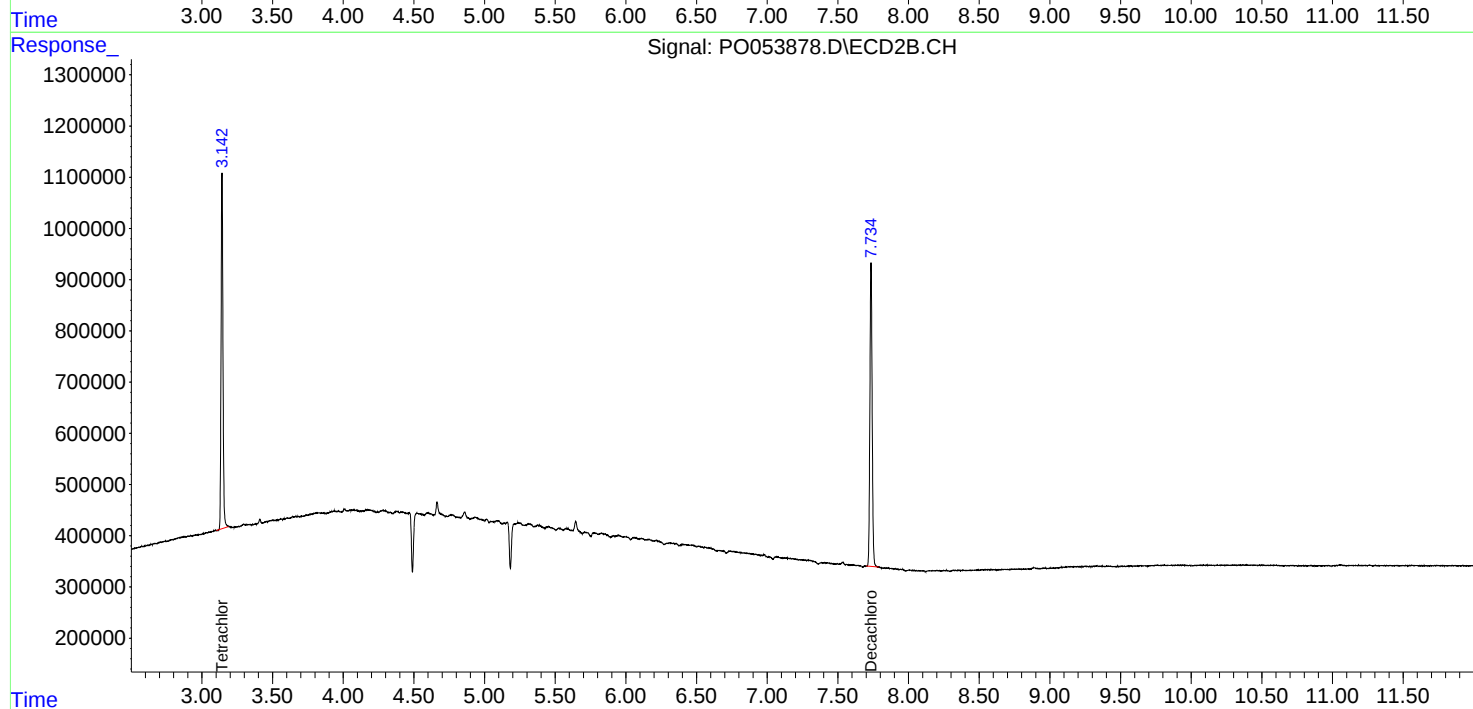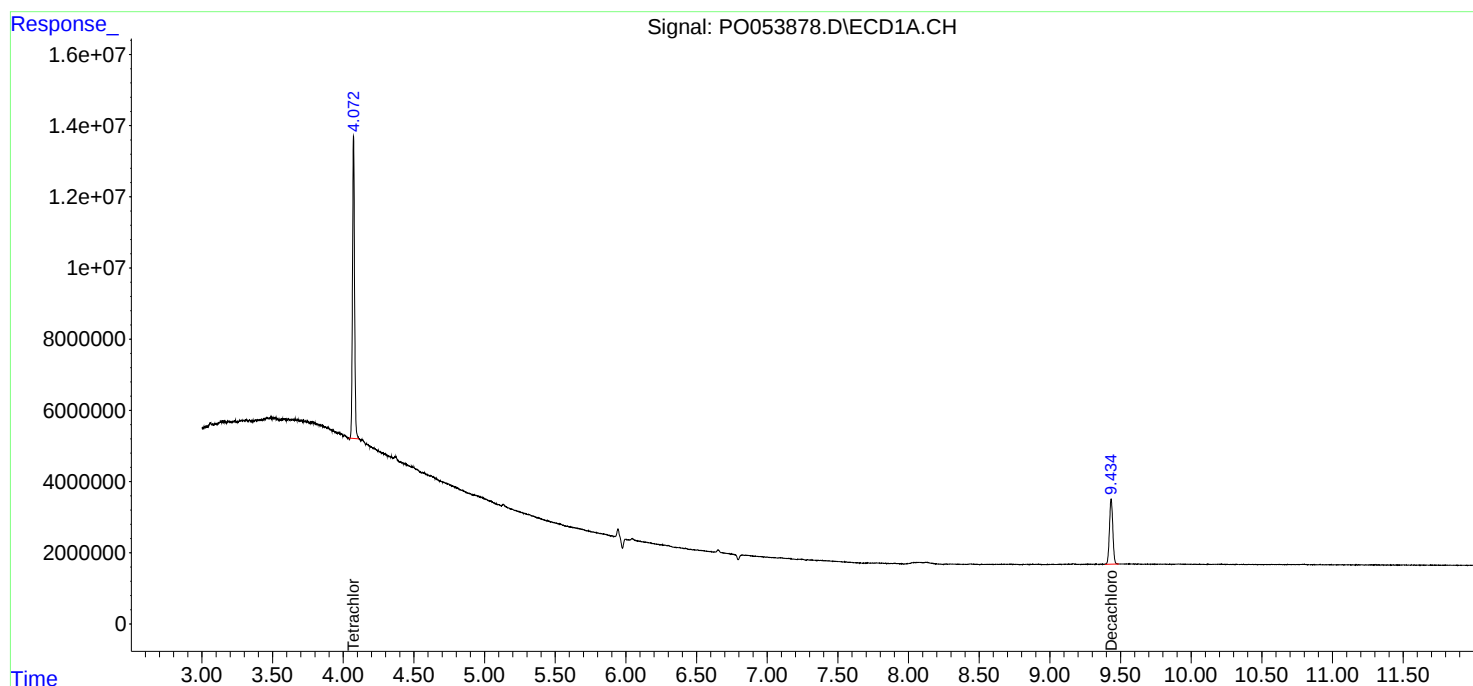


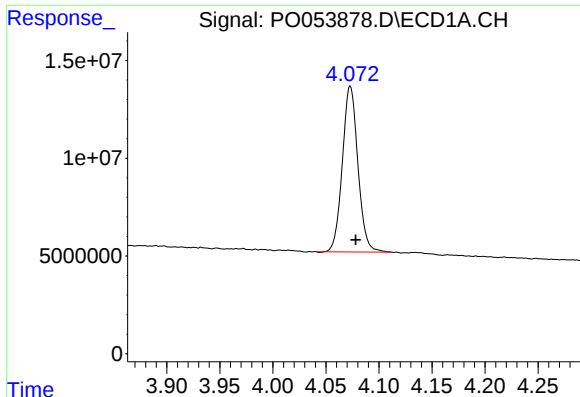

#1 Tetrachloro-m-xylene


R.T.: 4.073 min
Delta R.T.: -0.005 min
Response: 86333106
Conc: 24.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

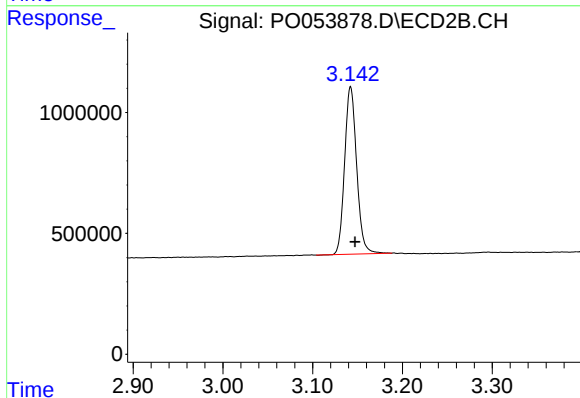


#1 Tetrachloro-m-xylene

R.T.: 3.142 min
Delta R.T.: -0.005 min
Response: 6441799
Conc: 23.60 ng/ml

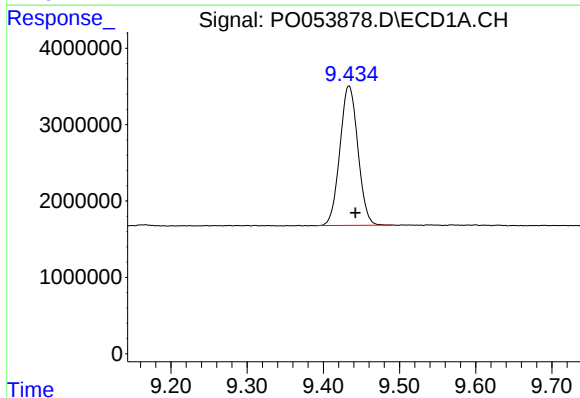

#2 Decachlorobiphenyl

R.T.: 9.434 min
Delta R.T.: -0.008 min
Response: 29978623
Conc: 23.87 ng/ml

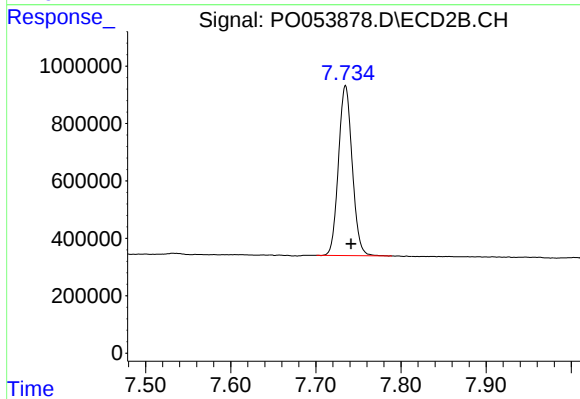

#2 Decachlorobiphenyl

R.T.: 7.735 min
Delta R.T.: -0.006 min
Response: 6639520
Conc: 23.76 ng/ml