

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021420\
 Data File : P0066536.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Feb 2020 9:39
 Operator : DD\AJ
 Sample : L1504-04RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-020720-04RE

Manual Integrations
 APPROVED

Sohil
 2/17/2020 3:33:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 14 22:10:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 13 16:40:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.130	3.411	481237	558540	14.062m	13.865
2) SA Decachlor...	9.607	8.296	503461	643660	10.979m	10.703

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021420\
Data File : P0066536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Feb 2020 9:39
Operator : DD\AJ
Sample : L1504-04RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-020720-04RE


Manual Integrations
APPROVED

Sohil
2/17/2020 3:33:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 14 22:10:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 13 16:40:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

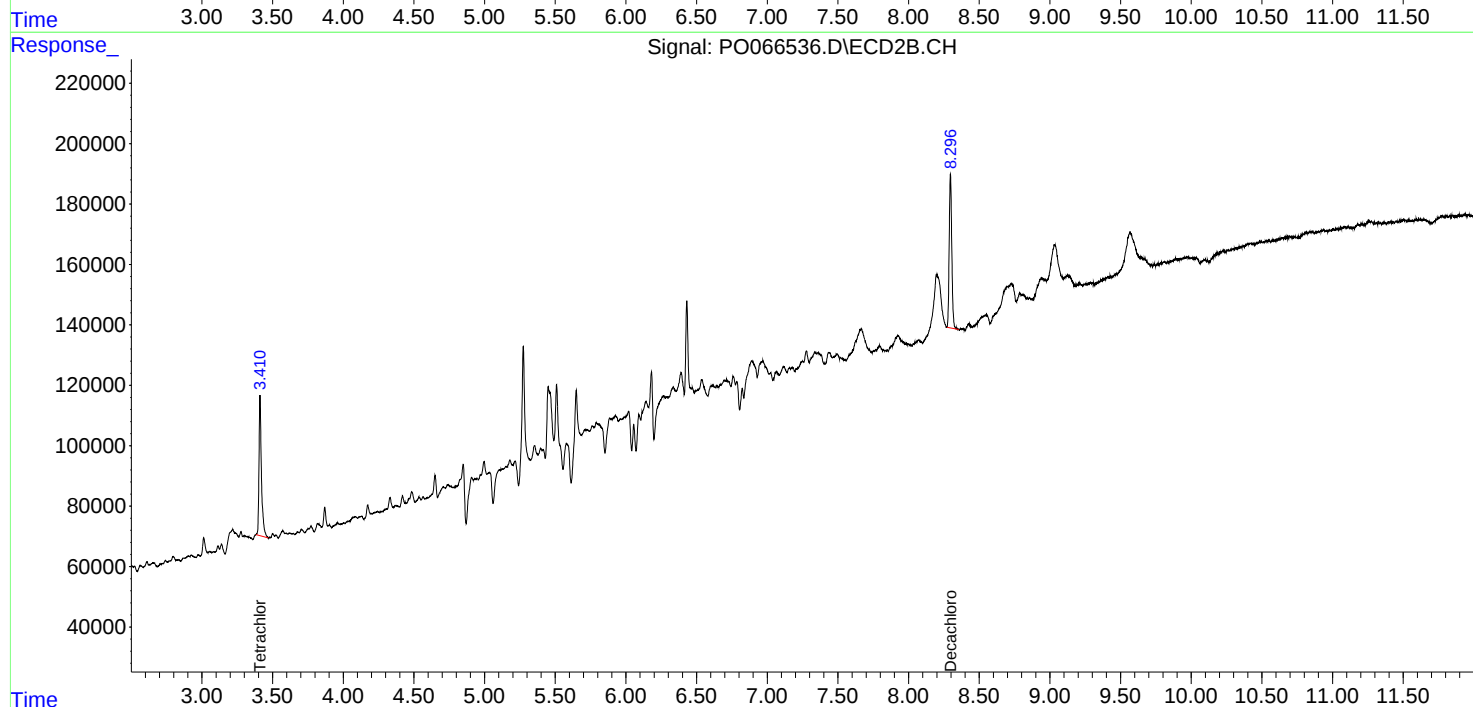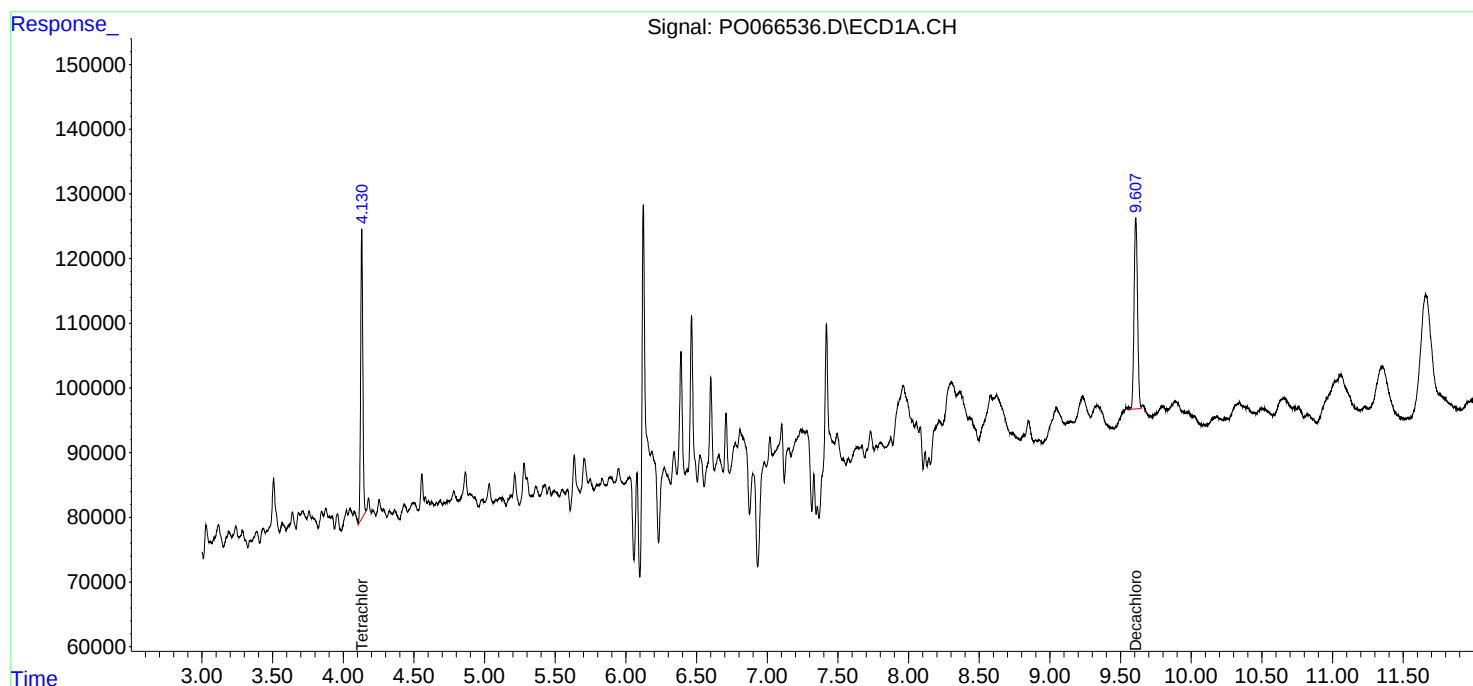

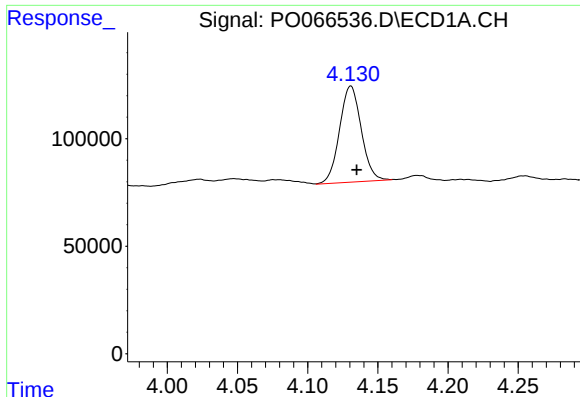


#1 Tetrachloro-m-xylene

R.T.: 4.130 min
Delta R.T.: -0.005 min
Response: 481237
Conc: 14.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-020720-04RE


Manual Integrations
APPROVED

Sohil
2/17/2020 3:33:54 PM

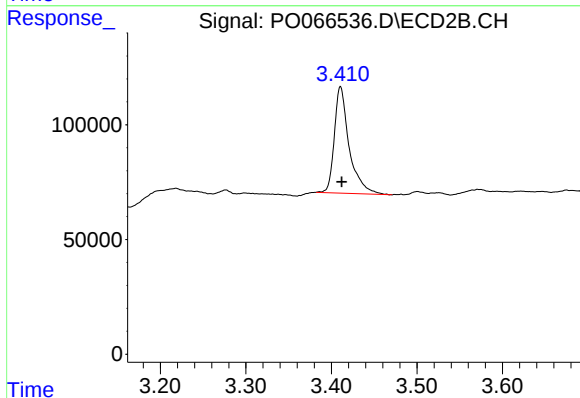


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.002 min
Response: 558540
Conc: 13.86 ng/ml

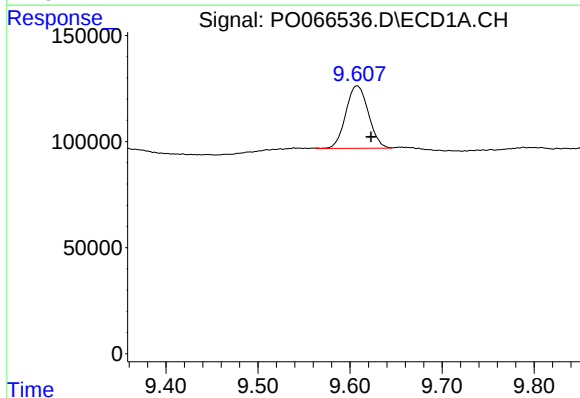

#2 Decachlorobiphenyl

R.T.: 9.607 min
Delta R.T.: -0.015 min
Response: 503461
Conc: 10.98 ng/ml m

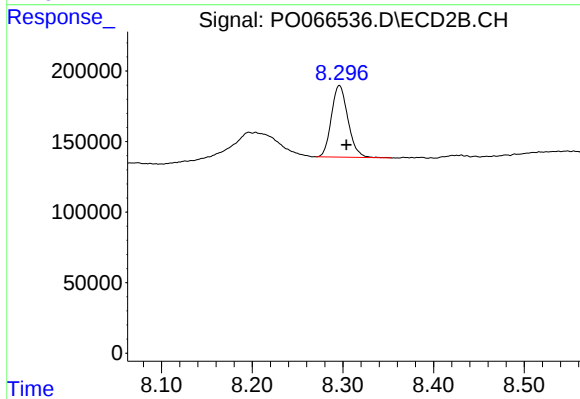

#2 Decachlorobiphenyl

R.T.: 8.296 min
Delta R.T.: -0.008 min
Response: 643660
Conc: 10.70 ng/ml