

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021522\
Data File : P0084650.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2022 13:37
Operator : YP\AJ
Sample : N1537-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-63A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:22:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.505	3.596	189831	67382	0.965	1.494 #
2) SA Decachlor...	10.426	8.624	171227	49614	1.380	1.361

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021522\
Data File : P0084650.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2022 13:37
Operator : YP\AJ
Sample : N1537-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-63A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:22:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

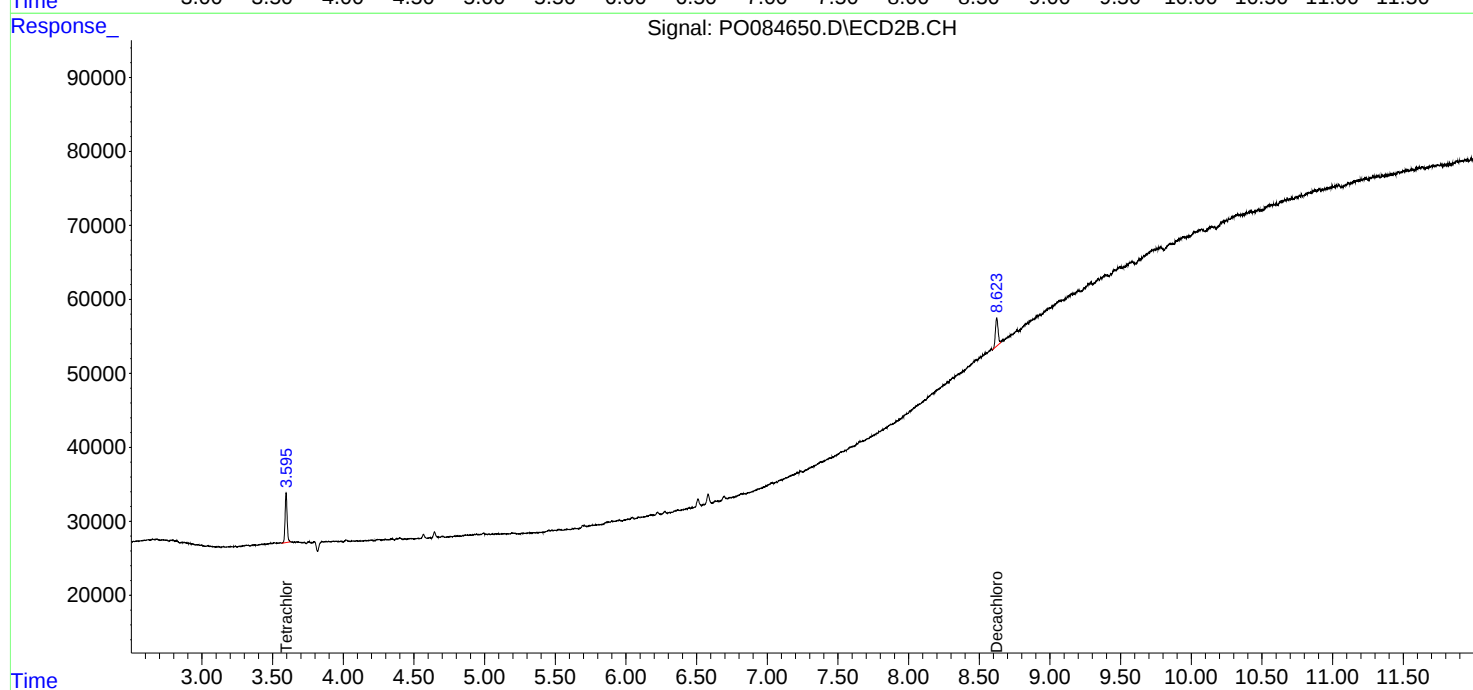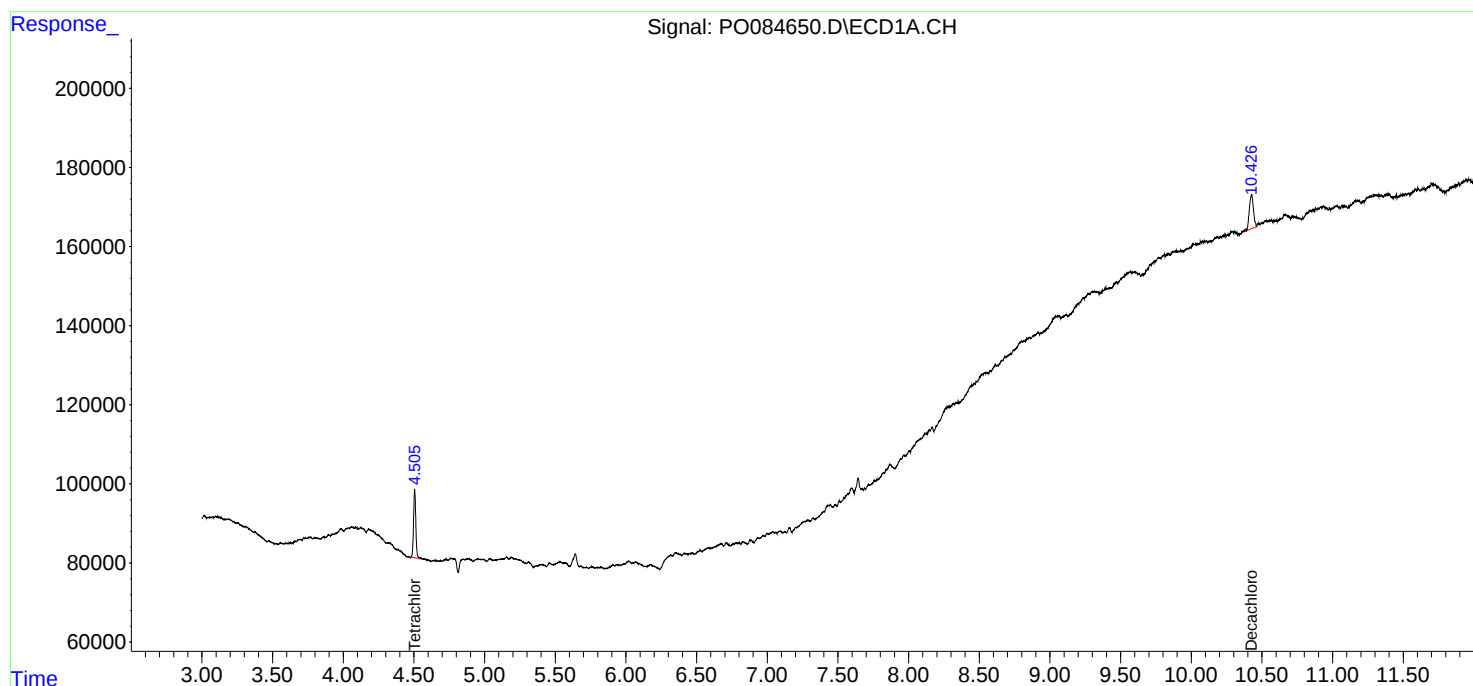


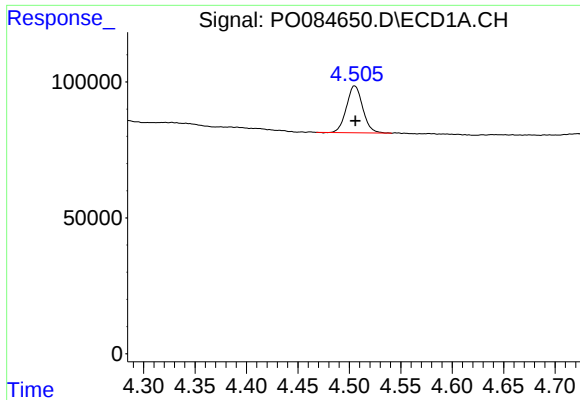

#1 Tetrachloro-m-xylene


R.T.: 4.505 min
Delta R.T.: 0.000 min
Response: 189831
Conc: 0.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-63A

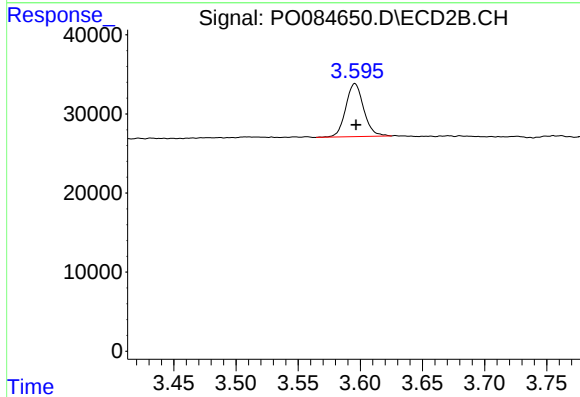


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: 0.000 min
Response: 67382
Conc: 1.49 ng/ml

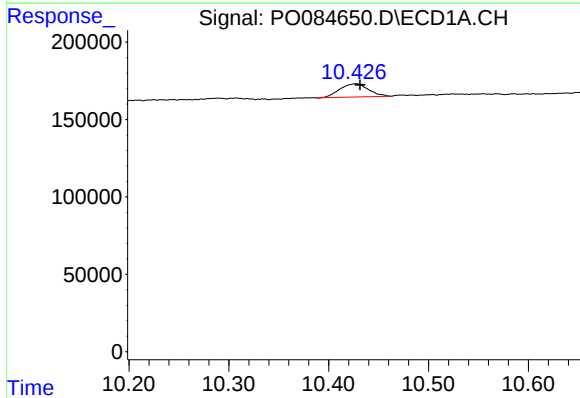

#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.005 min
Response: 171227
Conc: 1.38 ng/ml

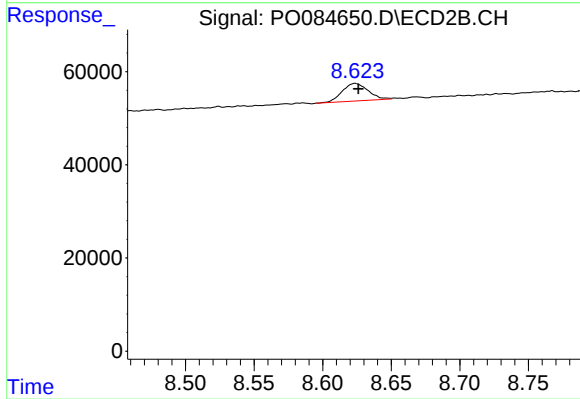

#2 Decachlorobiphenyl

R.T.: 8.624 min
Delta R.T.: -0.002 min
Response: 49614
Conc: 1.36 ng/ml