

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021522\
 Data File : P0084666.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2022 19:06
 Operator : YP\AJ
 Sample : N1511-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-NACOTE-1-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 01:24:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.505	3.597	3954549	946982	20.113	20.998
2) SA Decachlor...	10.422	8.620	2066602	561088	16.654	15.391

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021522\
Data File : P0084666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2022 19:06
Operator : YP\AJ
Sample : N1511-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE-AMENDED-NACOTE-1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 01:24:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

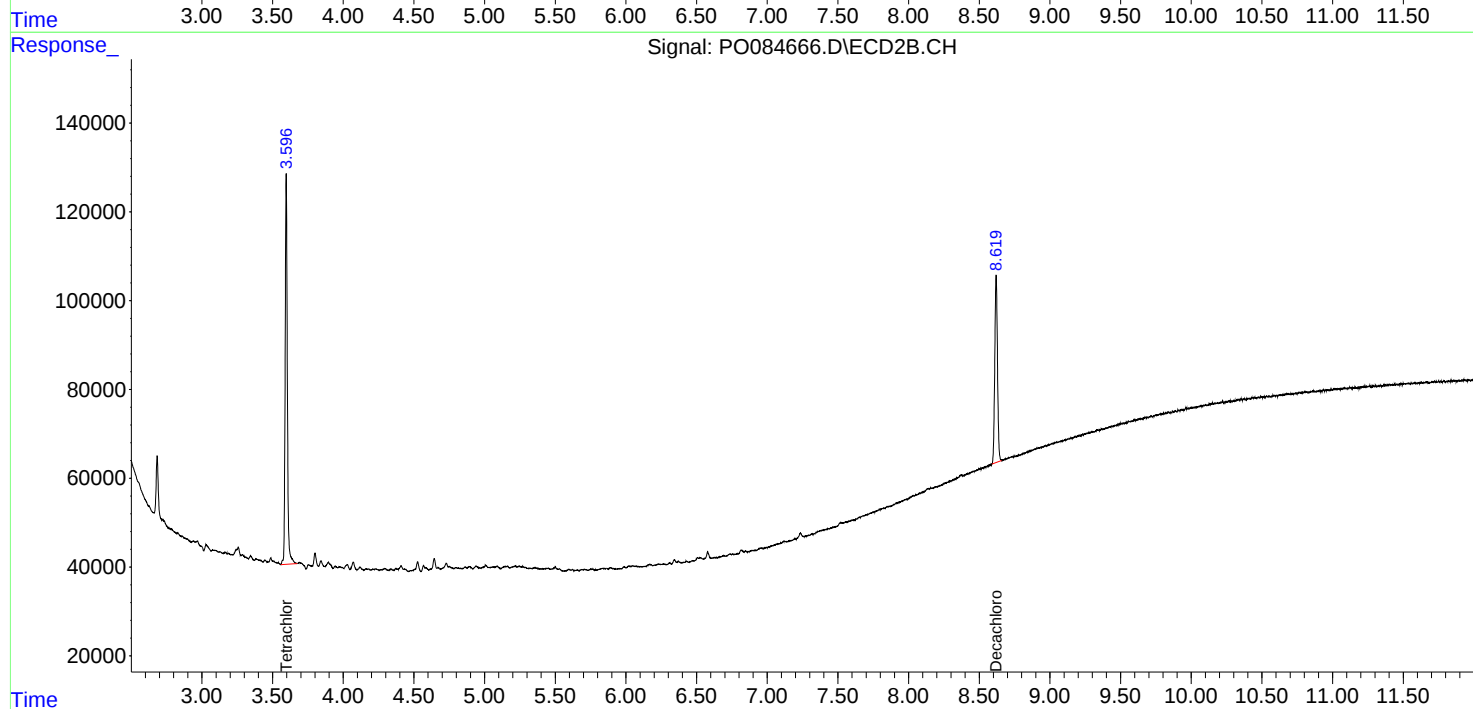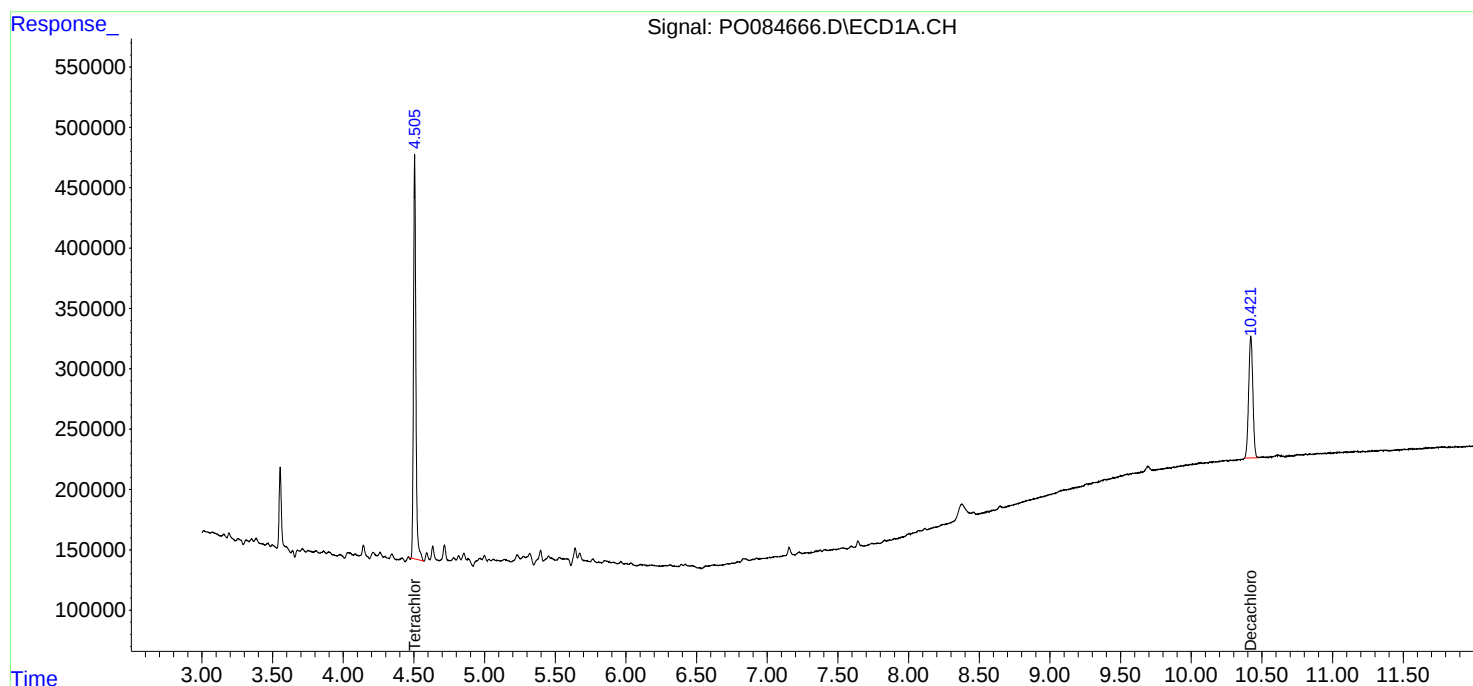


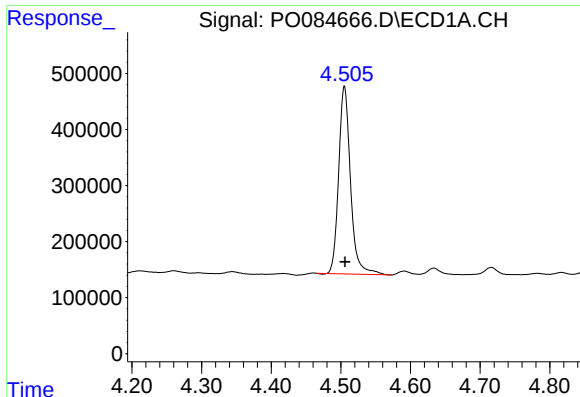

#1 Tetrachloro-m-xylene


R.T.: 4.505 min
Delta R.T.: 0.000 min
Response: 3954549
Conc: 20.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACHATE-AMENDED-NACOTE-1-COMP

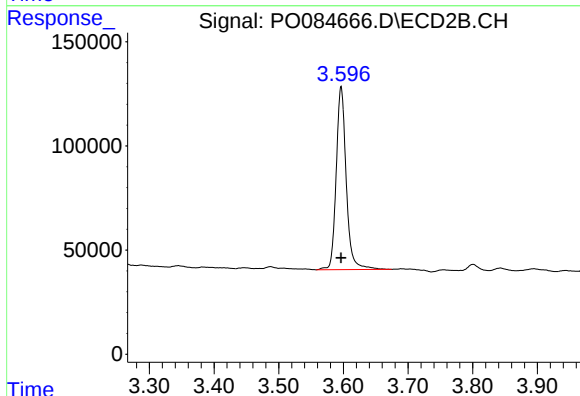


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: 0.000 min
Response: 946982
Conc: 21.00 ng/ml

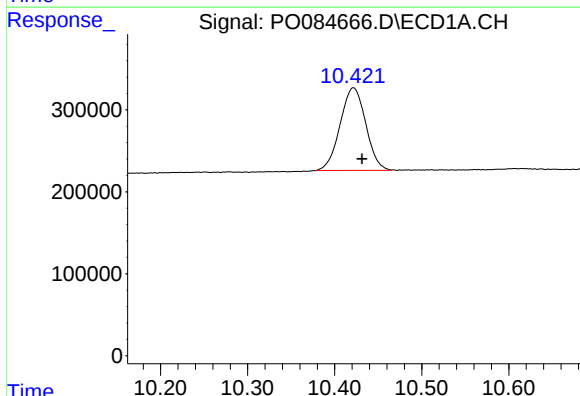

#2 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.010 min
Response: 2066602
Conc: 16.65 ng/ml

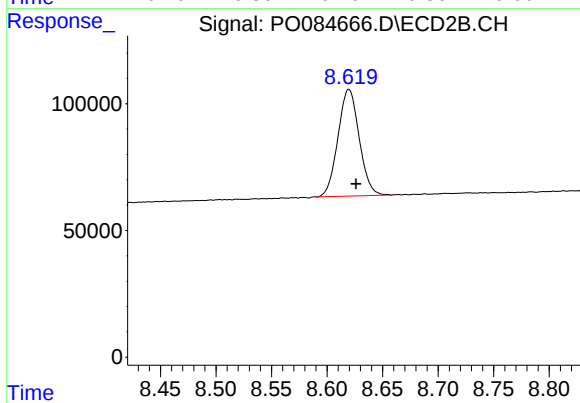

#2 Decachlorobiphenyl

R.T.: 8.620 min
Delta R.T.: -0.006 min
Response: 561088
Conc: 15.39 ng/ml