

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0021522\
 Data File : P0084672.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2022 21:24
 Operator : YP\AJ
 Sample : N1537-11 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 IRV-2022-55A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/16/2022
 Supervised By :Ankita Jodhani 02/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 00:39:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.503	3.594	143015	54662	0.727m	1.212m#
2) SA Decachlor...	10.417	8.619	154229	48200	1.243	1.322
Target Compounds						
26) L6 AR-1254-1	6.562	5.489	298270	143426	46.110	56.035
27) L6 AR-1254-2	6.784	5.638	411279	139054	41.629	62.126 #
28) L6 AR-1254-3	7.154	6.041	352572	170266	34.034	46.777 #
29) L6 AR-1254-4	7.443	6.271	390004	116696	53.270	51.936
30) L6 AR-1254-5	7.868	6.691	367459	149629	45.650	45.774

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021522\
Data File : PO084672.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2022 21:24
Operator : YP\AJ
Sample : N1537-11 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IRV-2022-55A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/16/2022
Supervised By :Ankita Jodhani 02/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:39:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

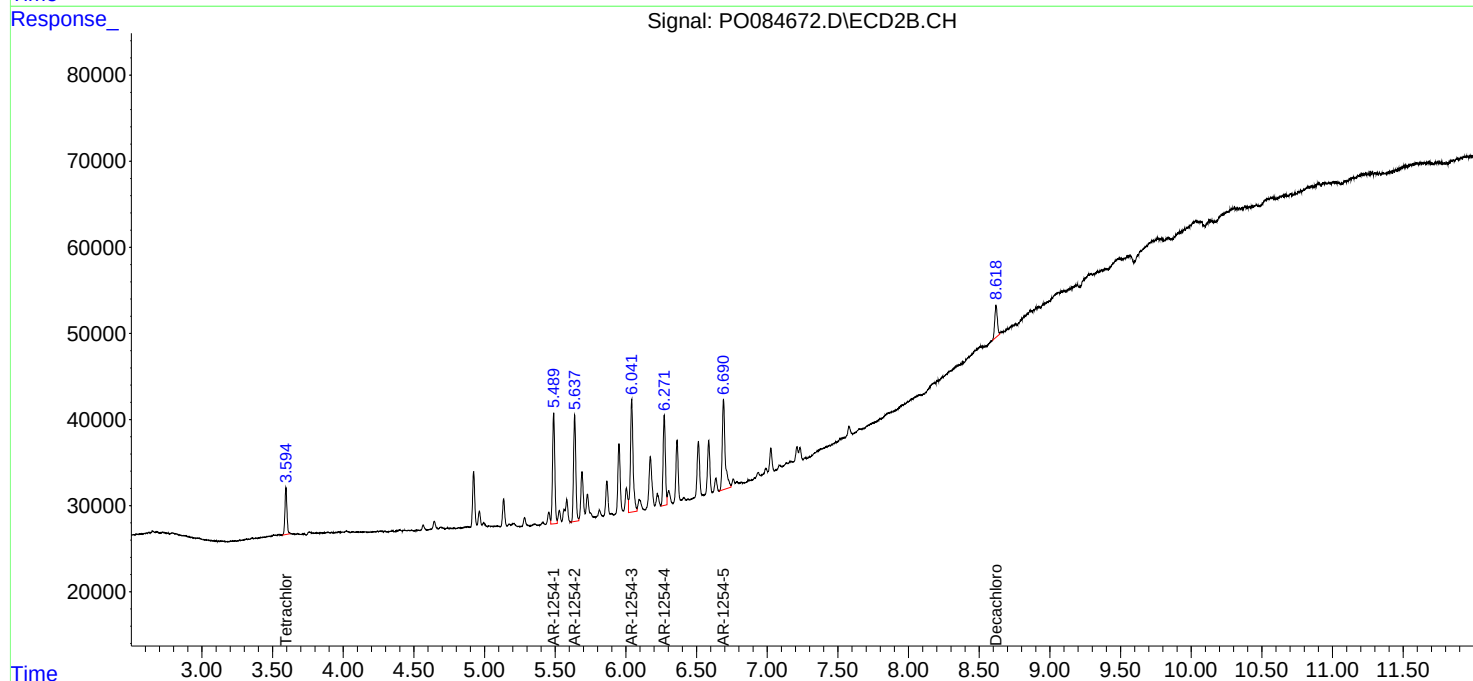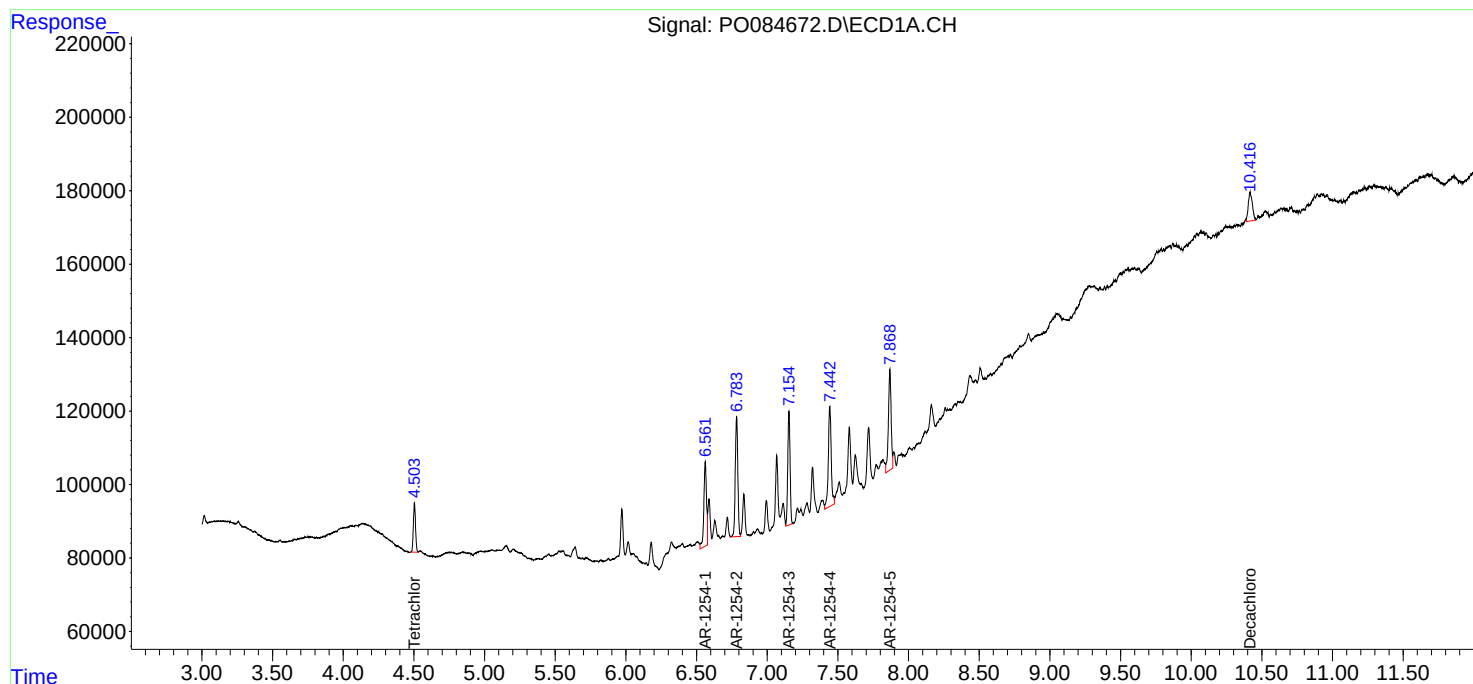

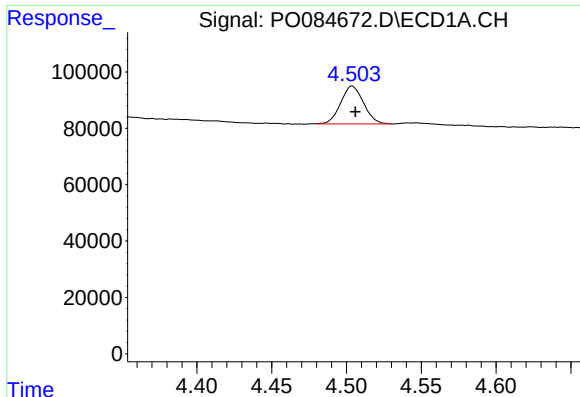

#1 Tetrachloro-m-xylene

R.T.: 4.503 min
Delta R.T.: -0.003 min
Response: 143015
Conc: 0.73 ng/ml

Instrument :

ECD_O


ClientSampleId :

IRV-2022-55A

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 02/16/2022
Supervised By :Ankita Jodhani 02/16/2022

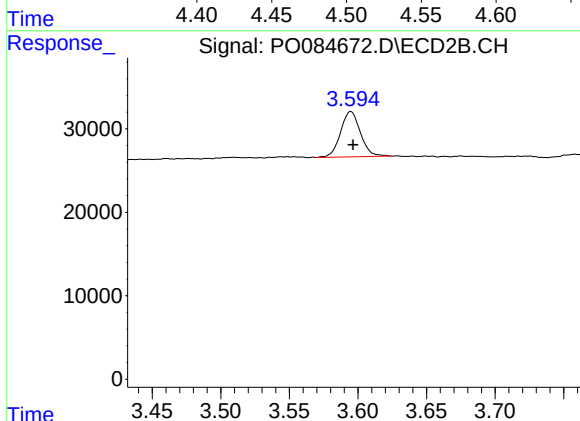


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: -0.002 min
Response: 54662
Conc: 1.21 ng/ml m

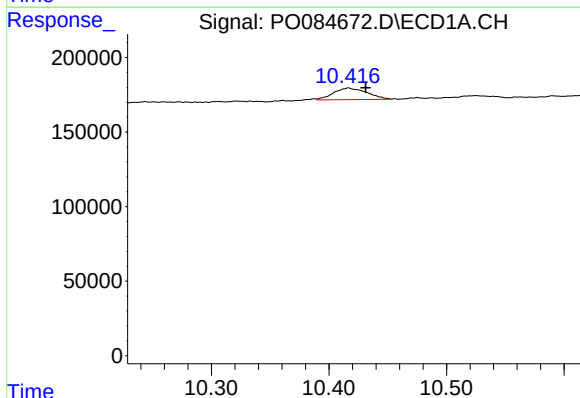


#2 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.015 min
Response: 154229
Conc: 1.24 ng/ml

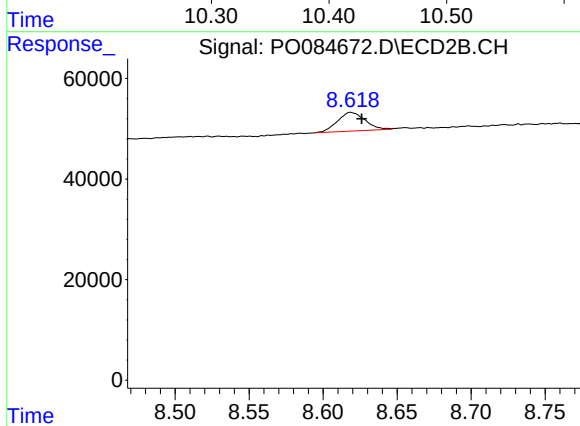

#2 Decachlorobiphenyl

R.T.: 8.619 min
Delta R.T.: -0.007 min
Response: 48200
Conc: 1.32 ng/ml

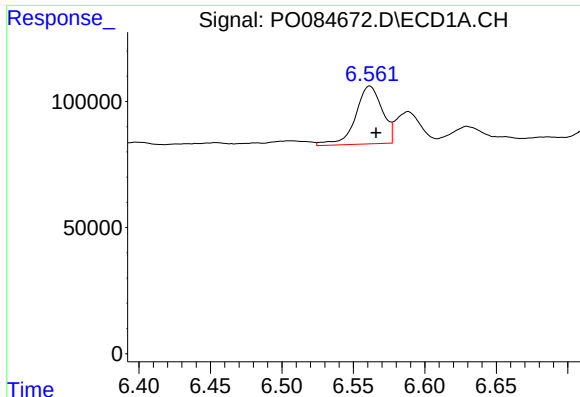


#26 AR-1254-1

R.T.: 6.562 min
Delta R.T.: -0.004 min
Response: 298270
Conc: 46.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-55A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/16/2022
Supervised By :Ankita Jodhani 02/16/2022

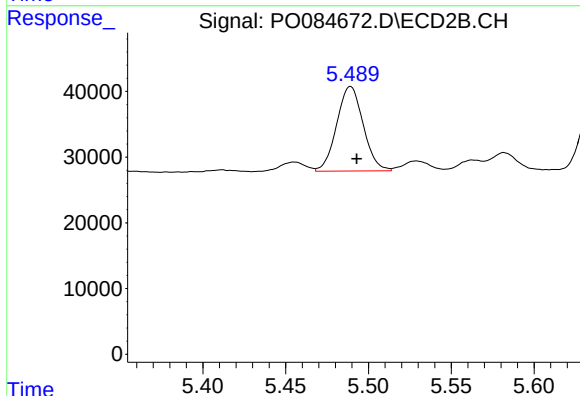


#26 AR-1254-1

R.T.: 5.489 min
Delta R.T.: -0.004 min
Response: 143426
Conc: 56.04 ng/ml

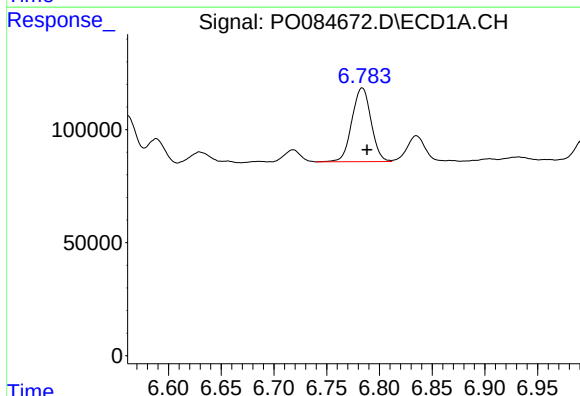


#27 AR-1254-2

R.T.: 6.784 min
Delta R.T.: -0.004 min
Response: 411279
Conc: 41.63 ng/ml

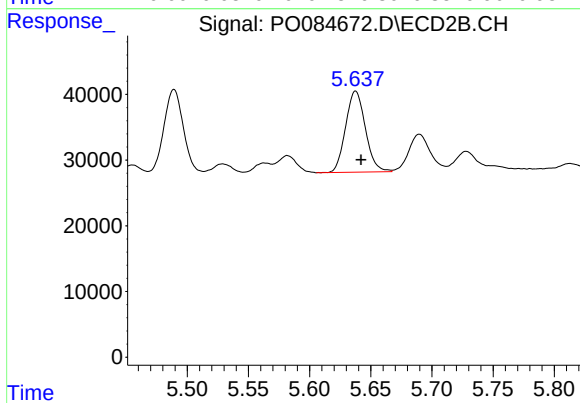

#27 AR-1254-2

R.T.: 5.638 min
Delta R.T.: -0.005 min
Response: 139054
Conc: 62.13 ng/ml

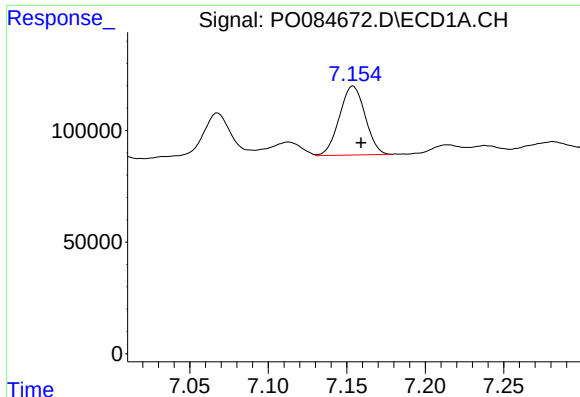


#28 AR-1254-3

R.T.: 7.154 min
Delta R.T.: -0.005 min
Response: 352572
Conc: 34.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-55A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/16/2022
Supervised By :Ankita Jodhani 02/16/2022

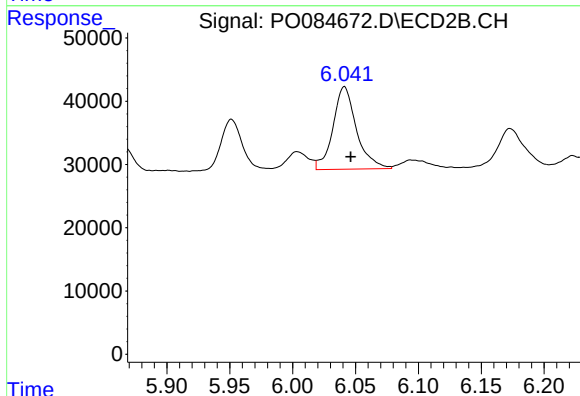


#28 AR-1254-3

R.T.: 6.041 min
Delta R.T.: -0.005 min
Response: 170266
Conc: 46.78 ng/ml

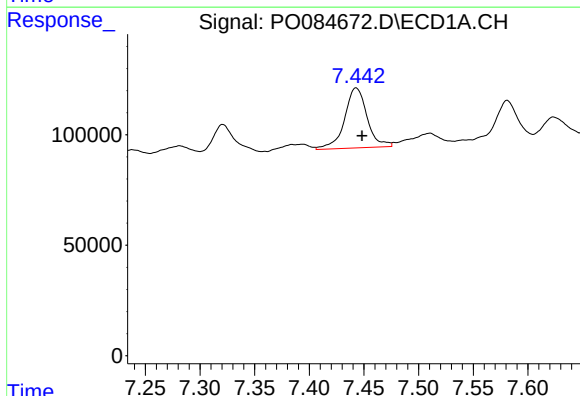


#29 AR-1254-4

R.T.: 7.443 min
Delta R.T.: -0.006 min
Response: 390004
Conc: 53.27 ng/ml

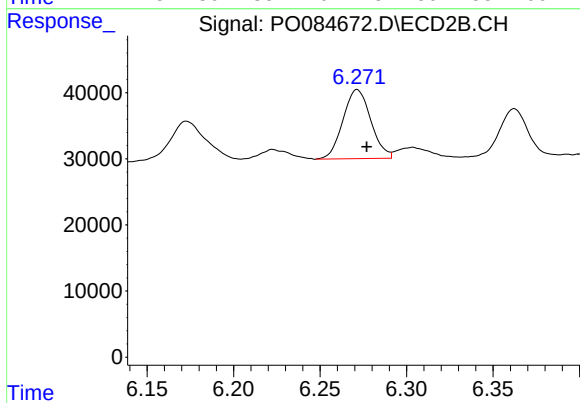

#29 AR-1254-4

R.T.: 6.271 min
Delta R.T.: -0.006 min
Response: 116696
Conc: 51.94 ng/ml

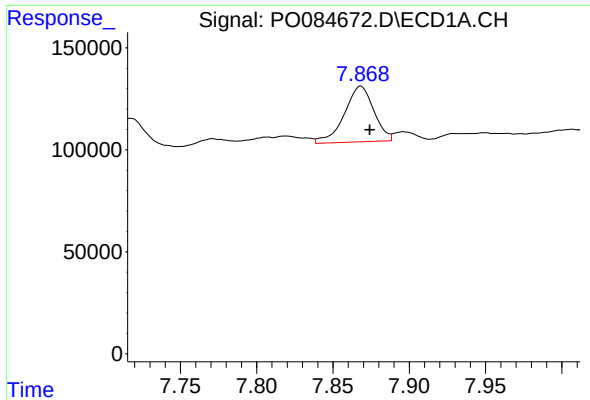


#30 AR-1254-5

R.T.: 7.868 min
Delta R.T.: -0.006 min
Response: 367459
Conc: 45.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-55A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/16/2022
Supervised By :Ankita Jodhani 02/16/2022

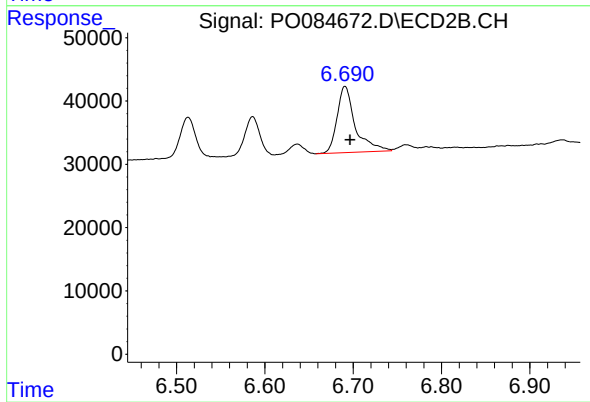

#30 AR-1254-5

R.T.: 6.691 min
Delta R.T.: -0.006 min
Response: 149629
Conc: 45.77 ng/ml