

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021522\
 Data File : P0084677.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Feb 2022 22:43
 Operator : YP\AJ
 Sample : N1537-16 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2022-58A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 00:42:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.504	3.594	260276	71442	1.324	1.584
2) SA Decachlor...	10.420	8.618	193880	53637	1.562	1.471

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021522\
Data File : P0084677.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Feb 2022 22:43
Operator : YP\AJ
Sample : N1537-16 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2022-58A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 00:42:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

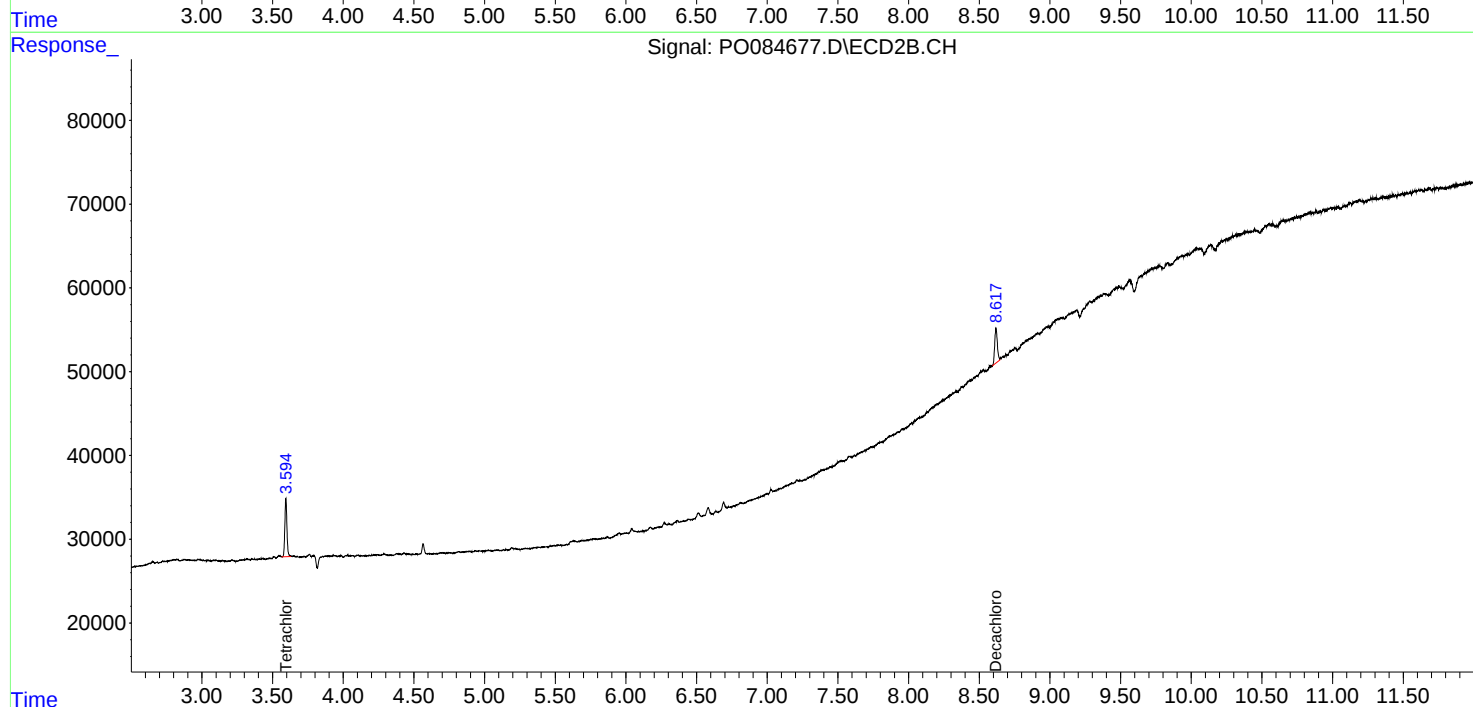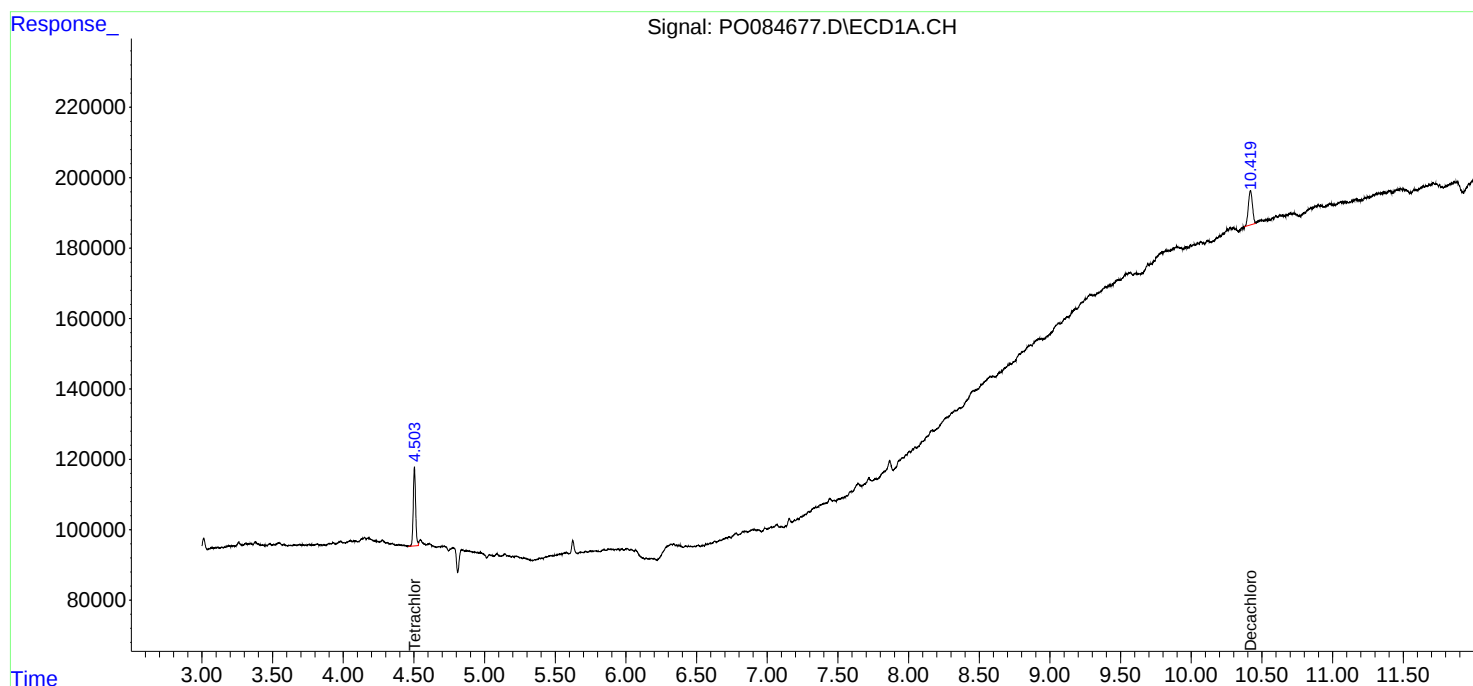


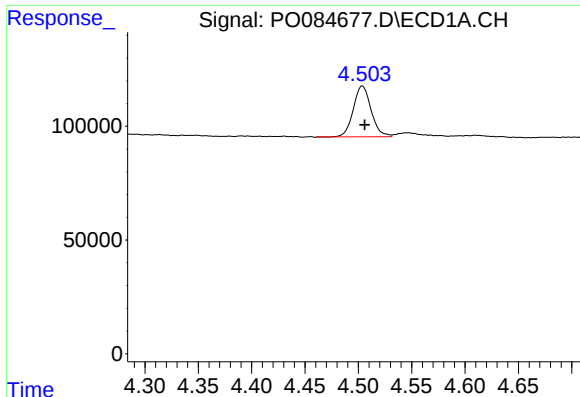

#1 Tetrachloro-m-xylene


R.T.: 4.504 min
Delta R.T.: -0.002 min
Response: 260276
Conc: 1.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2022-58A

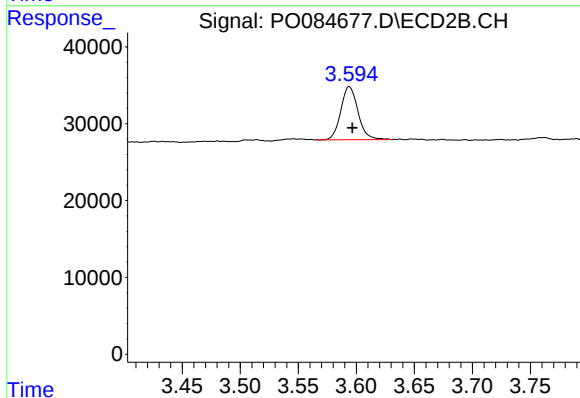


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: -0.003 min
Response: 71442
Conc: 1.58 ng/ml

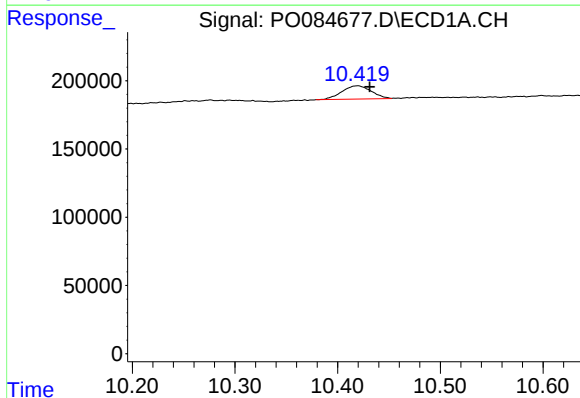

#2 Decachlorobiphenyl

R.T.: 10.420 min
Delta R.T.: -0.012 min
Response: 193880
Conc: 1.56 ng/ml

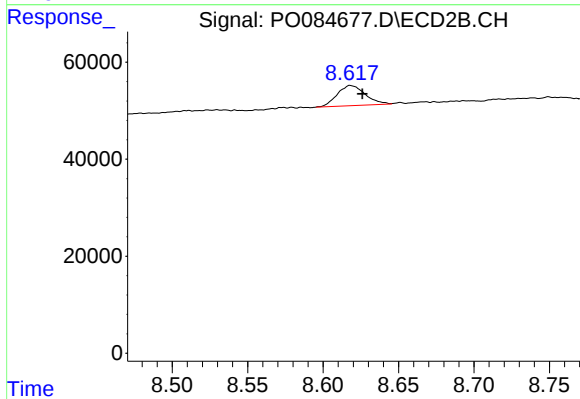

#2 Decachlorobiphenyl

R.T.: 8.618 min
Delta R.T.: -0.008 min
Response: 53637
Conc: 1.47 ng/ml