

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021524\
 Data File : P0101824.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Feb 2024 18:28
 Operator : YP/AJ
 Sample : P1486-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3418-3419

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/16/2024
 Supervised By :Ankita Jodhani 02/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 04:00:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.286	3.397	57501614	53049901	18.648m	19.958
2) SA Decachlor...	9.844	8.278	47271489	31990352	22.543	16.838 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021524\
Data File : PO101824.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Feb 2024 18:28
Operator : YP/AJ
Sample : P1486-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3418-3419


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/16/2024
Supervised By :Ankita Jodhani 02/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 04:00:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

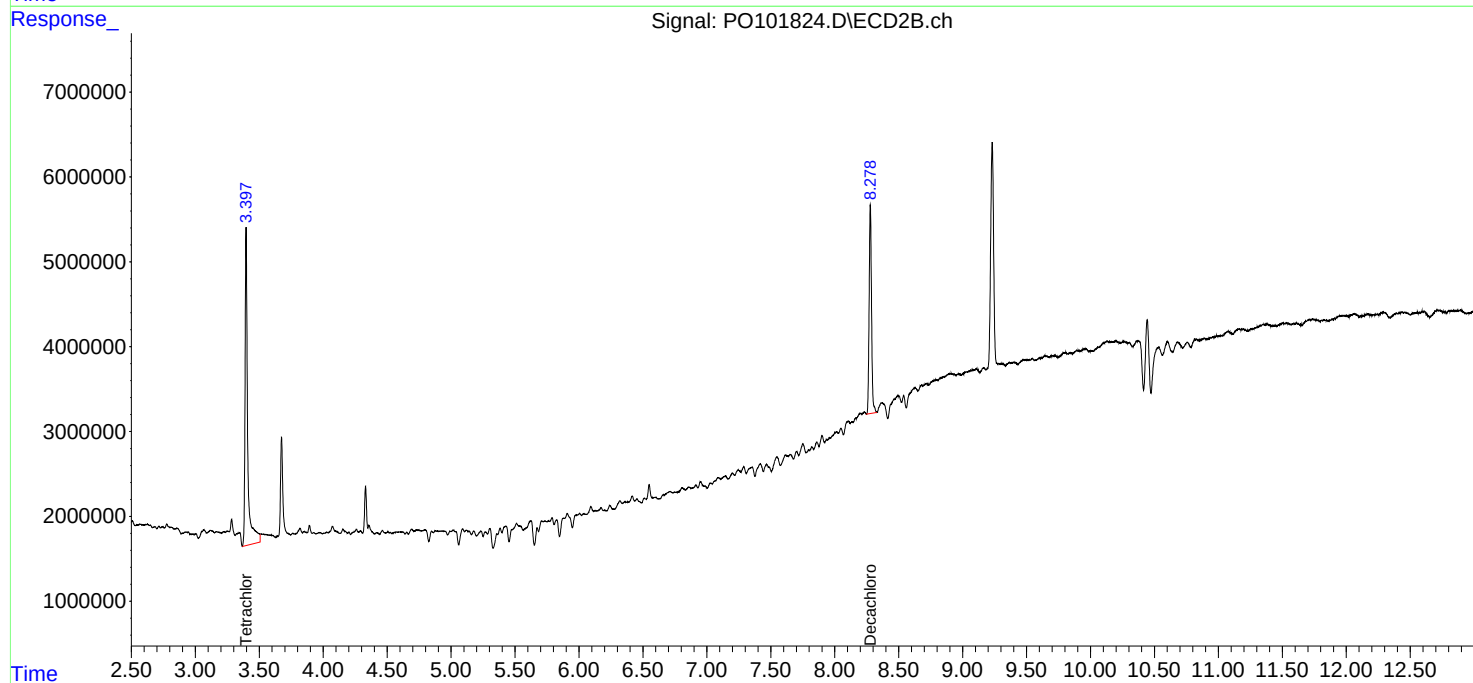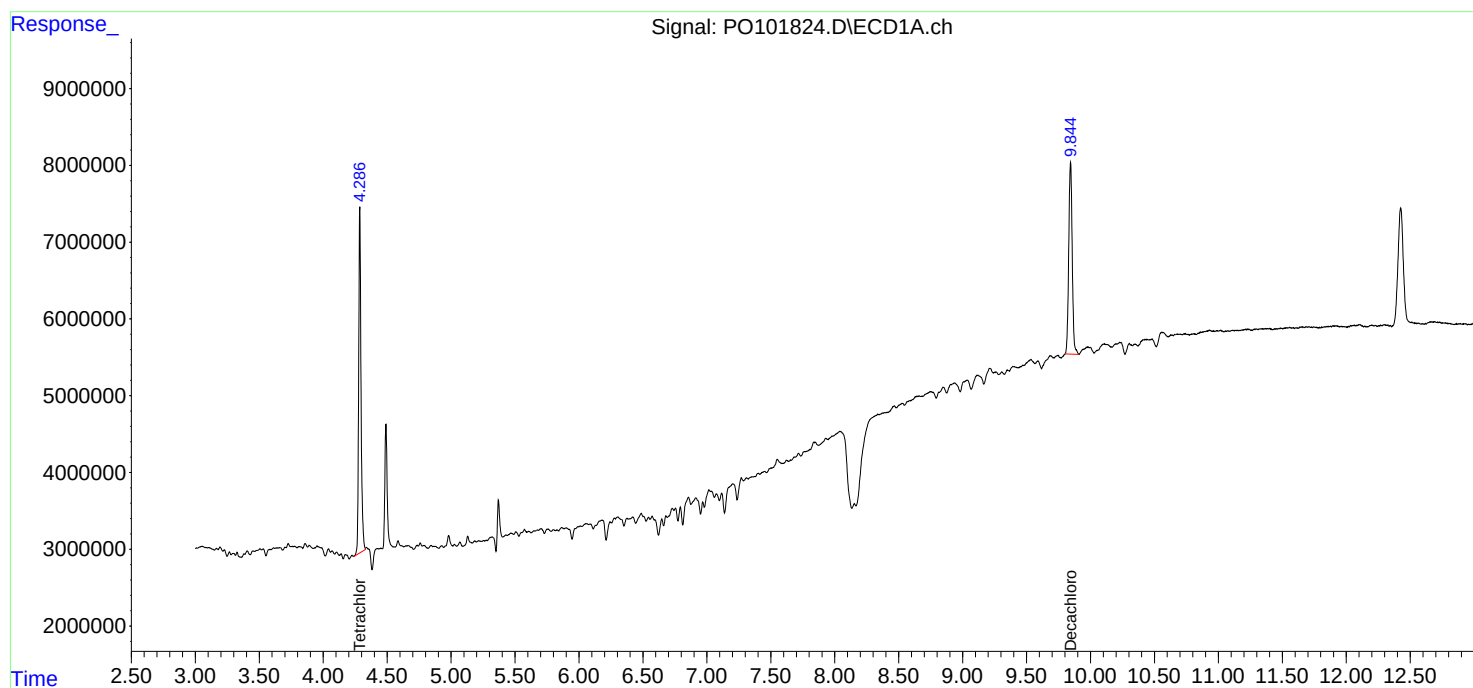

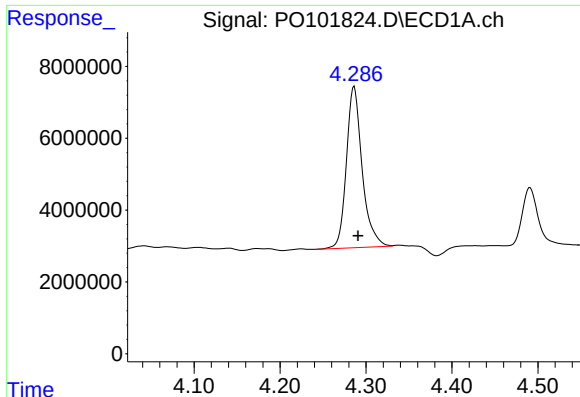


#1 Tetrachloro-m-xylene

R.T.: 4.286 min
Delta R.T.: -0.005 min
Response: 57501614
Conc: 18.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
3418-3419


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/16/2024
Supervised By :Ankita Jodhani 02/16/2024

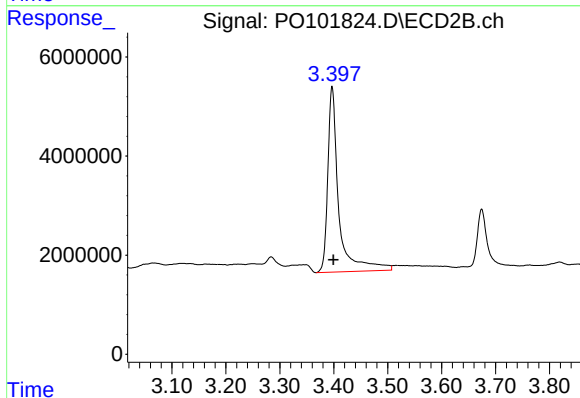


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: -0.003 min
Response: 53049901
Conc: 19.96 ng/ml

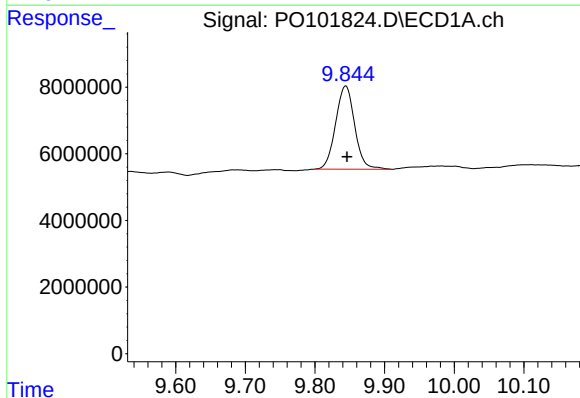

#2 Decachlorobiphenyl

R.T.: 9.844 min
Delta R.T.: -0.002 min
Response: 47271489
Conc: 22.54 ng/ml

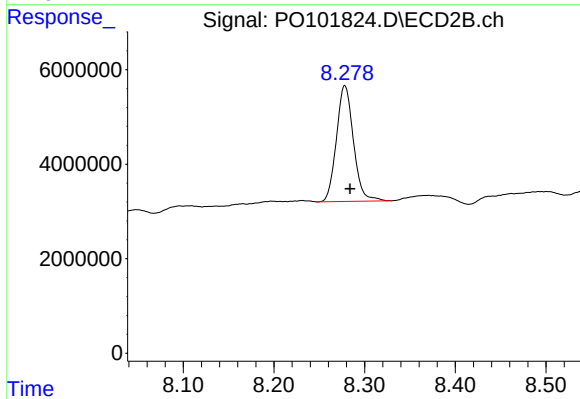

#2 Decachlorobiphenyl

R.T.: 8.278 min
Delta R.T.: -0.006 min
Response: 31990352
Conc: 16.84 ng/ml