

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021622\
 Data File : P0084707.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Feb 2022 17:27
 Operator : YP\AJ
 Sample : N1553-11 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LAW-2022-06A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 04:47:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.506	3.596	164454	60508	0.836	1.342 #
2) SA Decachlor...	10.425	8.623	184154	44655	1.484	1.225
Target Compounds						
31) L7 AR-1260-1	7.324	6.175	7117139	2421210	1028.387	999.266
32) L7 AR-1260-2	7.583	6.365	7585327	2510313	927.952	866.641
33) L7 AR-1260-3	7.948	6.518	5177539	2517683	843.781	925.197
34) L7 AR-1260-4	8.178	6.992	6127161	1805666	877.904	784.686
35) L7 AR-1260-5	8.511	7.236	11074528	3496378	804.630	660.490



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021622\
Data File : P0084707.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Feb 2022 17:27
Operator : YP\AJ
Sample : N1553-11 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LAW-2022-06A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 04:47:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

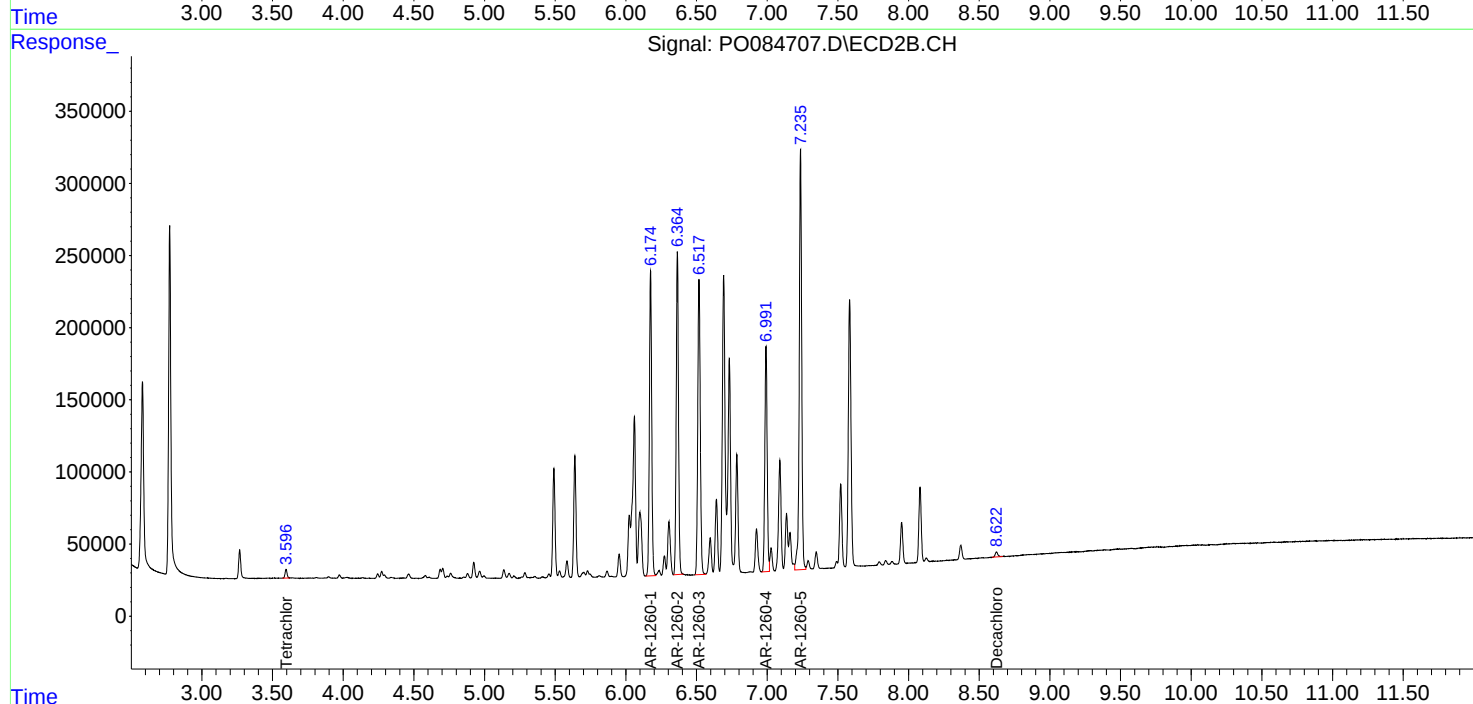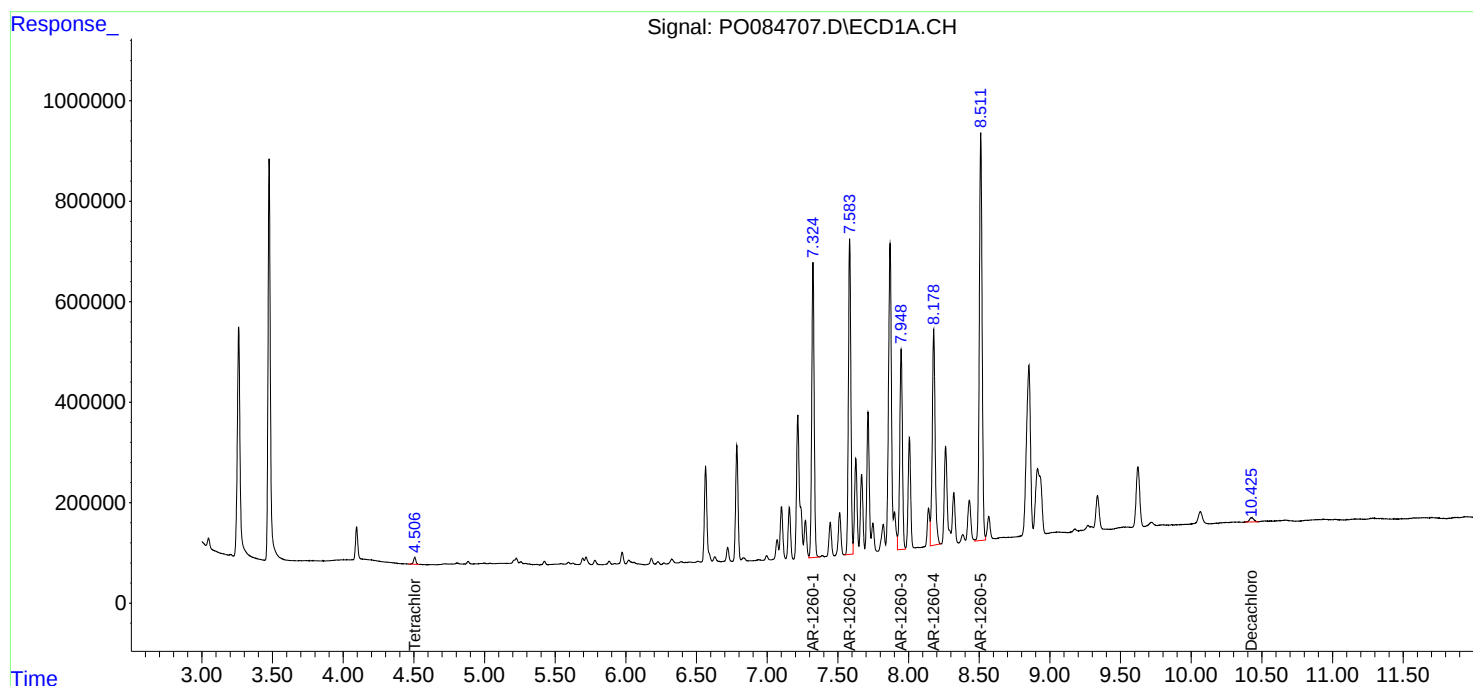


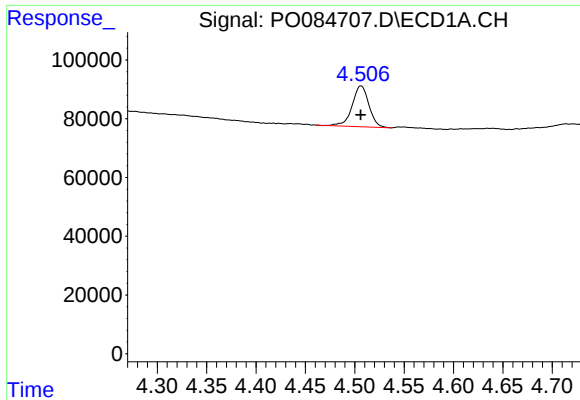

#1 Tetrachloro-m-xylene


R.T.: 4.506 min
Delta R.T.: 0.000 min
Response: 164454
Conc: 0.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2022-06A

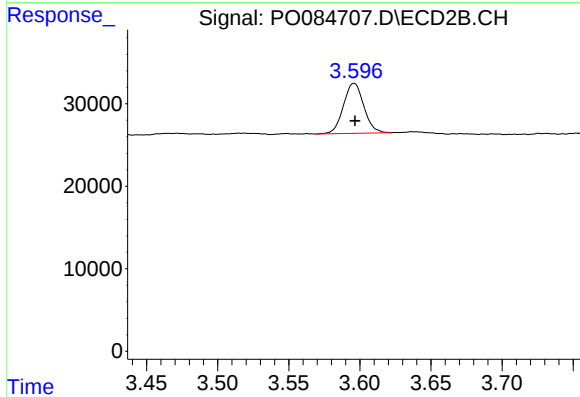


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: 0.000 min
Response: 60508
Conc: 1.34 ng/ml

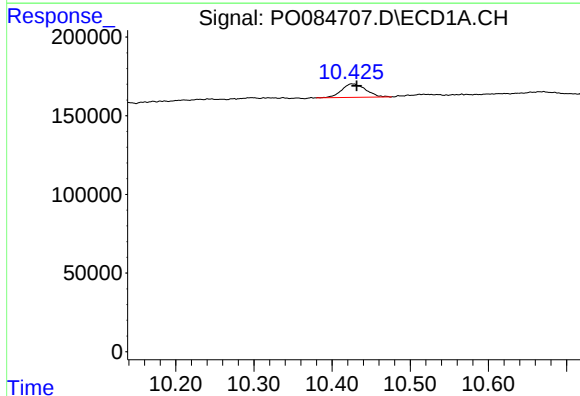


#2 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: -0.006 min
Response: 184154
Conc: 1.48 ng/ml

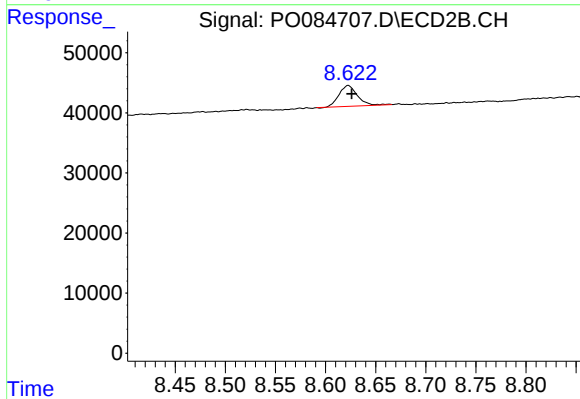

#2 Decachlorobiphenyl


R.T.: 8.623 min
Delta R.T.: -0.003 min
Response: 44655
Conc: 1.22 ng/ml

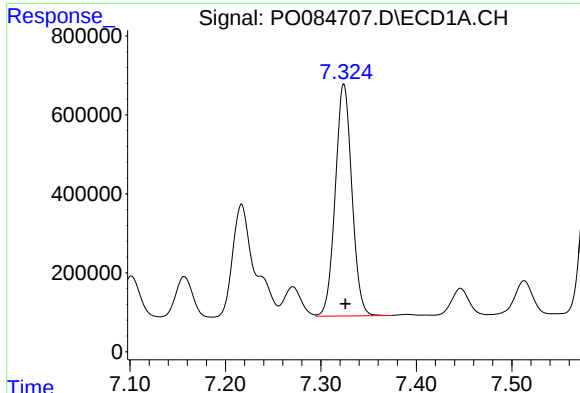

#31 AR-1260-1


R.T.: 7.324 min
Delta R.T.: -0.002 min
Response: 7117139
Conc: 1028.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2022-06A

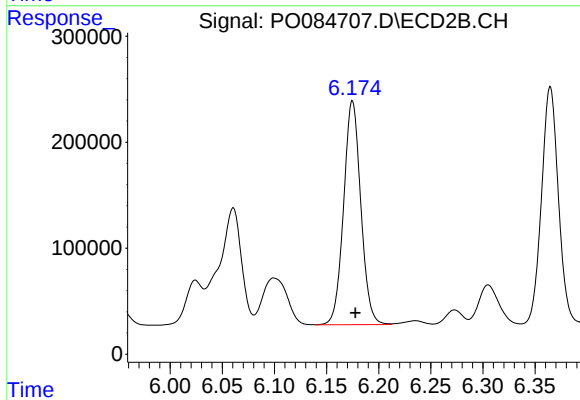


#31 AR-1260-1

R.T.: 6.175 min
Delta R.T.: -0.003 min
Response: 2421210
Conc: 999.27 ng/ml

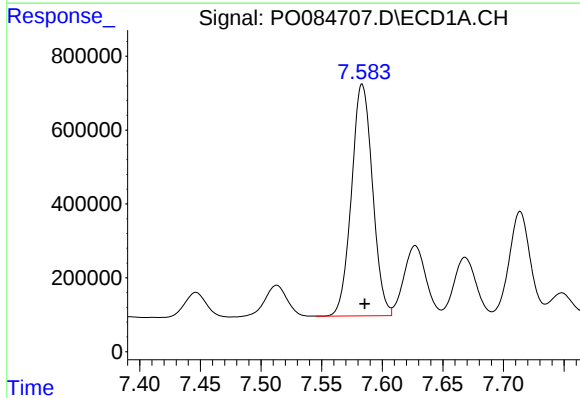


#32 AR-1260-2

R.T.: 7.583 min
Delta R.T.: -0.002 min
Response: 7585327
Conc: 927.95 ng/ml

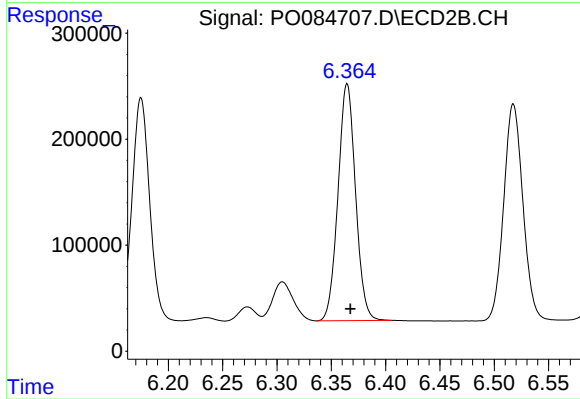

#32 AR-1260-2


R.T.: 6.365 min
Delta R.T.: -0.003 min
Response: 2510313
Conc: 866.64 ng/ml

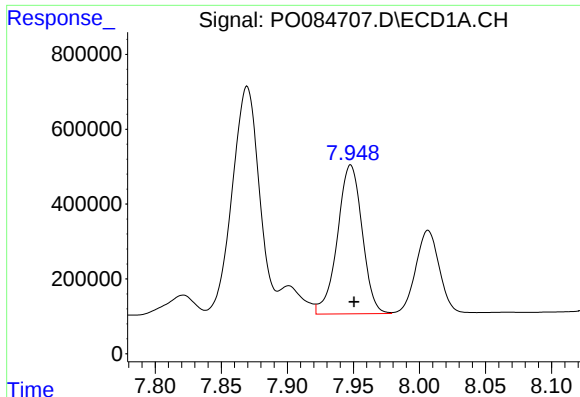

#33 AR-1260-3


R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 5177539
Conc: 843.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2022-06A

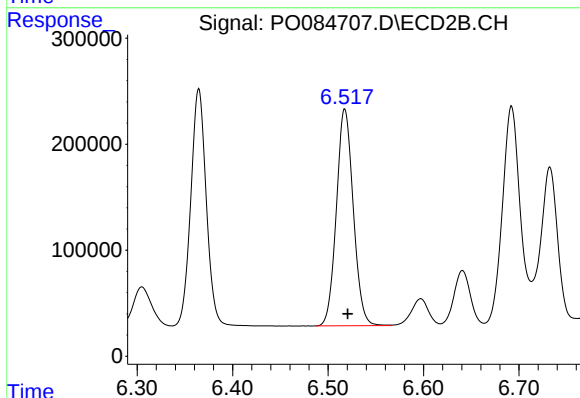


#33 AR-1260-3

R.T.: 6.518 min
Delta R.T.: -0.003 min
Response: 2517683
Conc: 925.20 ng/ml

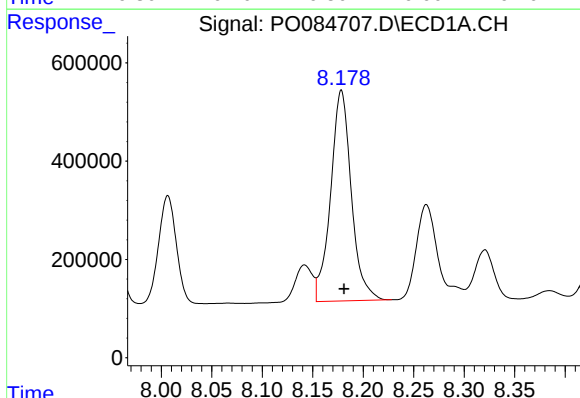


#34 AR-1260-4

R.T.: 8.178 min
Delta R.T.: -0.003 min
Response: 6127161
Conc: 877.90 ng/ml

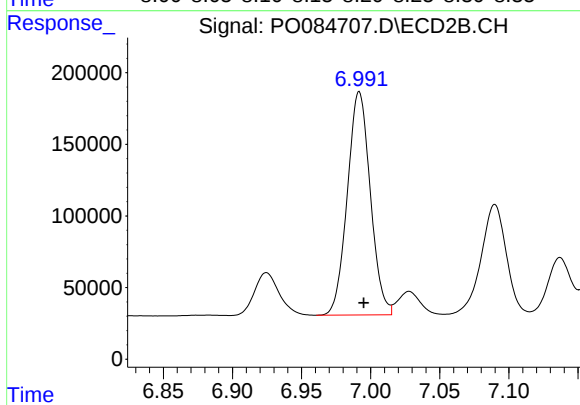

#34 AR-1260-4


R.T.: 6.992 min
Delta R.T.: -0.003 min
Response: 1805666
Conc: 784.69 ng/ml

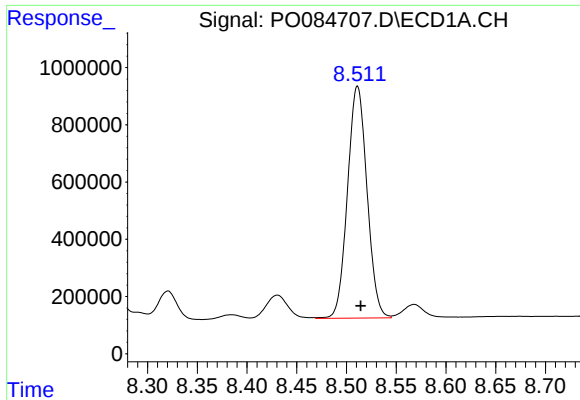

#35 AR-1260-5

R.T.: 8.511 min
Delta R.T.: -0.003 min
Response: 11074528
Conc: 804.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2022-06A

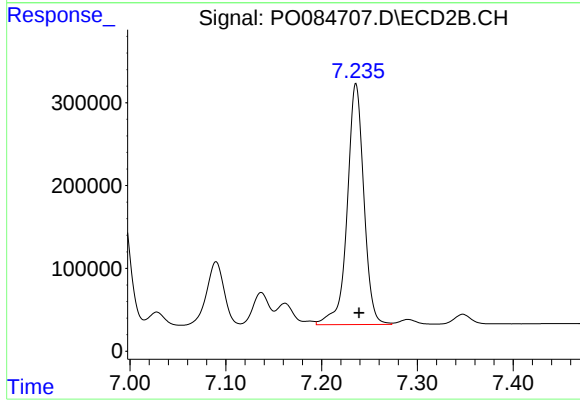

#35 AR-1260-5

R.T.: 7.236 min
Delta R.T.: -0.003 min
Response: 3496378
Conc: 660.49 ng/ml