

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021622\
Data File : P0084714.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Feb 2022 19:18
Operator : YP\AJ
Sample : N1553-18 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LAW-2022-09B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 04:51:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.506	3.596	205906	69564	1.047	1.542 #
2) SA Decachlor...	10.426	8.620	237774	63271	1.916	1.736

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021622\
Data File : P0084714.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Feb 2022 19:18
Operator : YP\AJ
Sample : N1553-18 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LAW-2022-09B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 04:51:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

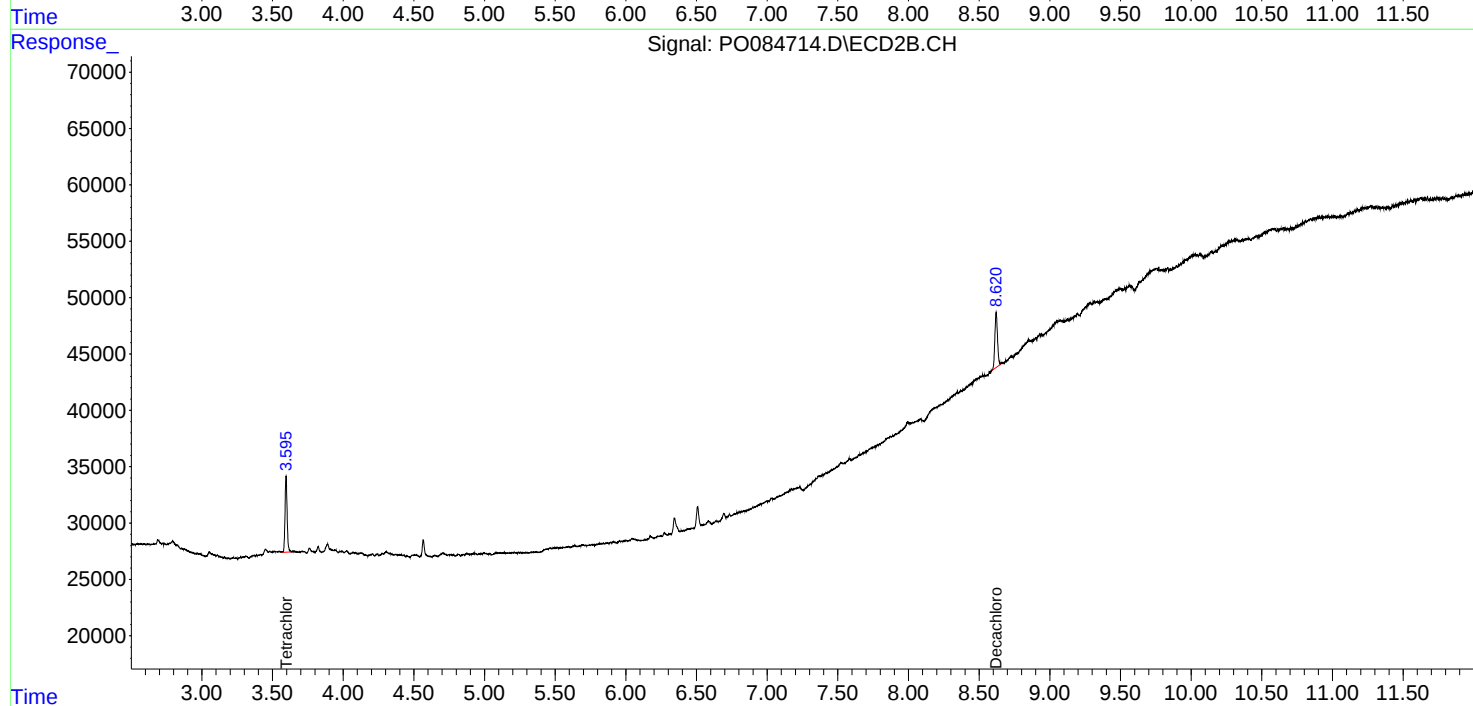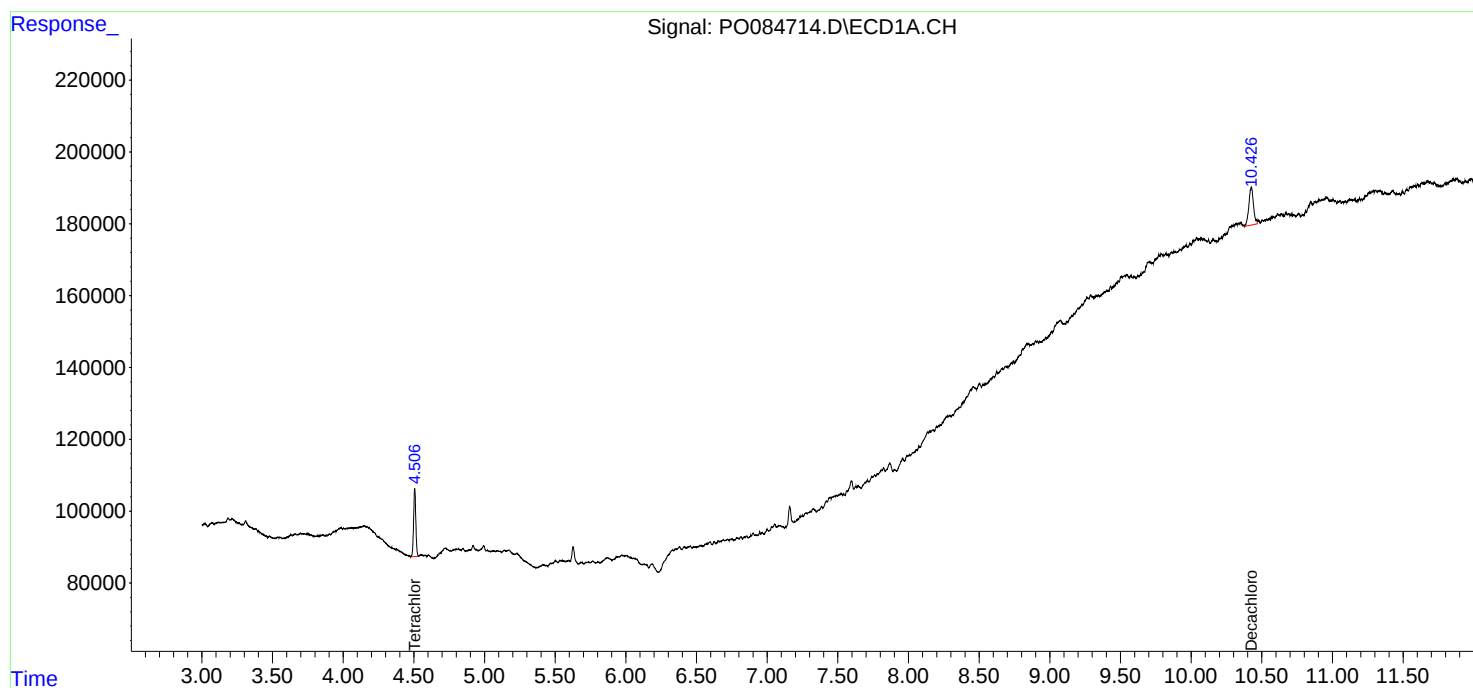


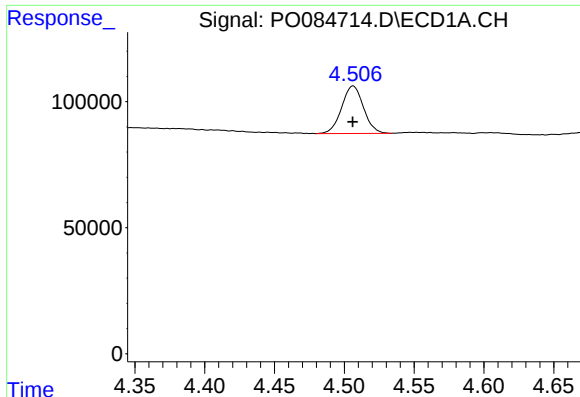

#1 Tetrachloro-m-xylene


R.T.: 4.506 min
Delta R.T.: 0.000 min
Response: 205906
Conc: 1.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2022-09B

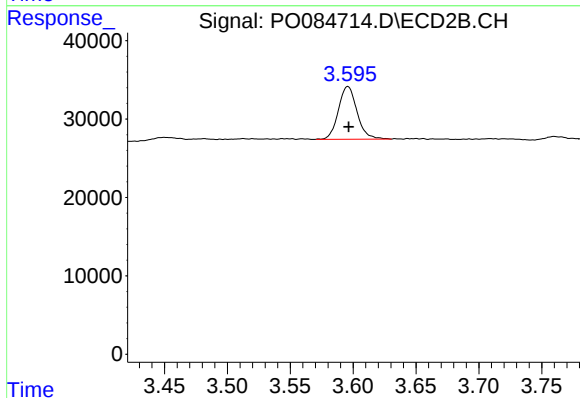


#1 Tetrachloro-m-xylene

R.T.: 3.596 min
Delta R.T.: 0.000 min
Response: 69564
Conc: 1.54 ng/ml

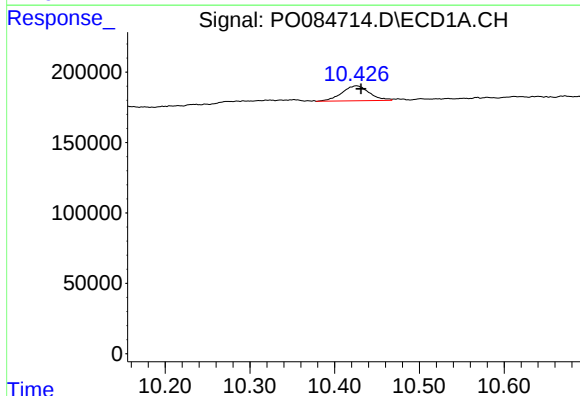

#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.005 min
Response: 237774
Conc: 1.92 ng/ml

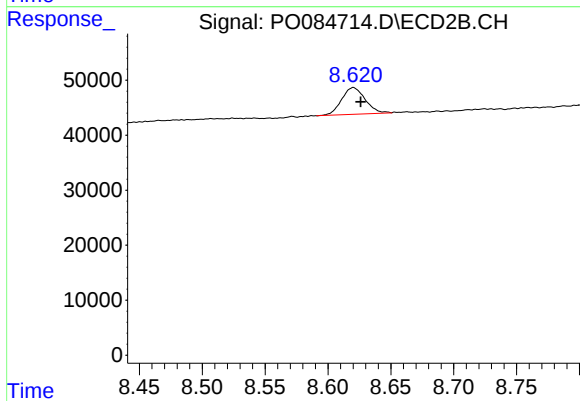

#2 Decachlorobiphenyl

R.T.: 8.620 min
Delta R.T.: -0.006 min
Response: 63271
Conc: 1.74 ng/ml