

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021623\
 Data File : P0092478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2023 11:01
 Operator : YP/AJ
 Sample : 01552-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-01-4.0-6.0

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
 Supervised By :Sohil Jodhani 02/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 20:33:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.645	53990034	25069321	18.650	17.854m
2) SA Decachlor...	10.374	8.686	47368893	21283704	22.951	18.853
Target Compounds						
31) L7 AR-1260-1	7.273	6.242	23822887	32594660	180.811	431.491 #
32) L7 AR-1260-2	7.533	6.410	36658789	10495764	247.216	119.796 #
33) L7 AR-1260-3	7.906	6.566	22557858	8299524	199.163	95.739 #
34) L7 AR-1260-4	8.137	7.040	23012206	9345750	185.635	139.556
35) L7 AR-1260-5	8.470	7.283	40947843	20636738	184.402	145.022

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021623\
Data File : PO092478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2023 11:01
Operator : YP/AJ
Sample : 01552-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-01-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 20:33:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

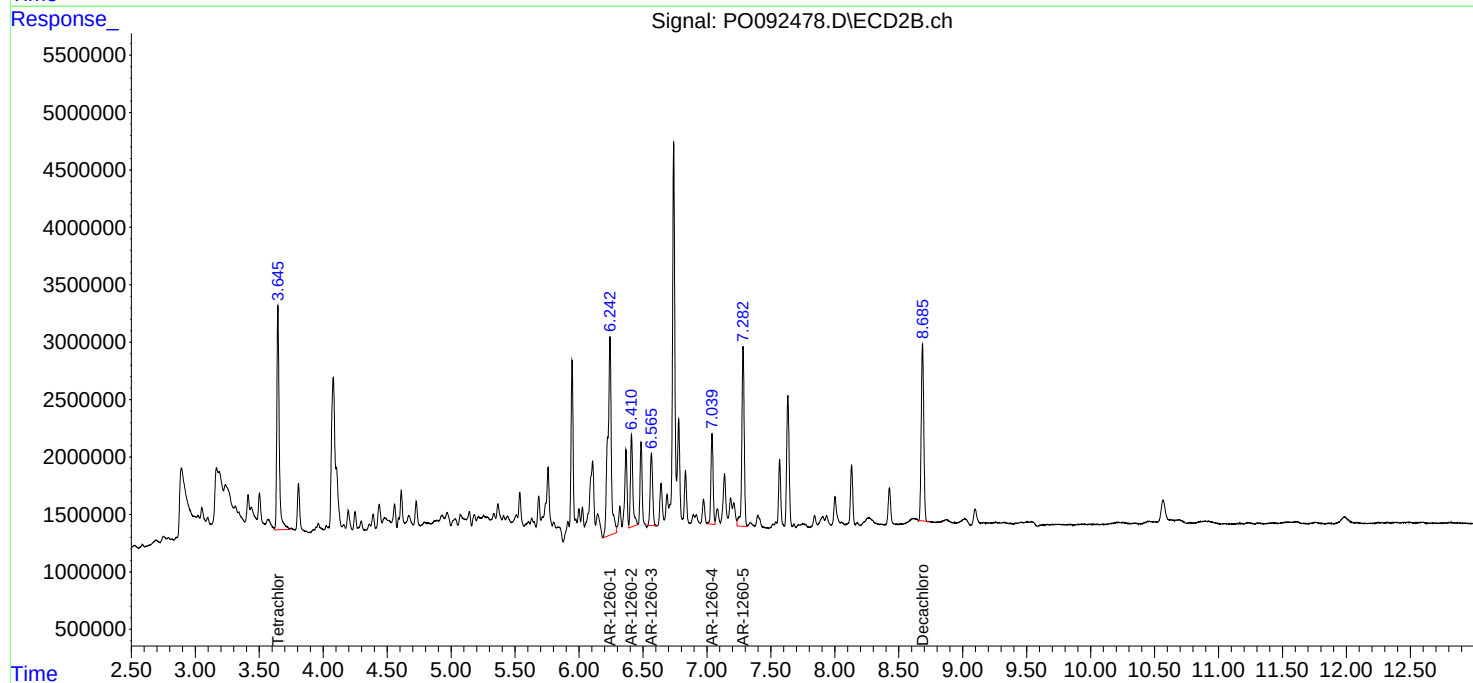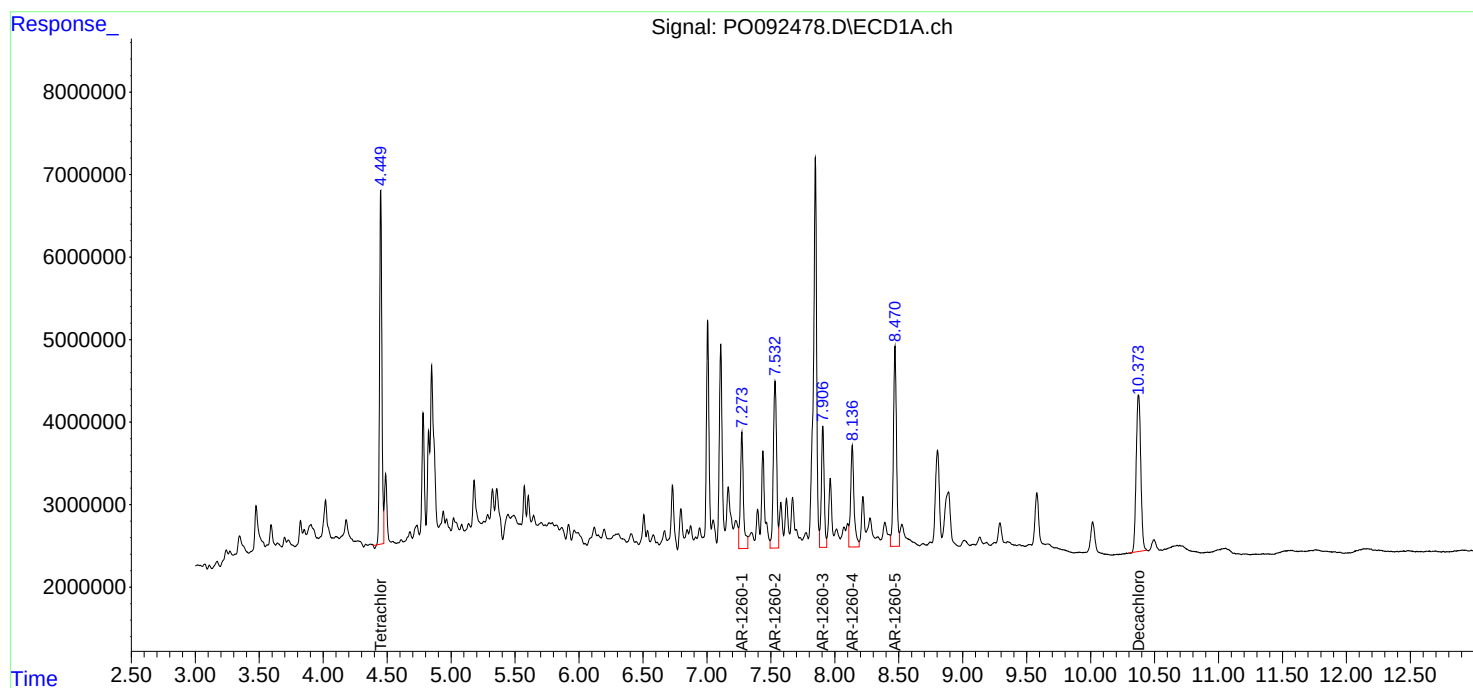

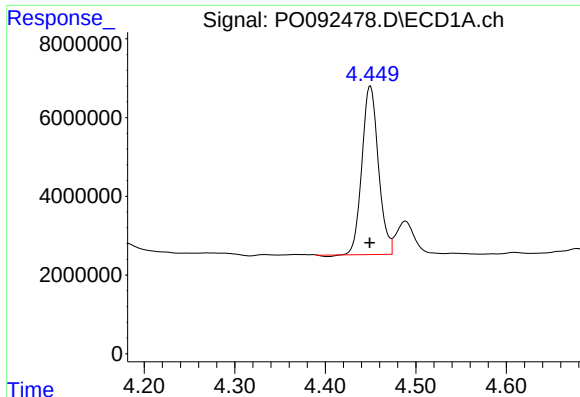


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: 0.000 min
Response: 53990034
Conc: 18.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

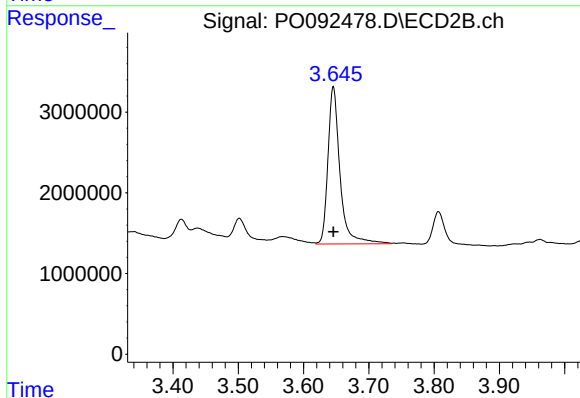


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 25069321
Conc: 17.85 ng/ml m

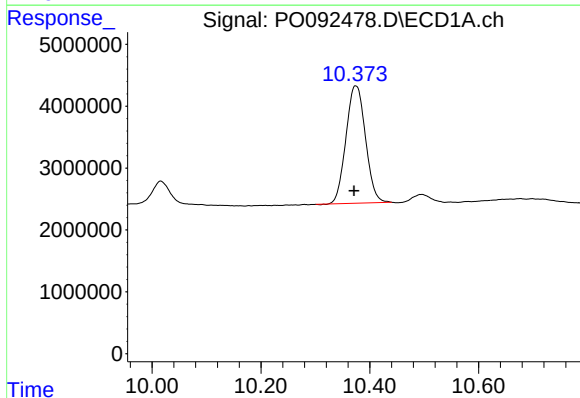


#2 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: 0.003 min
Response: 47368893
Conc: 22.95 ng/ml

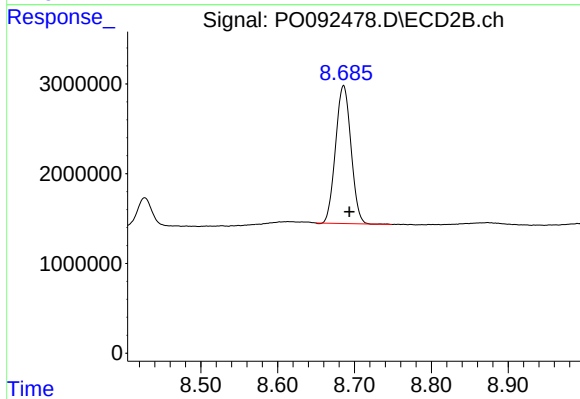

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: -0.007 min
Response: 21283704
Conc: 18.85 ng/ml

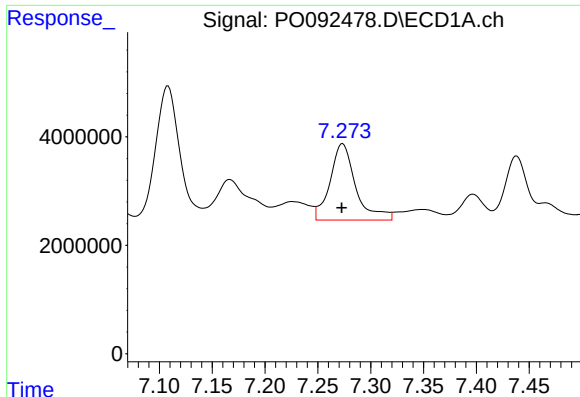


#31 AR-1260-1

R.T.: 7.273 min
Delta R.T.: 0.000 min
Response: 23822887
Conc: 180.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

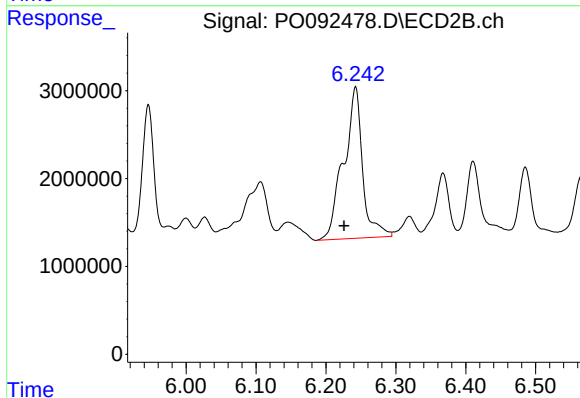


#31 AR-1260-1

R.T.: 6.242 min
Delta R.T.: 0.016 min
Response: 32594660
Conc: 431.49 ng/ml

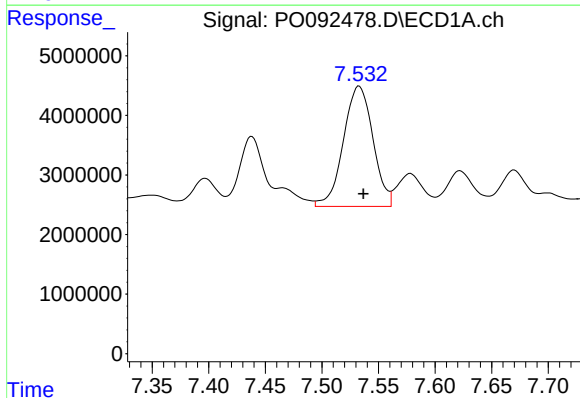


#32 AR-1260-2

R.T.: 7.533 min
Delta R.T.: -0.004 min
Response: 36658789
Conc: 247.22 ng/ml

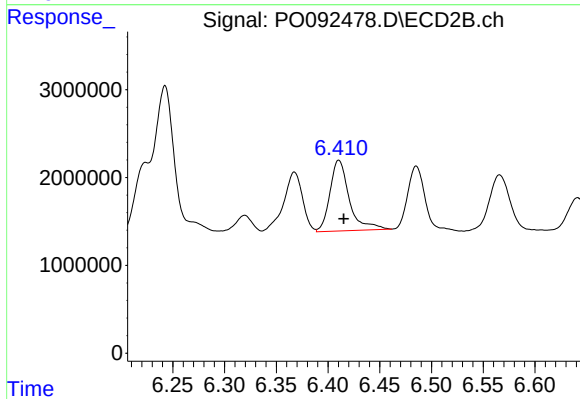

#32 AR-1260-2

R.T.: 6.410 min
Delta R.T.: -0.005 min
Response: 10495764
Conc: 119.80 ng/ml

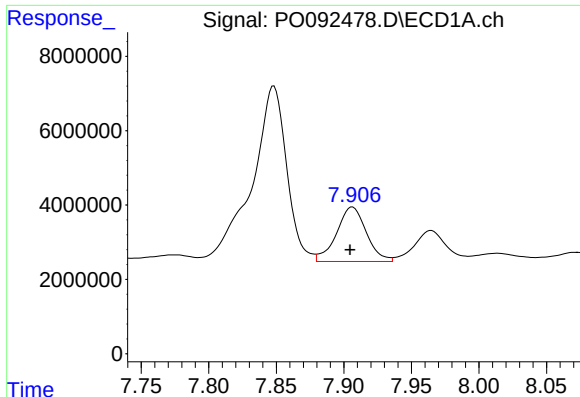


#33 AR-1260-3

R.T.: 7.906 min
Delta R.T.: 0.002 min
Response: 22557858
Conc: 199.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

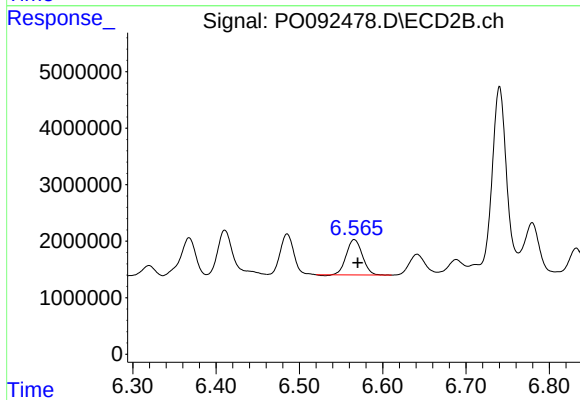


#33 AR-1260-3

R.T.: 6.566 min
Delta R.T.: -0.004 min
Response: 8299524
Conc: 95.74 ng/ml

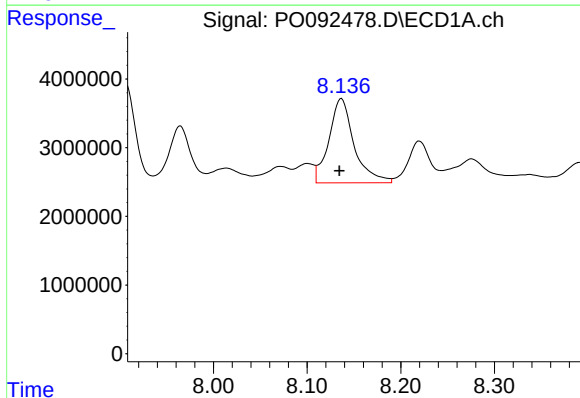


#34 AR-1260-4

R.T.: 8.137 min
Delta R.T.: 0.002 min
Response: 23012206
Conc: 185.63 ng/ml

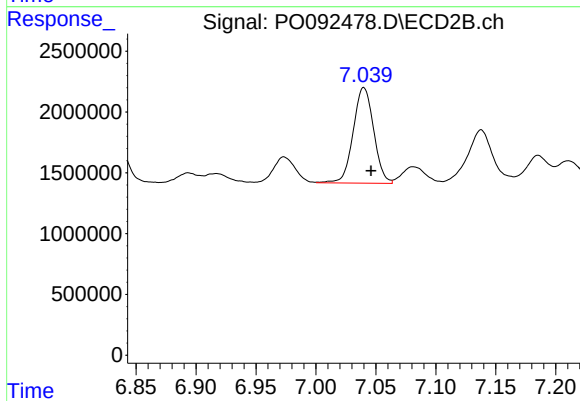

#34 AR-1260-4

R.T.: 7.040 min
Delta R.T.: -0.006 min
Response: 9345750
Conc: 139.56 ng/ml

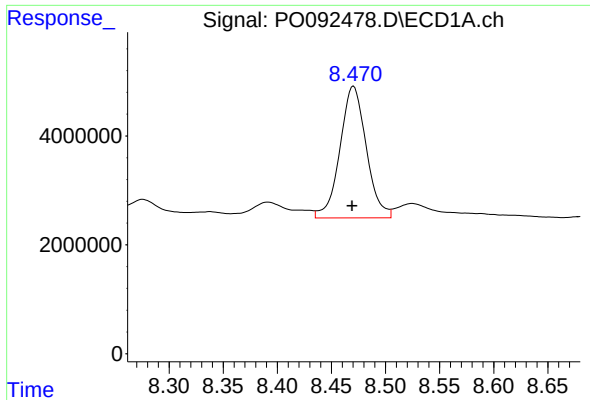


#35 AR-1260-5

R.T.: 8.470 min
Delta R.T.: 0.001 min
Response: 40947843
Conc: 184.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-4.0-6.0

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

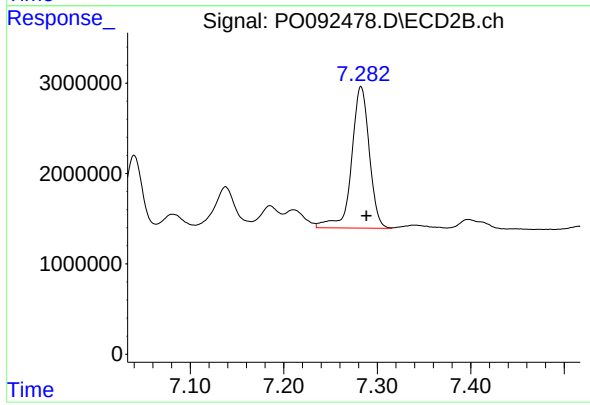

#35 AR-1260-5

R.T.: 7.283 min
Delta R.T.: -0.006 min
Response: 20636738
Conc: 145.02 ng/ml