

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021623\
 Data File : P0092499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2023 17:32
 Operator : YP/AJ
 Sample : 01552-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-02-0-2.0

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
 Supervised By :Sohil Jodhani 02/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 16 20:59:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.646	50814573	24495186	17.553	17.445
2) SA Decachlor...	10.374	8.685	46467073	20355176	22.514	18.031
Target Compounds						
31) L7 AR-1260-1	7.273	6.220	6722073	2641135	51.019	34.964m#
32) L7 AR-1260-2	7.528	6.410	13534787	3355325	91.274	38.297 #
33) L7 AR-1260-3	7.906	6.564	5159254	2255561	45.551	26.019m#
34) L7 AR-1260-4	8.136	7.039	5625677	2374856	45.381	35.463
35) L7 AR-1260-5	8.470	7.282	9921971	5634289	44.682	39.594

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021623\
Data File : PO092499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2023 17:32
Operator : YP/AJ
Sample : 01552-17
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 16 20:59:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

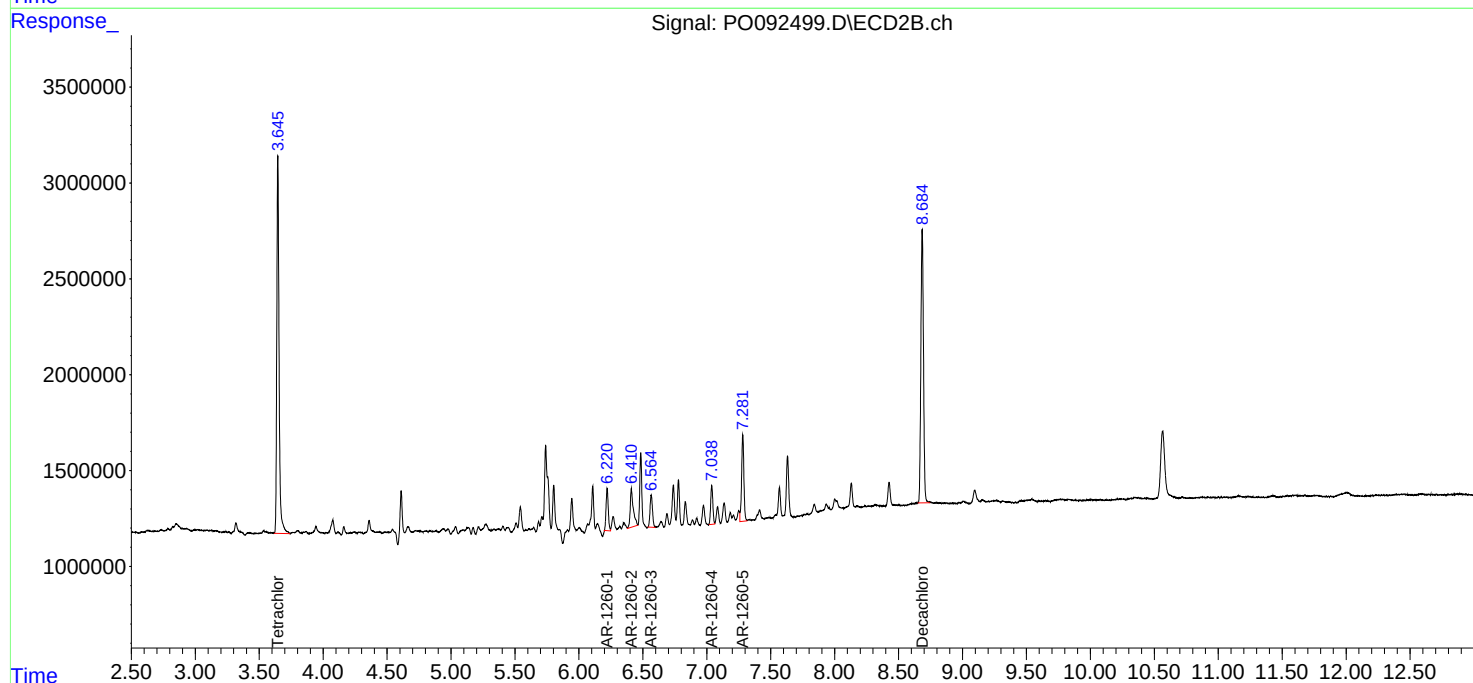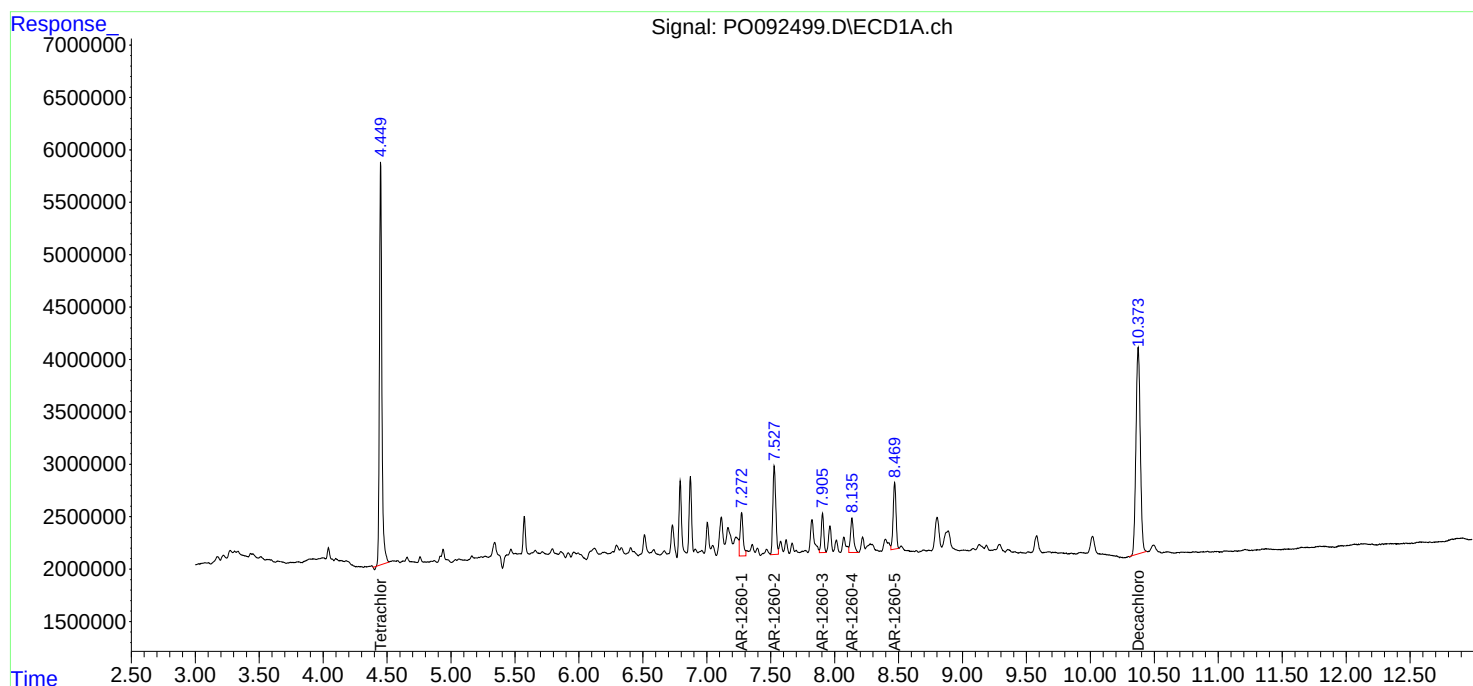

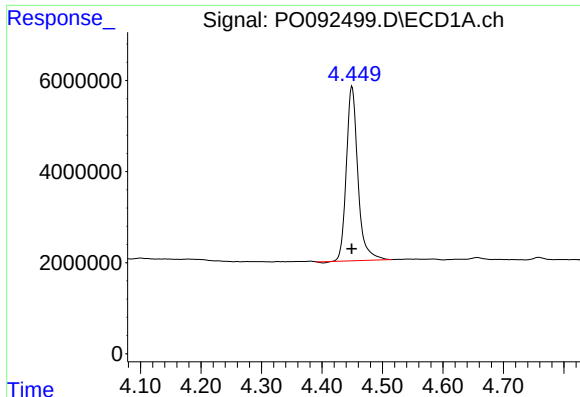


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: 0.000 min
Response: 50814573
Conc: 17.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

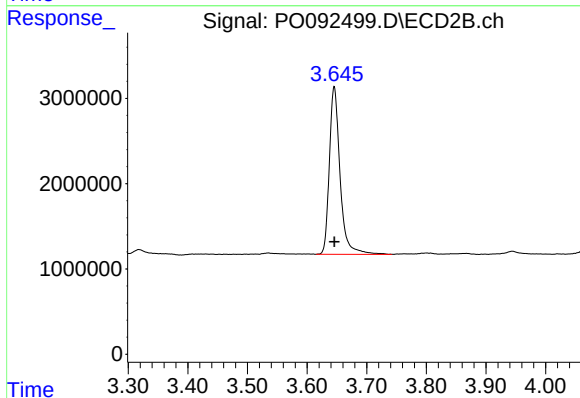


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 24495186
Conc: 17.44 ng/ml

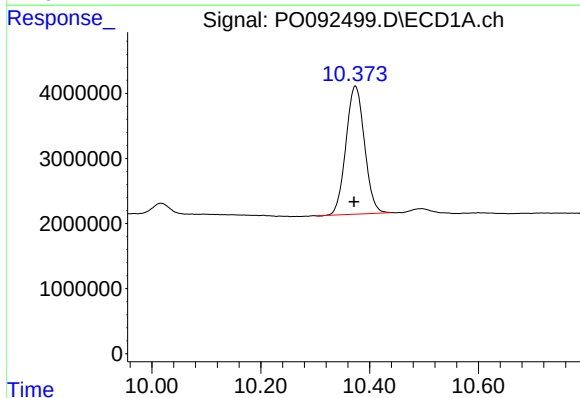


#2 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: 0.003 min
Response: 46467073
Conc: 22.51 ng/ml

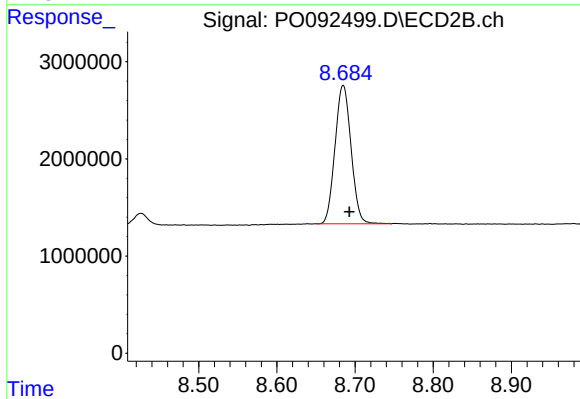

#2 Decachlorobiphenyl

R.T.: 8.685 min
Delta R.T.: -0.008 min
Response: 20355176
Conc: 18.03 ng/ml

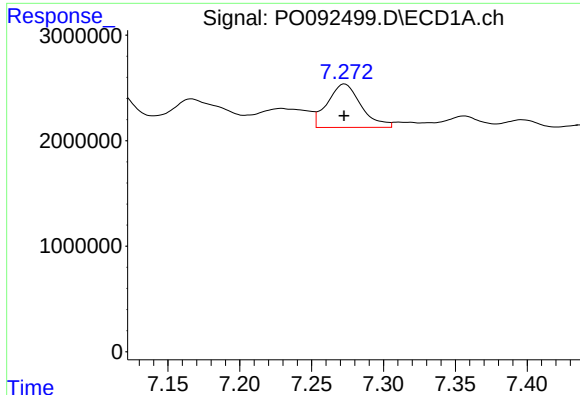


#31 AR-1260-1

R.T.: 7.273 min
Delta R.T.: 0.000 min
Response: 6722073
Conc: 51.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

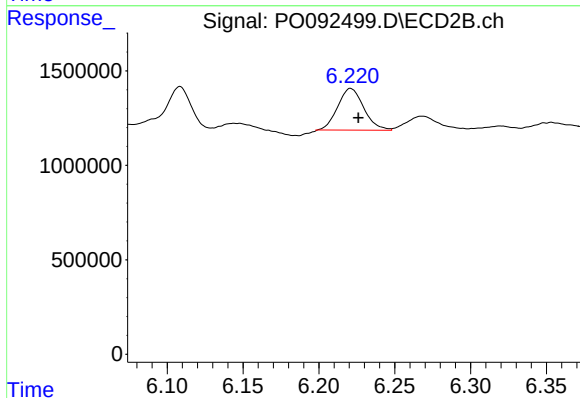


#31 AR-1260-1

R.T.: 6.220 min
Delta R.T.: -0.006 min
Response: 2641135
Conc: 34.96 ng/ml m

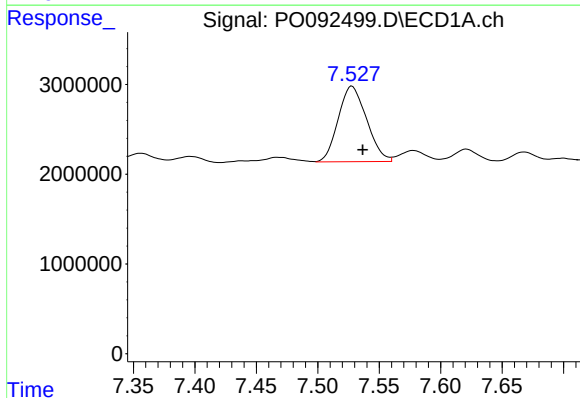


#32 AR-1260-2

R.T.: 7.528 min
Delta R.T.: -0.009 min
Response: 13534787
Conc: 91.27 ng/ml

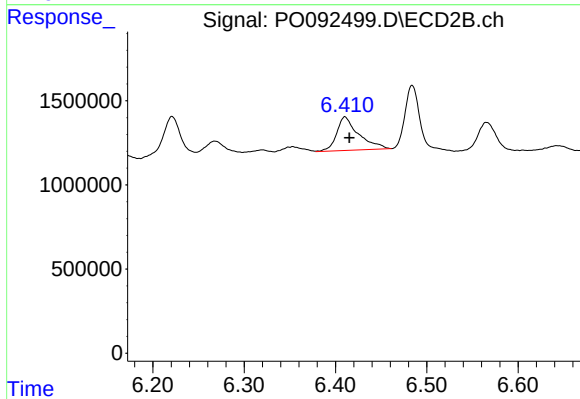

#32 AR-1260-2

R.T.: 6.410 min
Delta R.T.: -0.005 min
Response: 3355325
Conc: 38.30 ng/ml

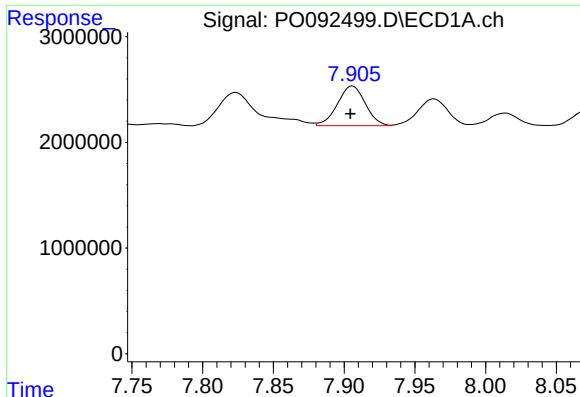


#33 AR-1260-3

R.T.: 7.906 min
Delta R.T.: 0.001 min
Response: 5159254
Conc: 45.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

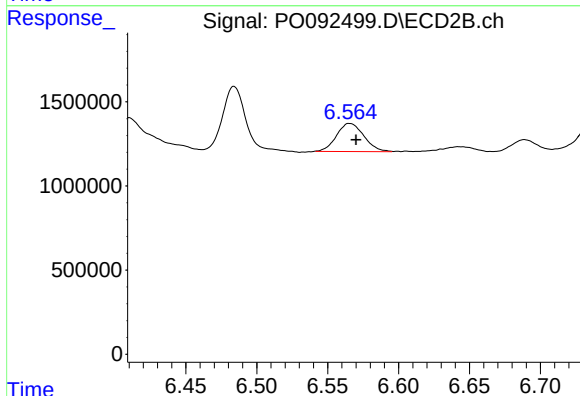


#33 AR-1260-3

R.T.: 6.564 min
Delta R.T.: -0.006 min
Response: 2255561
Conc: 26.02 ng/ml m

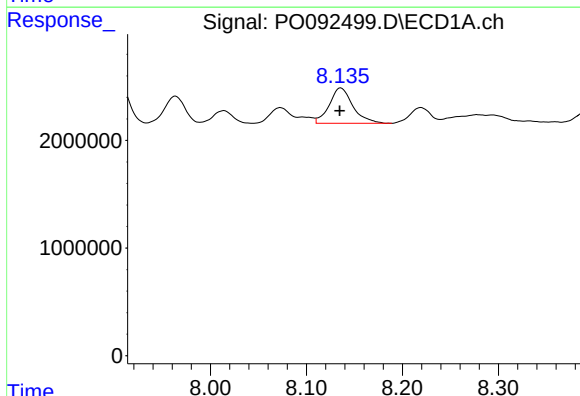


#34 AR-1260-4

R.T.: 8.136 min
Delta R.T.: 0.001 min
Response: 5625677
Conc: 45.38 ng/ml

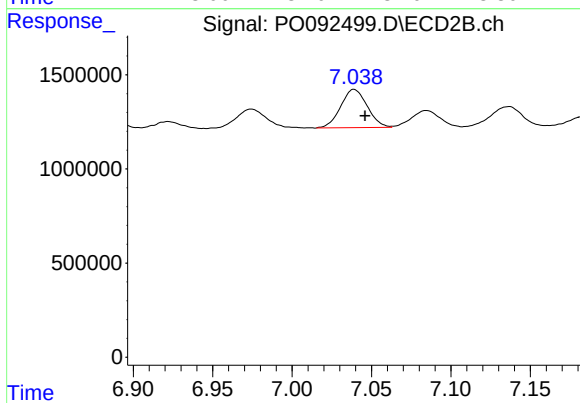

#34 AR-1260-4

R.T.: 7.039 min
Delta R.T.: -0.007 min
Response: 2374856
Conc: 35.46 ng/ml

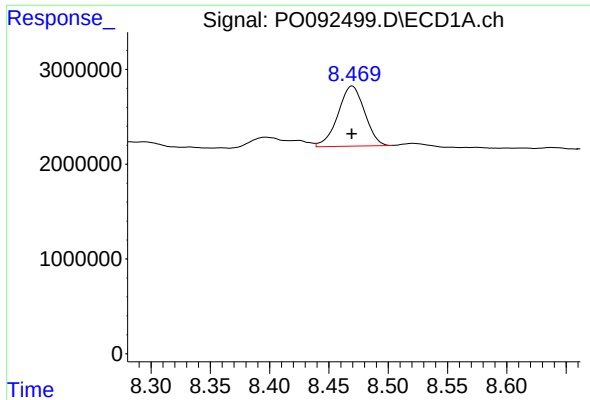


#35 AR-1260-5

R.T.: 8.470 min
Delta R.T.: 0.000 min
Response: 9921971
Conc: 44.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

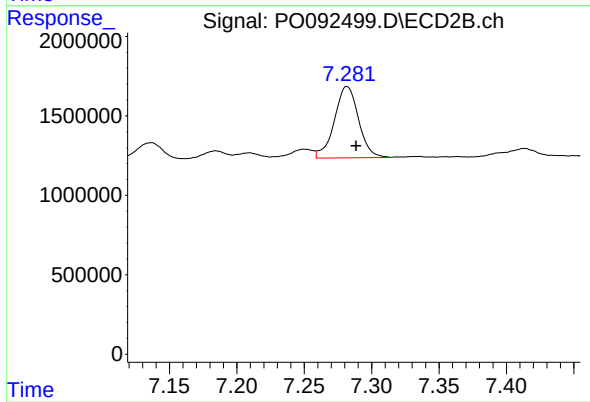

#35 AR-1260-5

R.T.: 7.282 min
Delta R.T.: -0.007 min
Response: 5634289
Conc: 39.59 ng/ml