

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021623\
 Data File : P0092510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Feb 2023 21:39
 Operator : YP/AJ
 Sample : 01570-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-6-021523

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
 Supervised By :Sohil Jodhani 02/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 04:28:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.644	55951361	24905420	19.328	17.737
2) SA Decachlor...	10.375	8.682	41972800	18951584	20.336m	16.788

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021623\
Data File : PO092510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Feb 2023 21:39
Operator : YP/AJ
Sample : 01570-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-6-021523


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 04:28:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

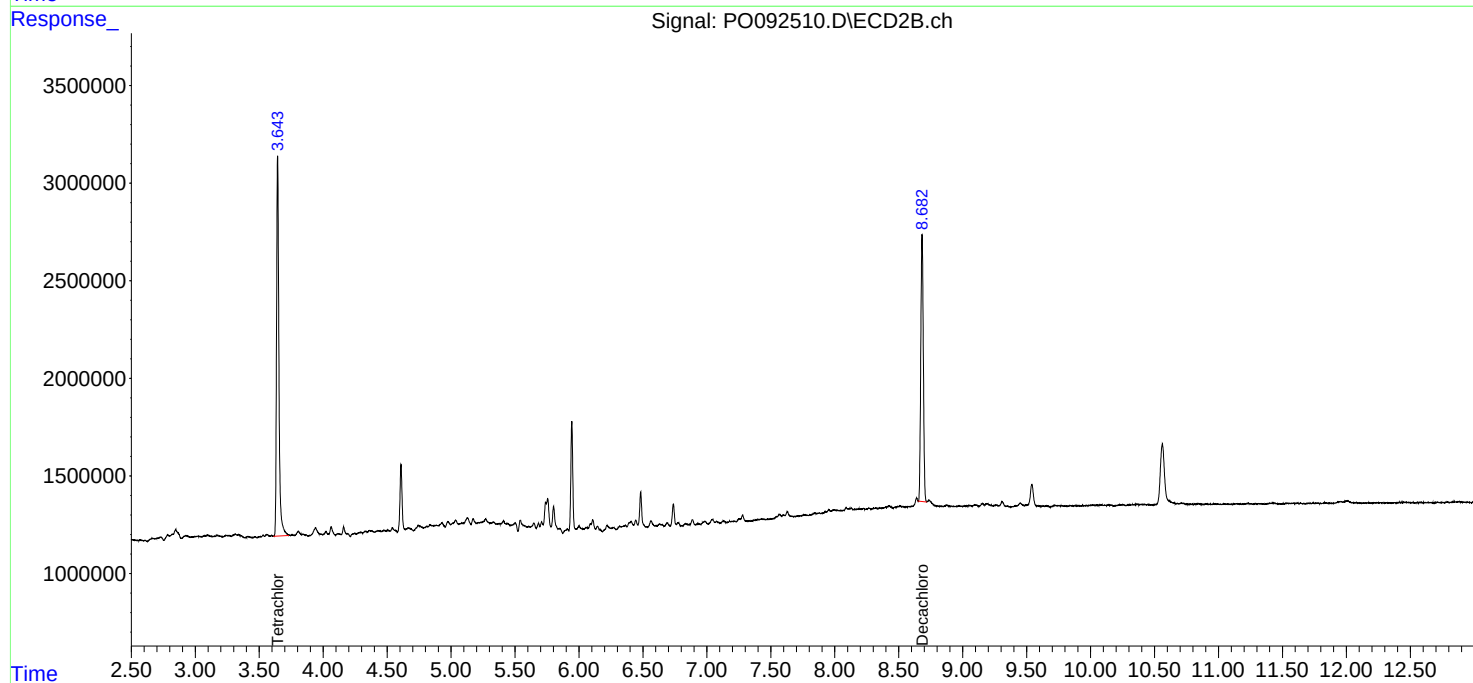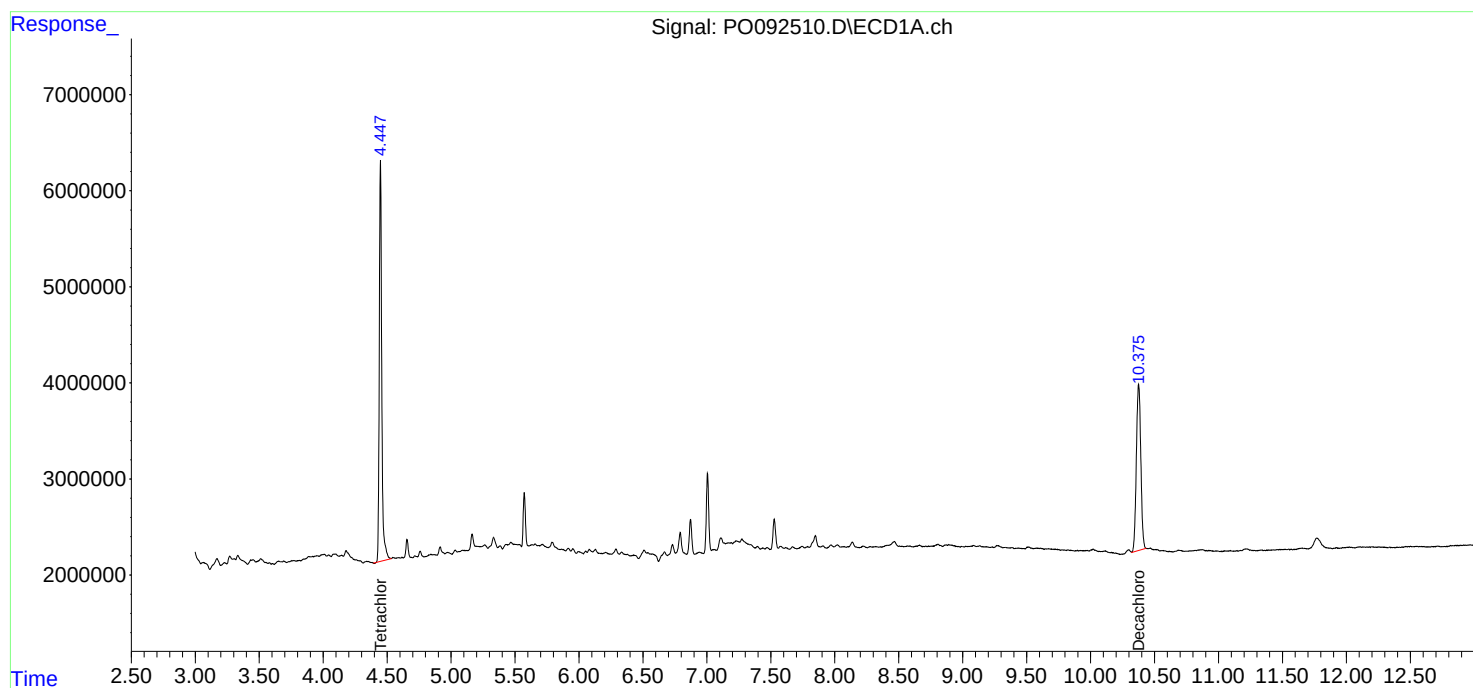

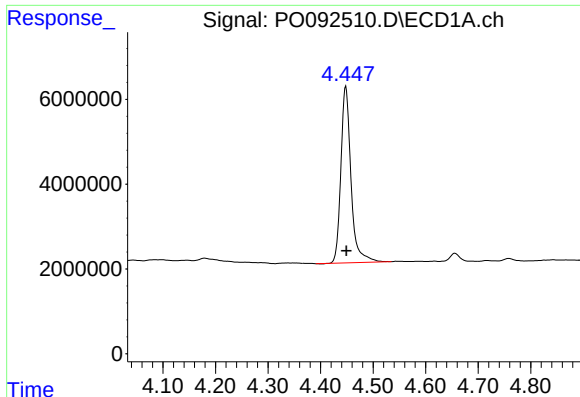


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.001 min
Response: 55951361
Conc: 19.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-6-021523


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/17/2023
Supervised By :Sohil Jodhani 02/17/2023

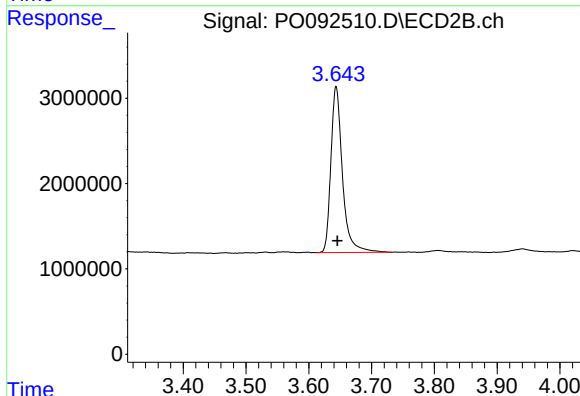


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.002 min
Response: 24905420
Conc: 17.74 ng/ml

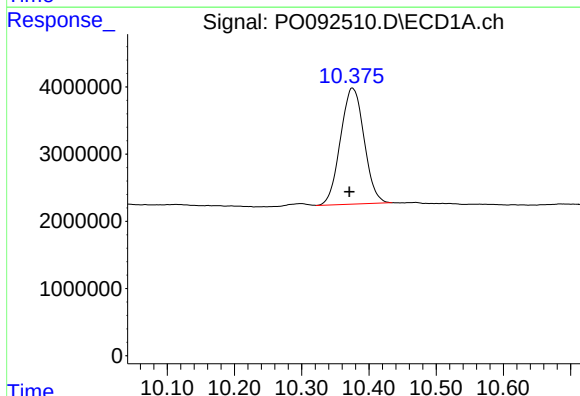

#2 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.003 min
Response: 41972800
Conc: 20.34 ng/ml m

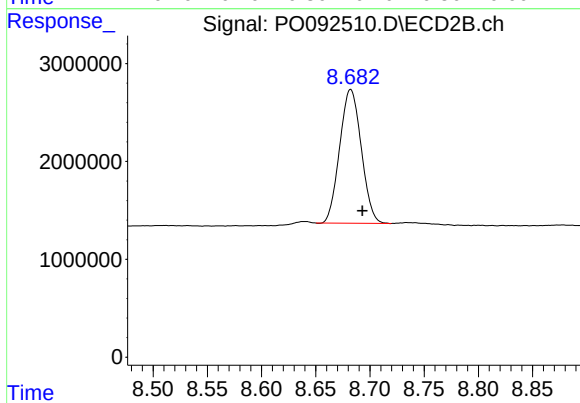

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.011 min
Response: 18951584
Conc: 16.79 ng/ml