

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021722\
 Data File : P0084728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Feb 2022 11:44
 Operator : YP\AJ
 Sample : N1553-24 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LAW-2022-12B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 04:56:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 14 17:50:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.597	262984	72763	1.338	1.613
2) SA Decachlor...	10.431	8.624	408603	57313	3.293m	1.572m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021722\
Data File : P0084728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Feb 2022 11:44
Operator : YP\AJ
Sample : N1553-24 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LAW-2022-12B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 04:56:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021422.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 14 17:50:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

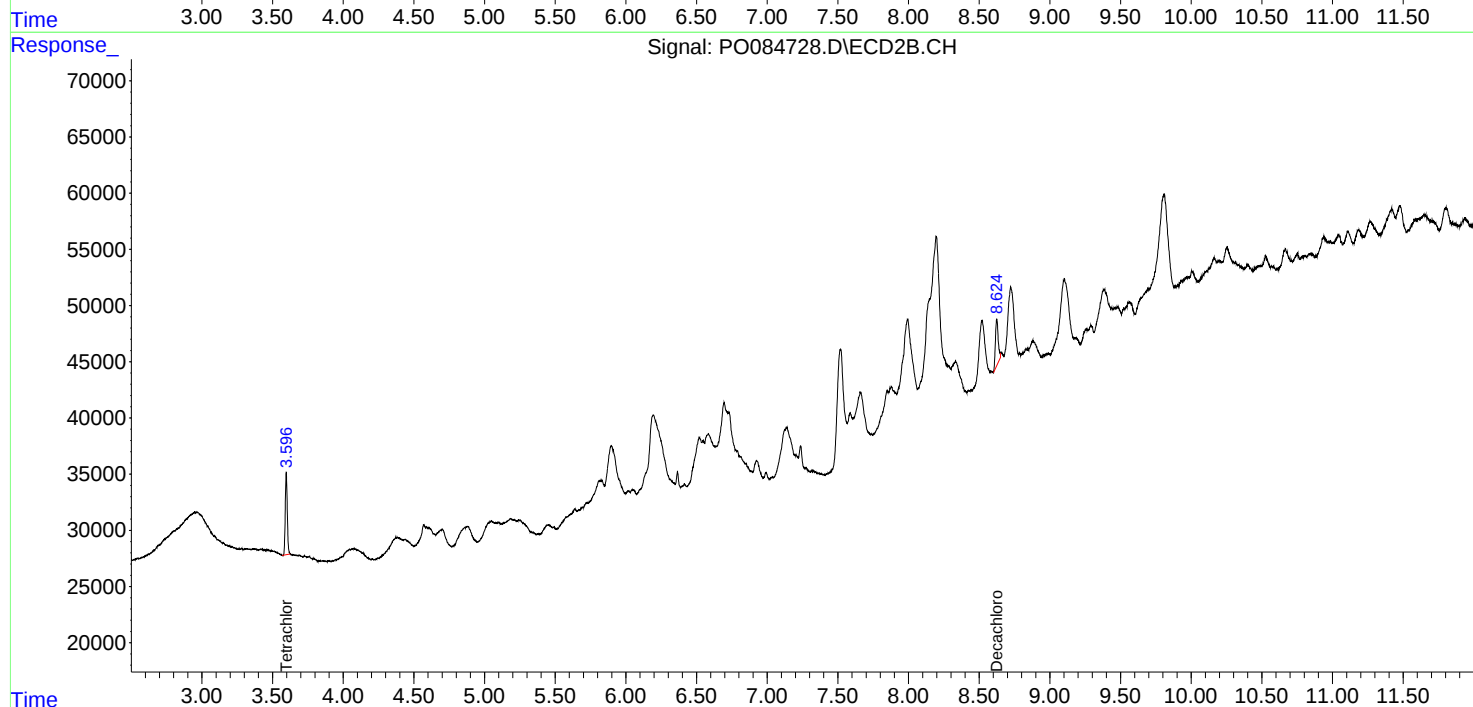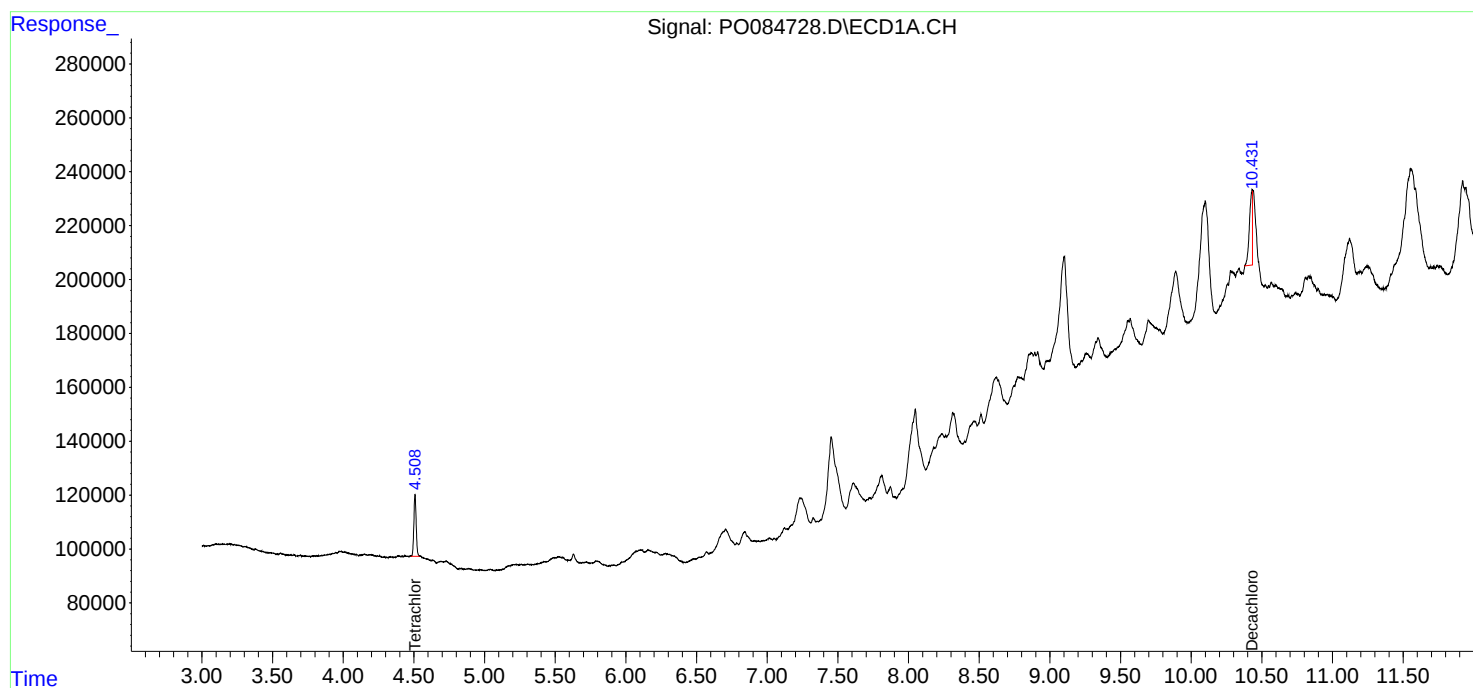


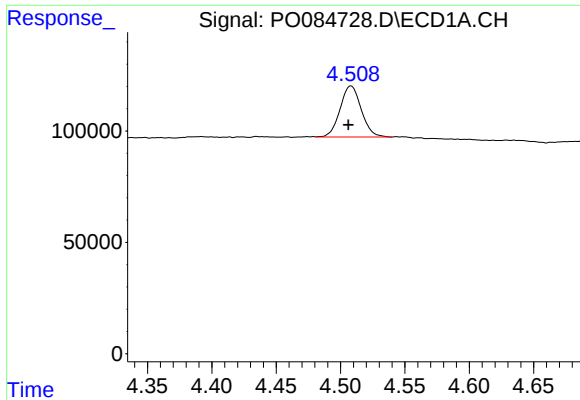

#1 Tetrachloro-m-xylene


R.T.: 4.508 min
Delta R.T.: 0.002 min
Response: 262984
Conc: 1.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2022-12B

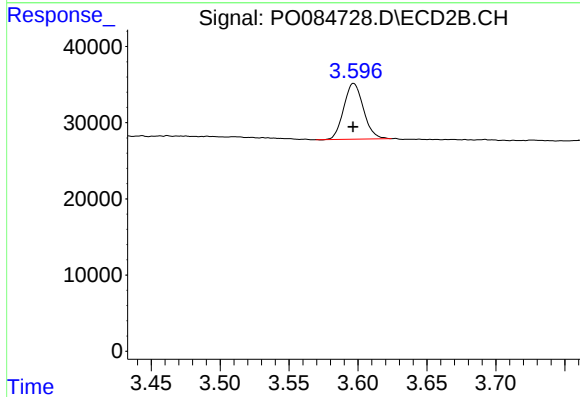


#1 Tetrachloro-m-xylene

R.T.: 3.597 min
Delta R.T.: 0.000 min
Response: 72763
Conc: 1.61 ng/ml

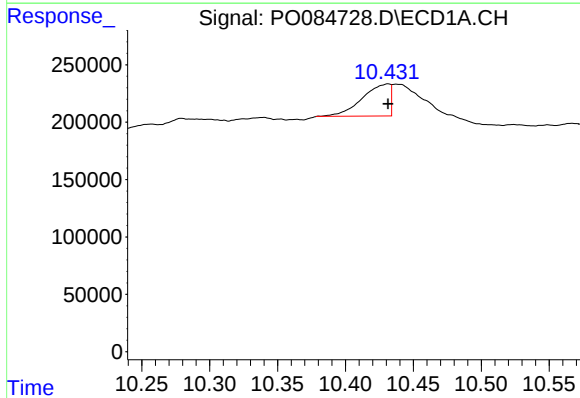

#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: 0.000 min
Response: 408603
Conc: 3.29 ng/ml m

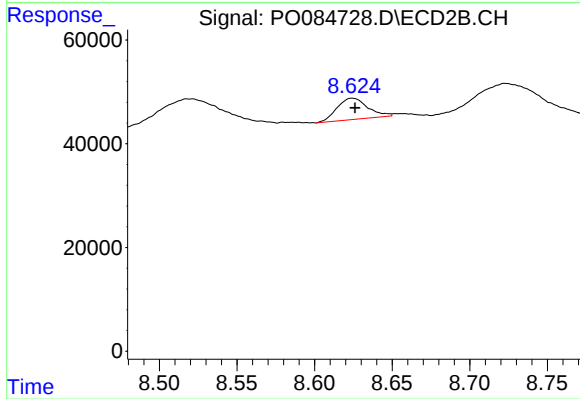

#2 Decachlorobiphenyl

R.T.: 8.624 min
Delta R.T.: -0.002 min
Response: 57313
Conc: 1.57 ng/ml m