

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 12:16
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 13:00:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.643	54609037	23934637	18.864	17.046
2) SA Decachlor...	10.391	8.685	43186680	22163716	20.924	19.633
Target Compounds						
3) L1 AR-1016-1	5.579f	0.000	1274718	0	13.938	N.D. #
9) L2 AR-1221-2	4.761	0.000	867953	0	31.363	N.D. #
10) L2 AR-1221-3	4.761f	0.000	867953	0	10.286	N.D. #
11) L3 AR-1232-1	4.761f	0.000	867953	0	12.544	N.D. #
16) L4 AR-1242-1	5.579f	0.000	1274718	0	16.345	N.D. #
21) L5 AR-1248-1	5.579f	0.000	1274718	0	21.961	N.D. #
33) L7 AR-1260-3	0.000	6.554	0	482318	N.D.	5.564 #
40) L8 AR-1262-5	0.000	8.070f	0	278163	N.D.	5.398 #
44) L9 AR-1268-4	0.000	8.070f	0	278163	N.D.	4.431 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
Data File : P0092548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 12:16
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 13:00:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

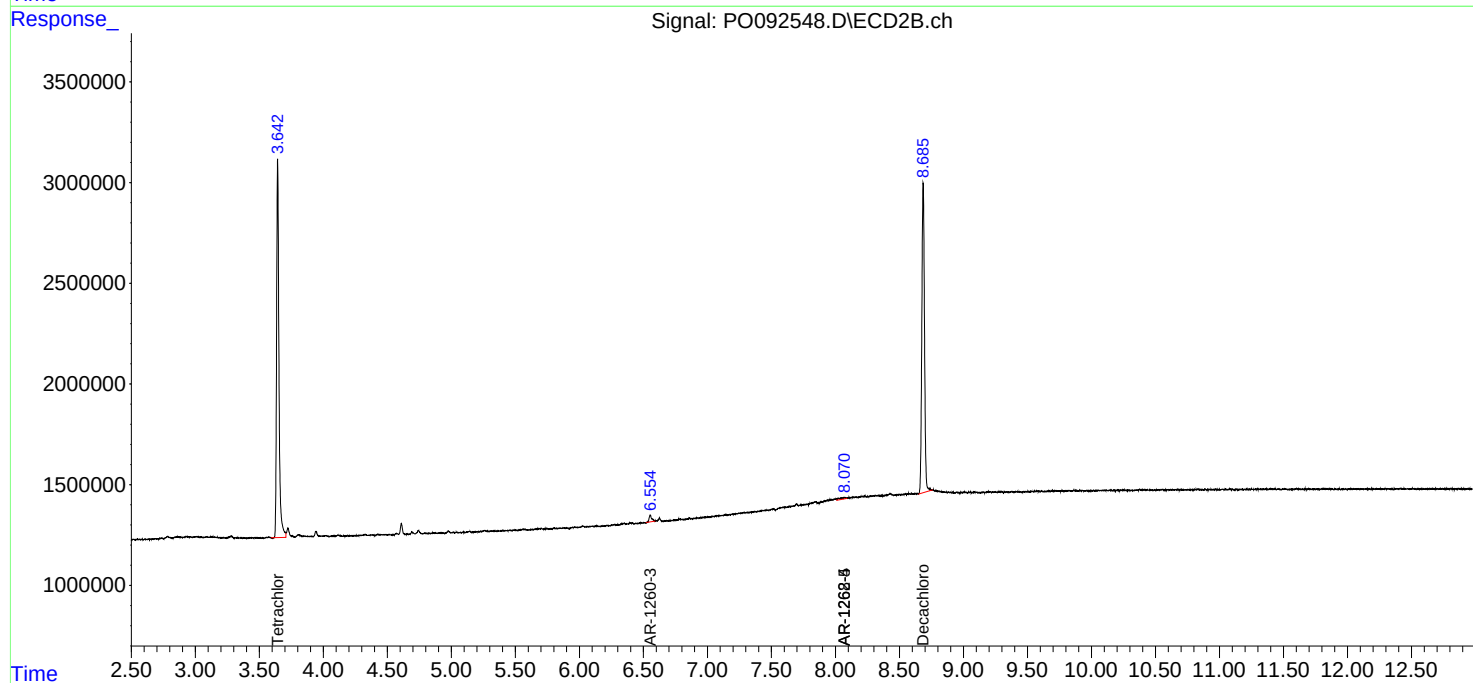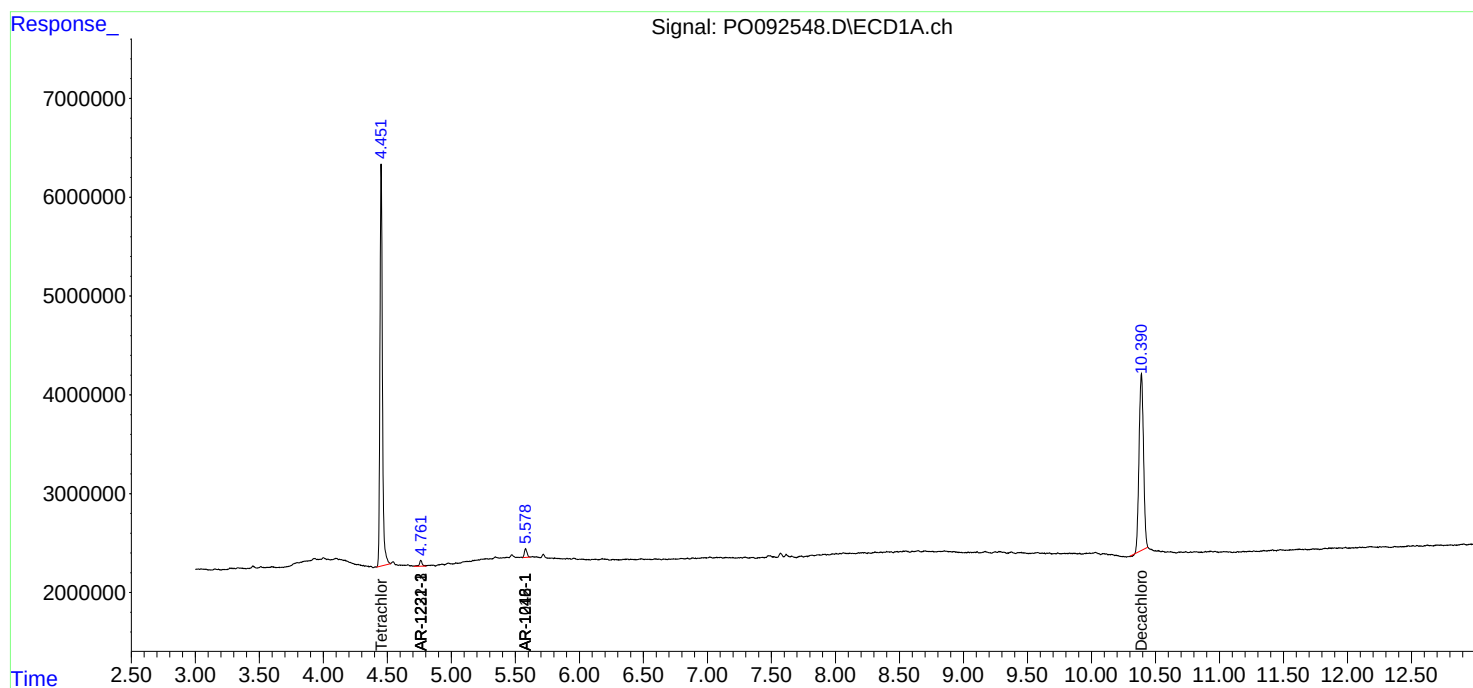


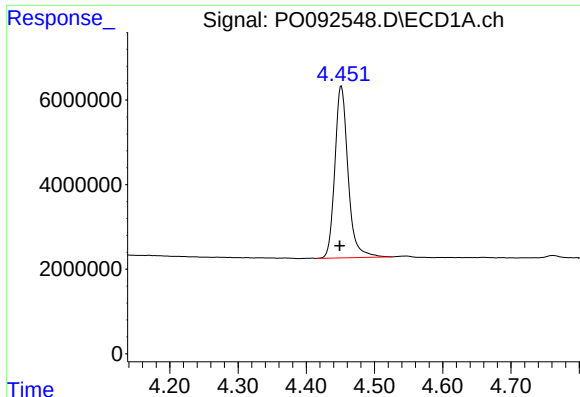

#1 Tetrachloro-m-xylene


R.T.: 4.451 min
Delta R.T.: 0.002 min
Response: 54609037
Conc: 18.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

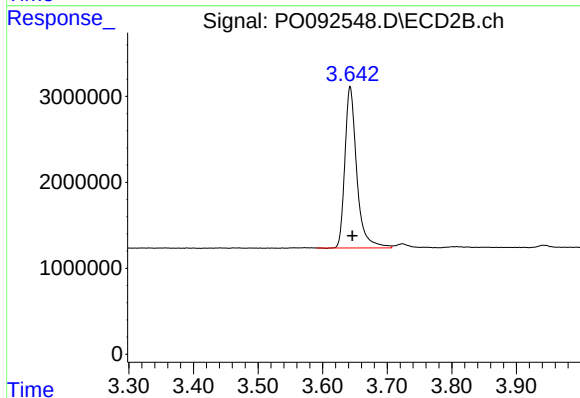


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.003 min
Response: 23934637
Conc: 17.05 ng/ml

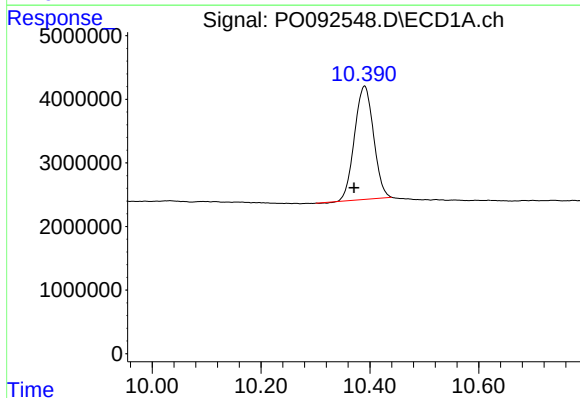


#2 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: 0.019 min
Response: 43186680
Conc: 20.92 ng/ml

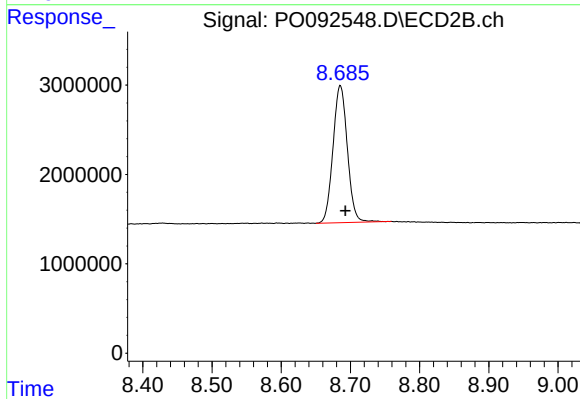

#2 Decachlorobiphenyl


R.T.: 8.685 min
Delta R.T.: -0.008 min
Response: 22163716
Conc: 19.63 ng/ml

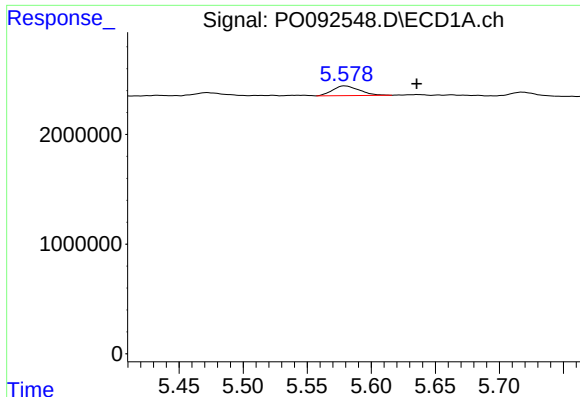

#3 AR-1016-1


R.T.: 5.579 min
Delta R.T.: -0.056 min
Response: 1274718
Conc: 13.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

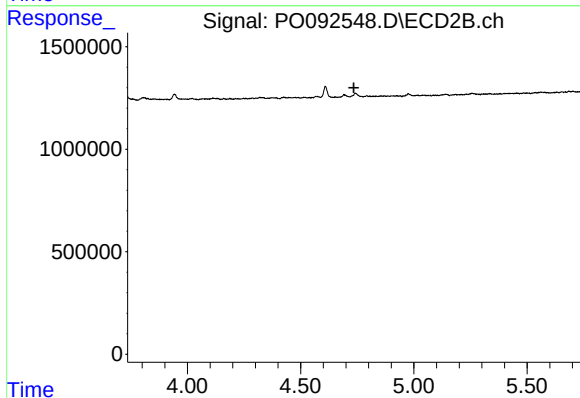


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

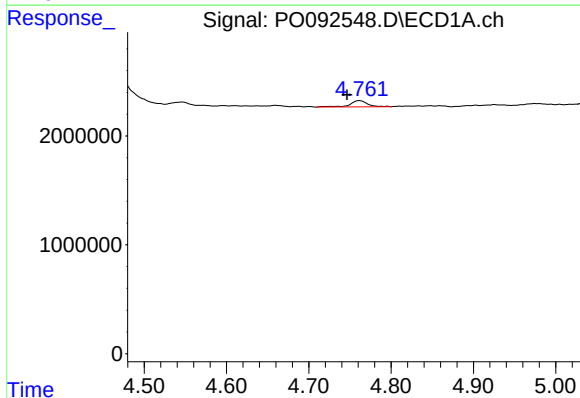


#9 AR-1221-2

R.T.: 4.761 min
Delta R.T.: 0.015 min
Response: 867953
Conc: 31.36 ng/ml

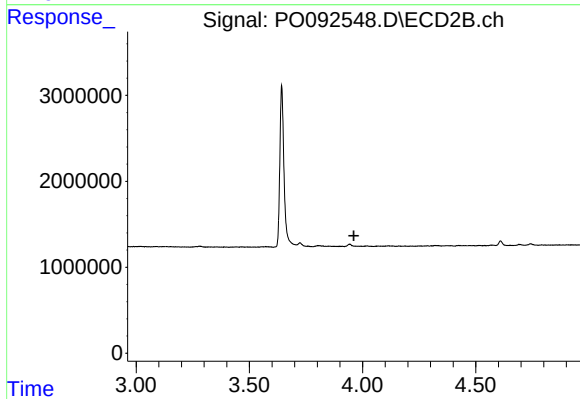

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.962 min
Response: 0
Conc: N.D.

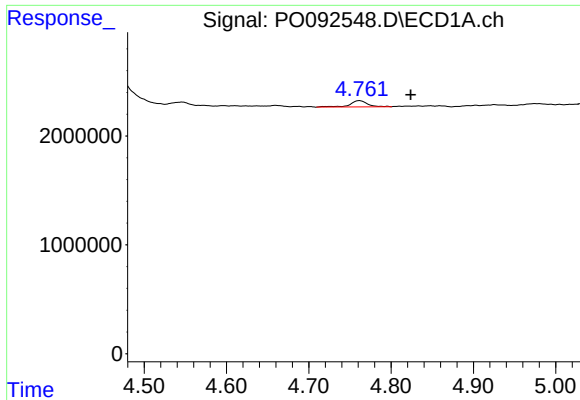

#10 AR-1221-3


R.T.: 4.761 min
Delta R.T.: -0.062 min
Response: 867953
Conc: 10.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

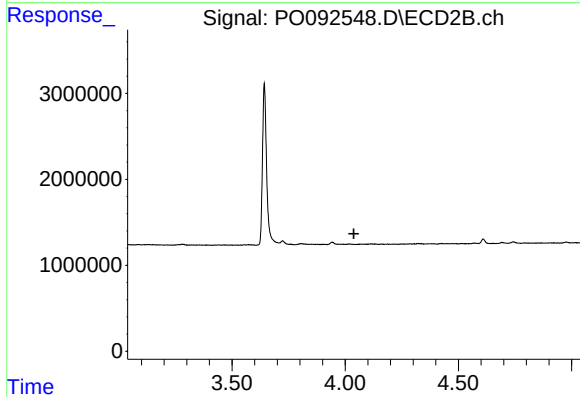


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.038 min
Response: 0
Conc: N.D.

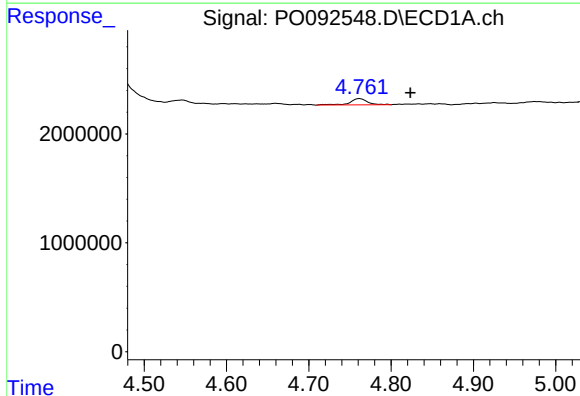


#11 AR-1232-1

R.T.: 4.761 min
Delta R.T.: -0.062 min
Response: 867953
Conc: 12.54 ng/ml

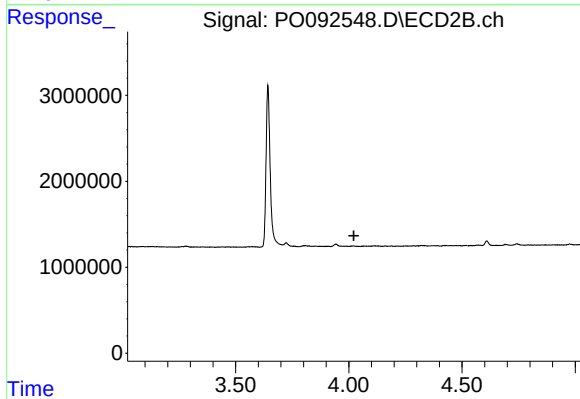

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.022 min
Response: 0
Conc: N.D.

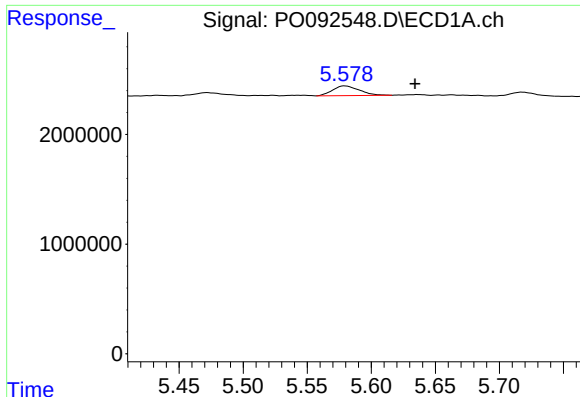

#16 AR-1242-1


R.T.: 5.579 min
Delta R.T.: -0.055 min
Response: 1274718
Conc: 16.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

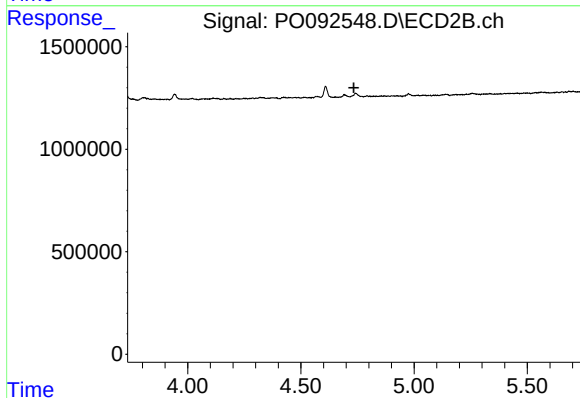


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

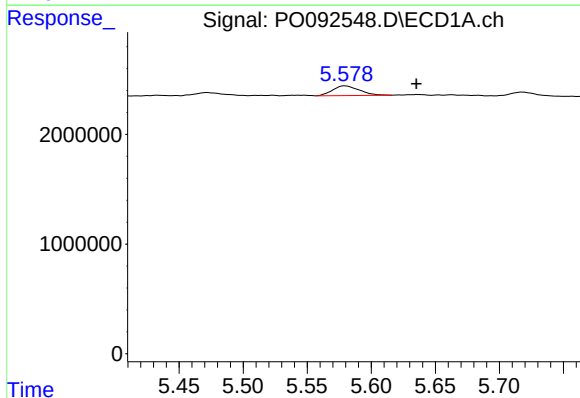


#21 AR-1248-1

R.T.: 5.579 min
Delta R.T.: -0.056 min
Response: 1274718
Conc: 21.96 ng/ml

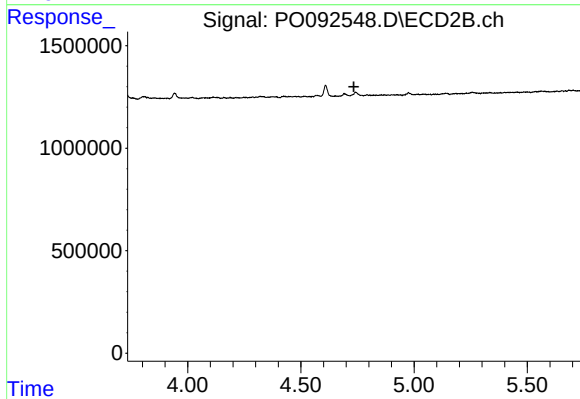

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

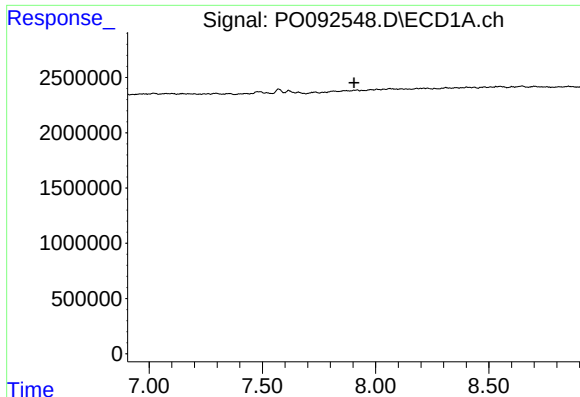

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

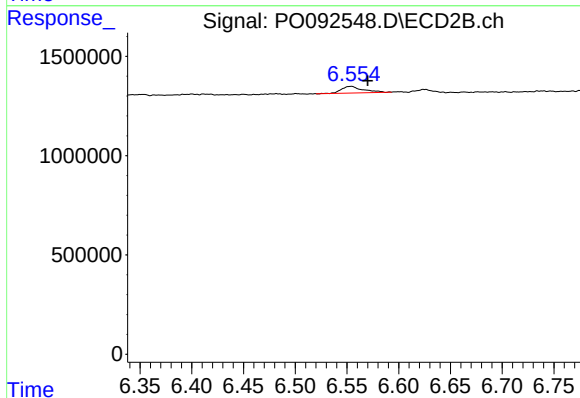


#33 AR-1260-3

R.T.: 6.554 min
Delta R.T.: -0.016 min
Response: 482318
Conc: 5.56 ng/ml

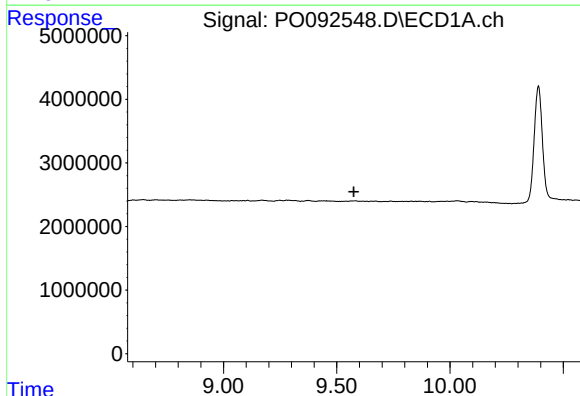


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.575 min
Response: 0
Conc: N.D.

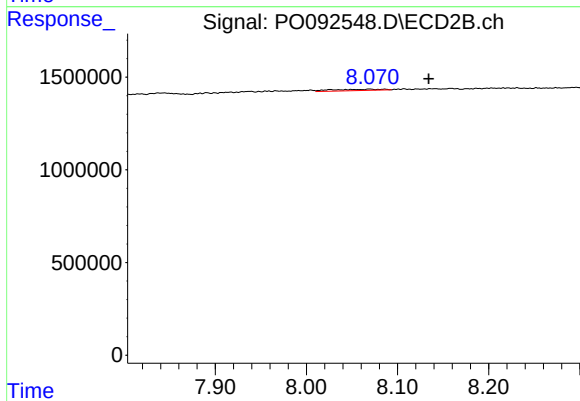

#40 AR-1262-5


R.T.: 8.070 min
Delta R.T.: -0.064 min
Response: 278163
Conc: 5.40 ng/ml

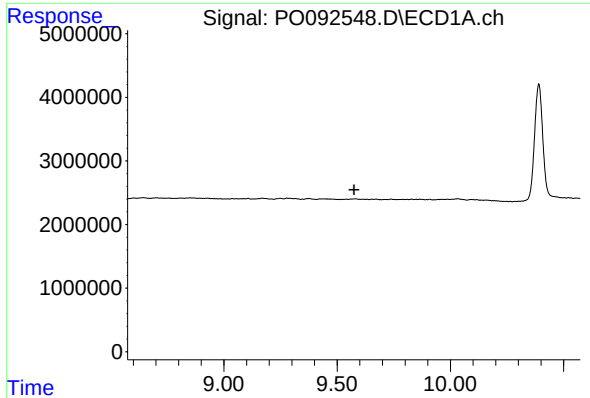

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

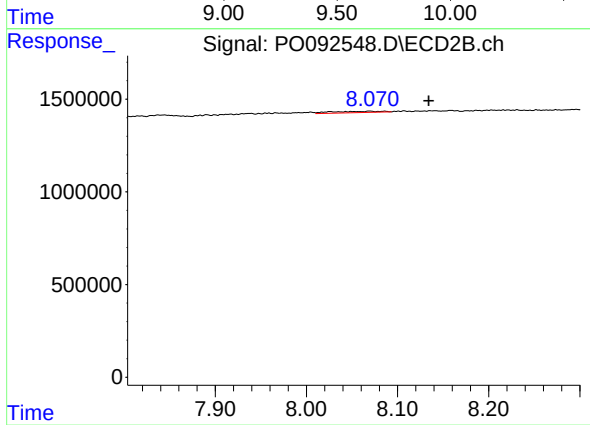

#44 AR-1268-4

R.T.: 8.070 min
Delta R.T.: -0.065 min
Response: 278163
Conc: 4.43 ng/ml