

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 13:12
 Operator : YP/AJ
 Sample : 01584-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV2023-9A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:00:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.453	3.644	3234851	1753156	1.117	1.249
2)	SA Decachlor...	10.393	8.688	3663343	1519184	1.775	1.346
Target Compounds							
3)	L1 AR-1016-1	5.579f	0.000	1185082	0	12.958	N.D. #
9)	L2 AR-1221-2	4.788f	0.000	2926349	0	105.742	N.D. #
10)	L2 AR-1221-3	4.788f	0.000	2926349	0	34.679	N.D. #
11)	L3 AR-1232-1	4.788f	0.000	2926349	0	42.291	N.D. #
16)	L4 AR-1242-1	5.579f	0.000	1185082	0	15.196	N.D. #
21)	L5 AR-1248-1	5.579f	0.000	1185082	0	20.417	N.D. #
35)	L7 AR-1260-5	0.000	7.314	0	127497	N.D.	0.896 #
37)	L8 AR-1262-2	0.000	7.314	0	127497	N.D.	0.864 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
Data File : P0092551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 13:12
Operator : YP/AJ
Sample : 01584-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV2023-9A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:00:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

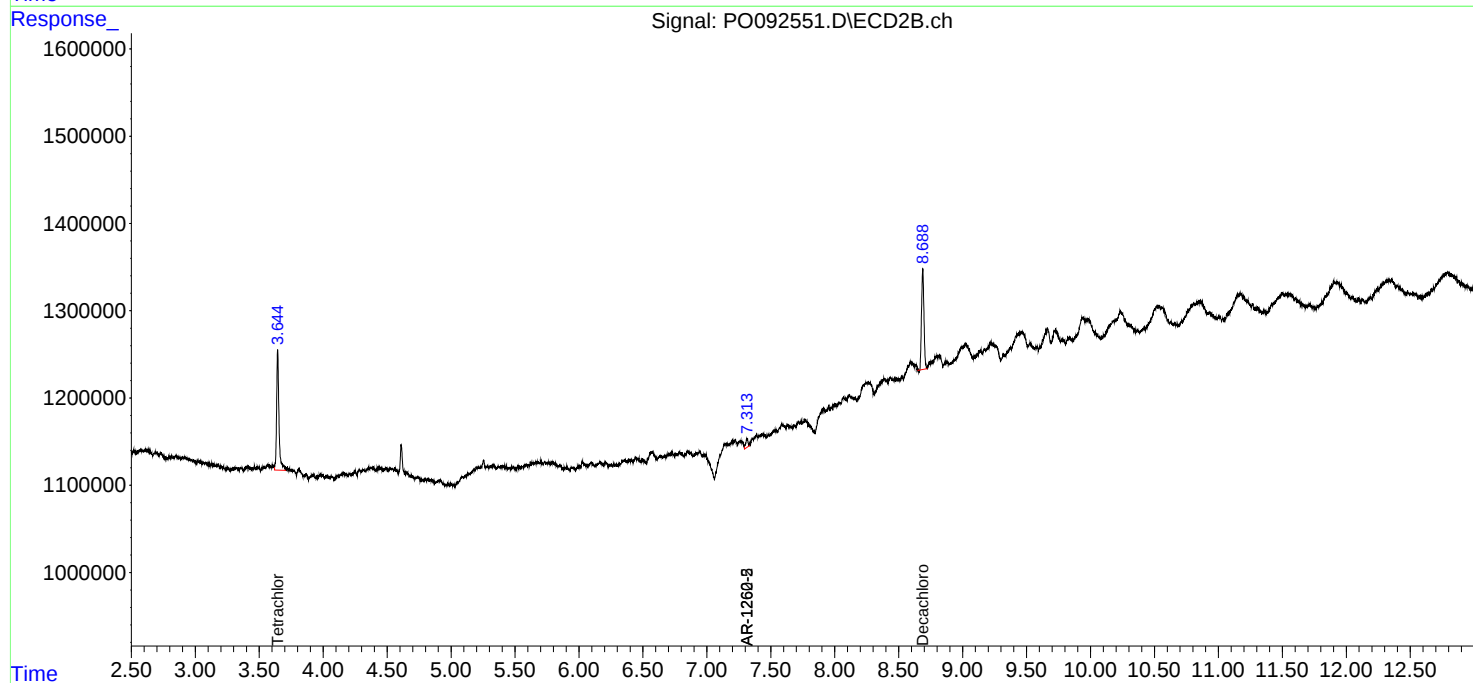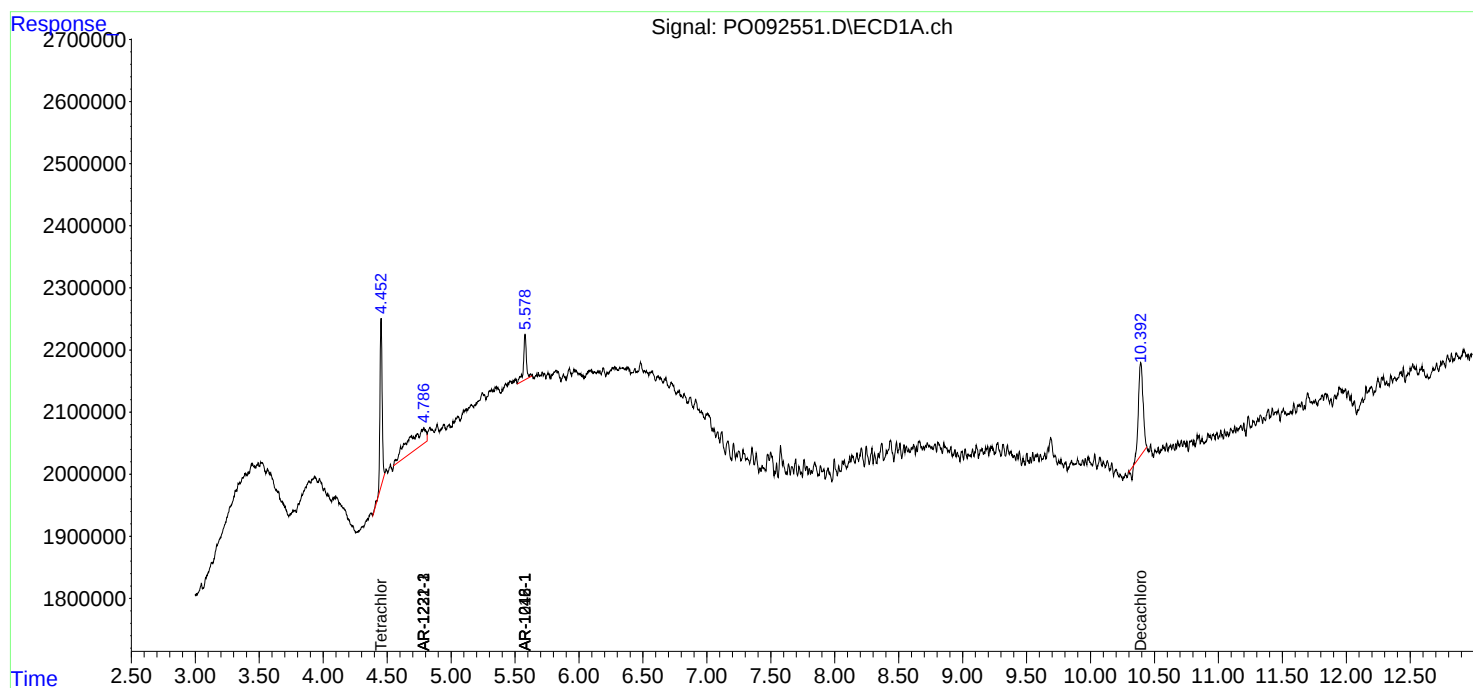


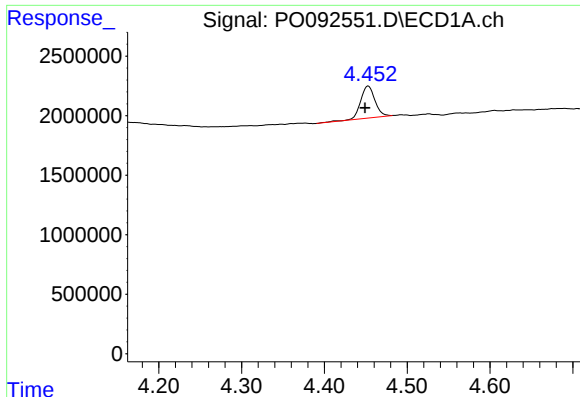

#1 Tetrachloro-m-xylene


R.T.: 4.453 min
Delta R.T.: 0.004 min
Response: 3234851
Conc: 1.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV2023-9A

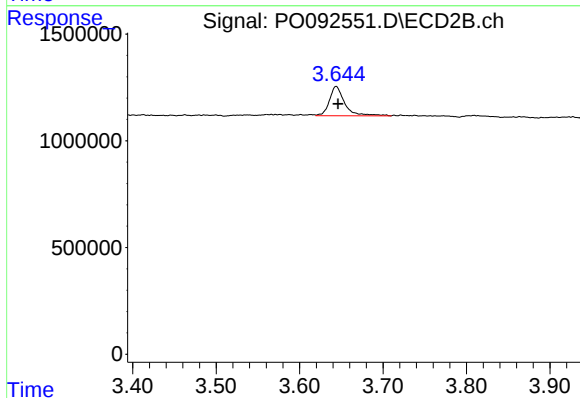


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.002 min
Response: 1753156
Conc: 1.25 ng/ml

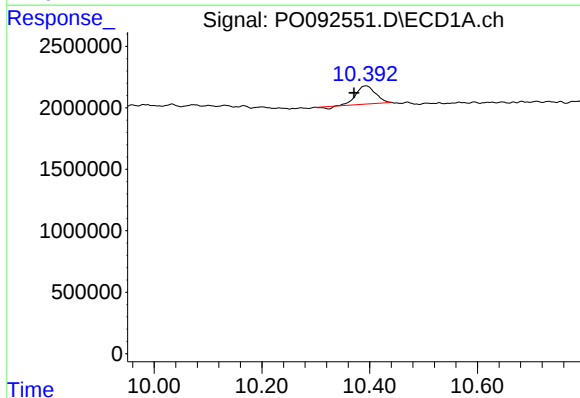


#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.022 min
Response: 3663343
Conc: 1.77 ng/ml

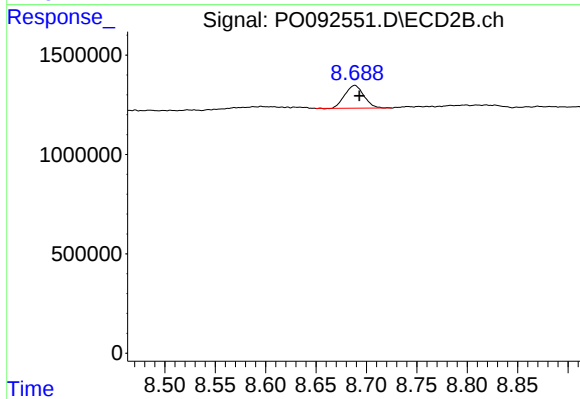

#2 Decachlorobiphenyl


R.T.: 8.688 min
Delta R.T.: -0.005 min
Response: 1519184
Conc: 1.35 ng/ml

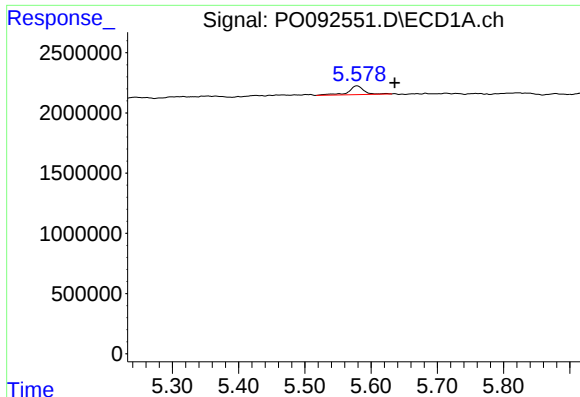

#3 AR-1016-1


R.T.: 5.579 min
Delta R.T.: -0.057 min
Response: 1185082
Conc: 12.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV2023-9A

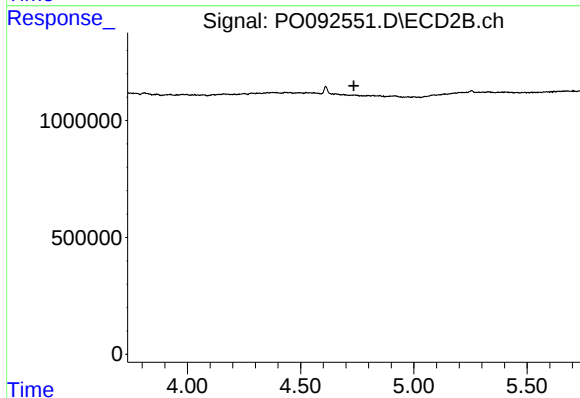


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

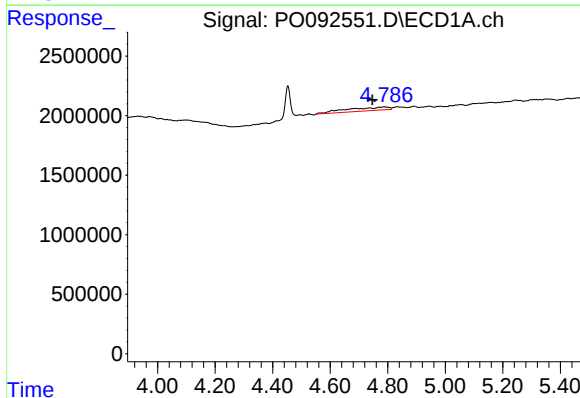


#9 AR-1221-2

R.T.: 4.788 min
Delta R.T.: 0.041 min
Response: 2926349
Conc: 105.74 ng/ml

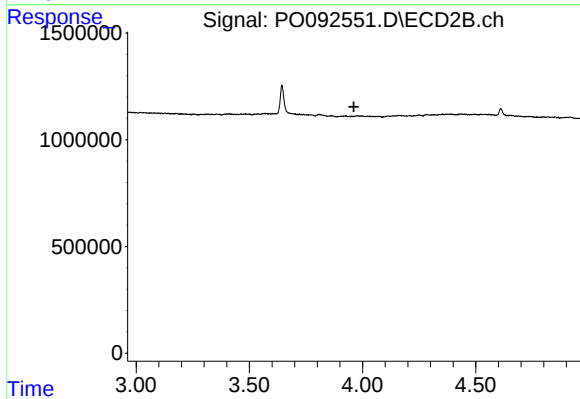

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.962 min
Response: 0
Conc: N.D.

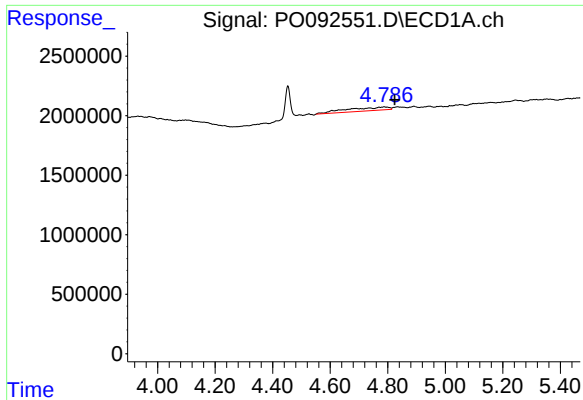

#10 AR-1221-3


R.T.: 4.788 min
Delta R.T.: -0.036 min
Response: 2926349
Conc: 34.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV2023-9A

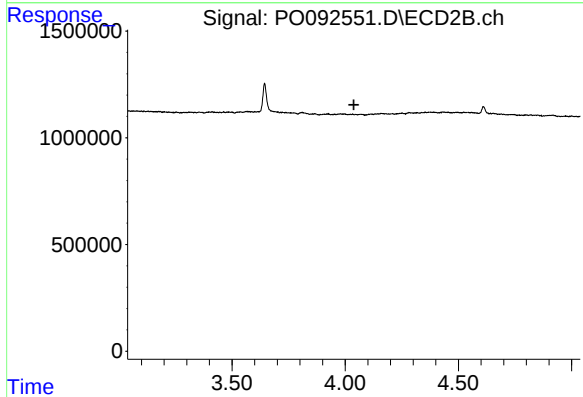


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.038 min
Response: 0
Conc: N.D.

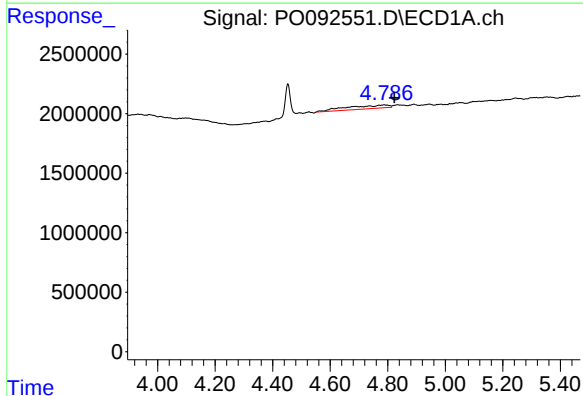


#11 AR-1232-1

R.T.: 4.788 min
Delta R.T.: -0.036 min
Response: 2926349
Conc: 42.29 ng/ml

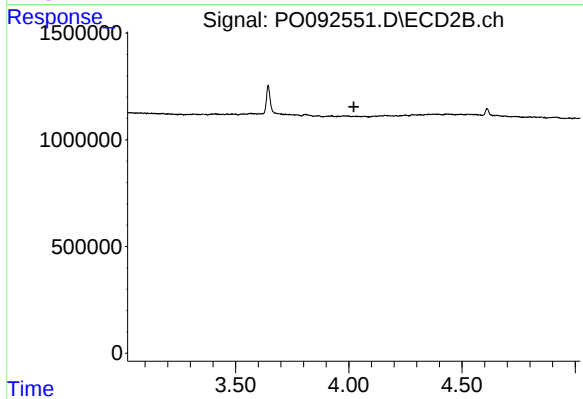

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.022 min
Response: 0
Conc: N.D.

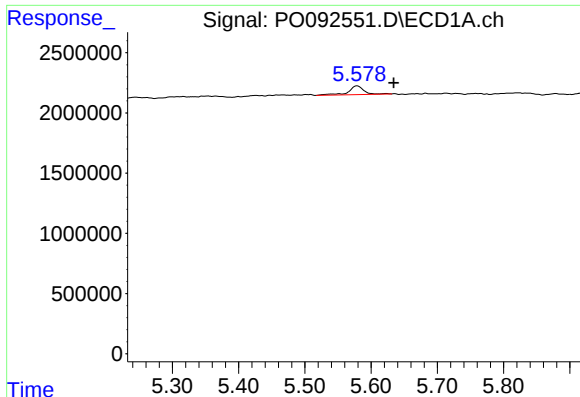

#16 AR-1242-1


R.T.: 5.579 min
Delta R.T.: -0.055 min
Response: 1185082
Conc: 15.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV2023-9A

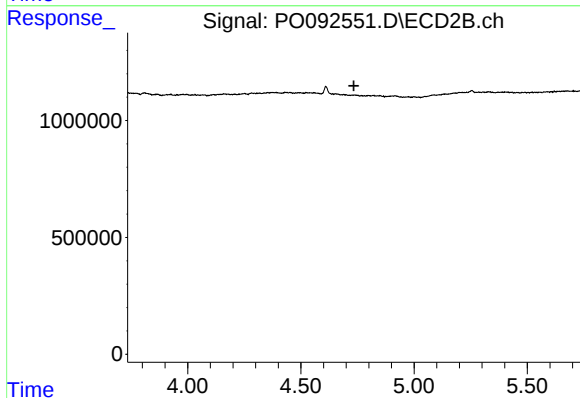


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

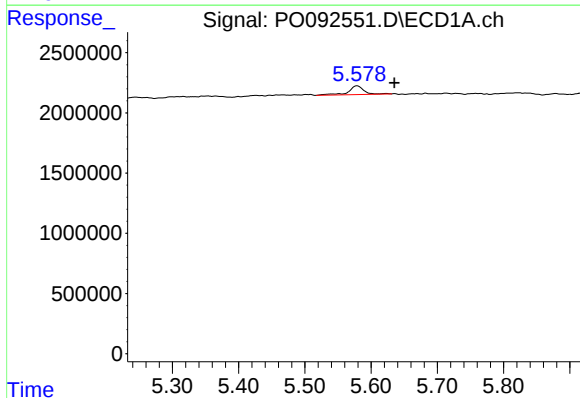


#21 AR-1248-1

R.T.: 5.579 min
Delta R.T.: -0.057 min
Response: 1185082
Conc: 20.42 ng/ml

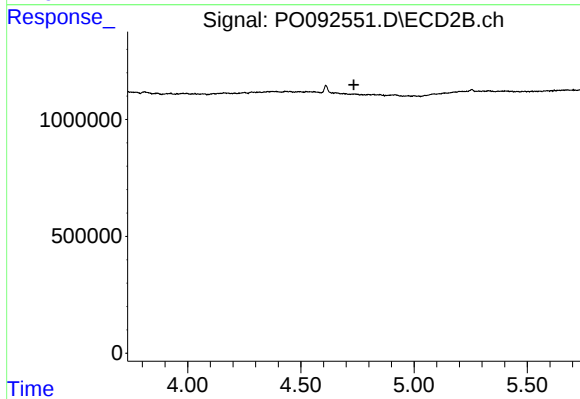

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

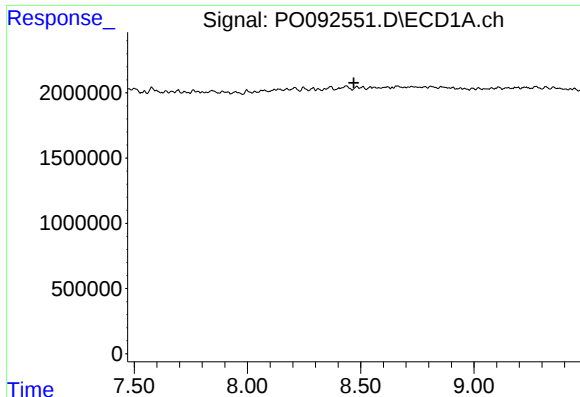

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IRV2023-9A

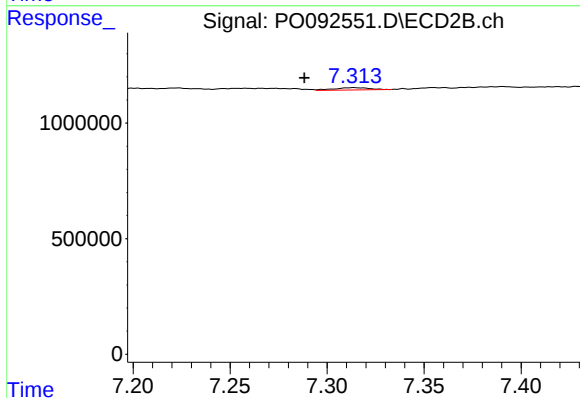


#35 AR-1260-5

R.T.: 7.314 min
Delta R.T.: 0.025 min
Response: 127497
Conc: 0.90 ng/ml

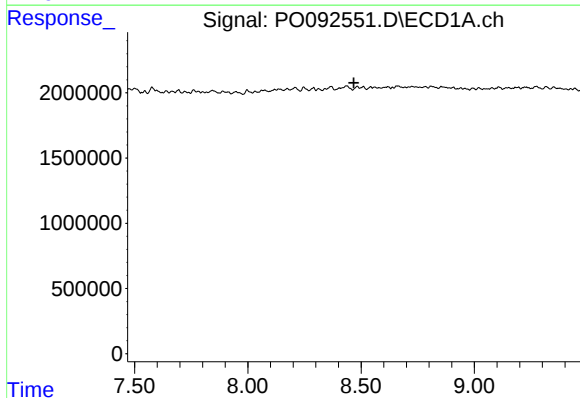

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.468 min
Response: 0
Conc: N.D.

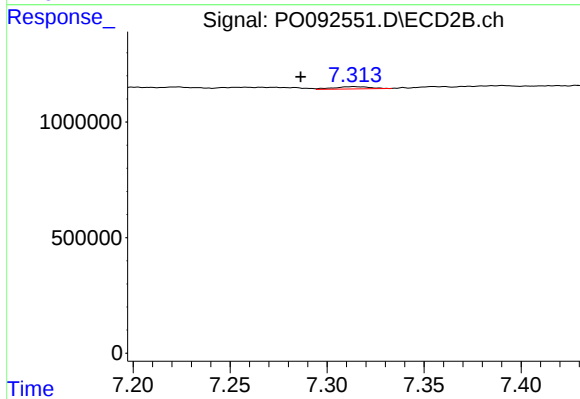

#37 AR-1262-2

R.T.: 7.314 min
Delta R.T.: 0.027 min
Response: 127497
Conc: 0.86 ng/ml