

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 14:44
 Operator : YP/AJ
 Sample : 01590-04 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC271315LOZ-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 15:45:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.452	3.642	3270228	1639732	1.130	1.168
2) SA Decachlor...	10.393	8.688	3905016	2039247	1.892	1.806
Target Compounds						
7) L1 AR-1016-5	6.173f	0.000	885515	0	12.324	N.D. #
23) L5 AR-1248-3	6.173f	0.000	885515	0	9.029	N.D. #
30) L6 AR-1254-5	7.797	0.000	717114	0	5.097	N.D. #
32) L7 AR-1260-2	7.586f	0.000	3185997	0	21.485	N.D. #
34) L7 AR-1260-4	8.163	0.000	1657802	0	13.373	N.D. #
36) L8 AR-1262-1	7.797	0.000	717114	0	6.637	N.D. #
40) L8 AR-1262-5	0.000	8.083f	0	1075864	N.D.	20.880 #
44) L9 AR-1268-4	0.000	8.083f	0	1075864	N.D.	17.139 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021723\
Data File : PO092556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 14:44
Operator : YP/AJ
Sample : 01590-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 15:45:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

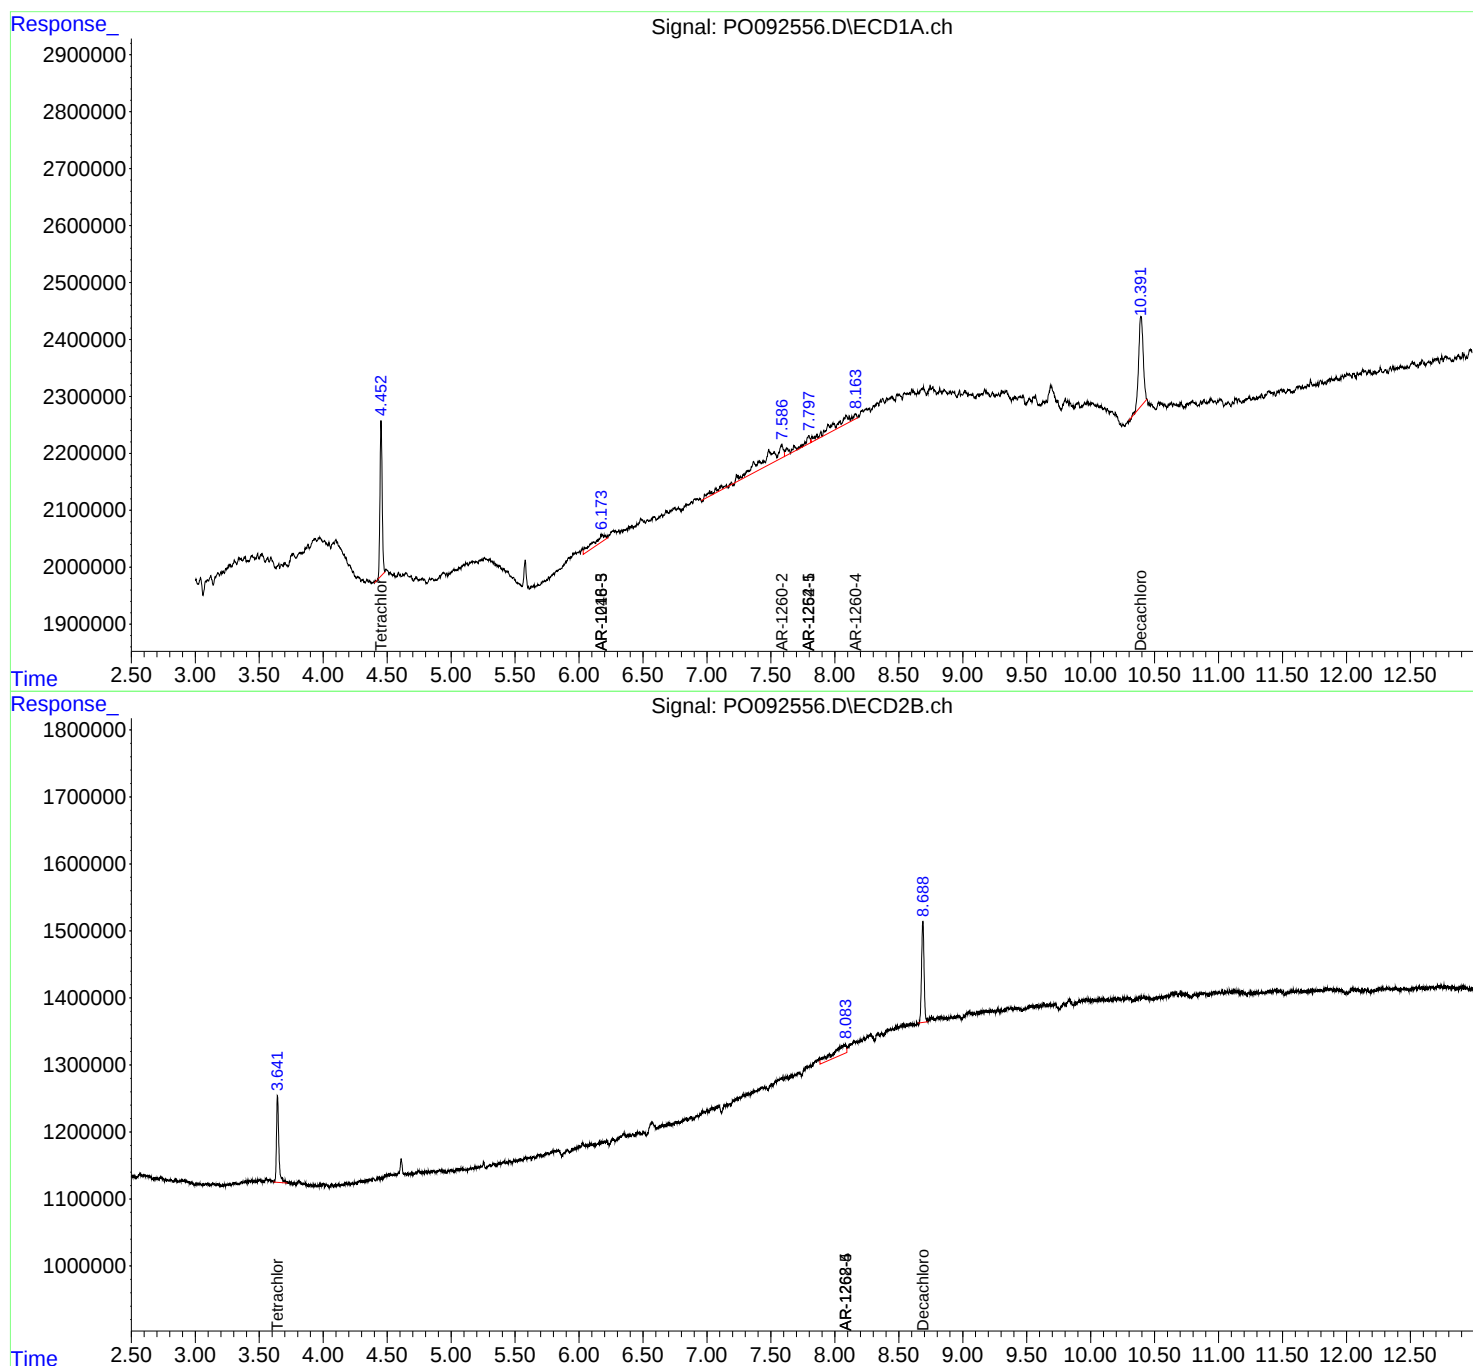


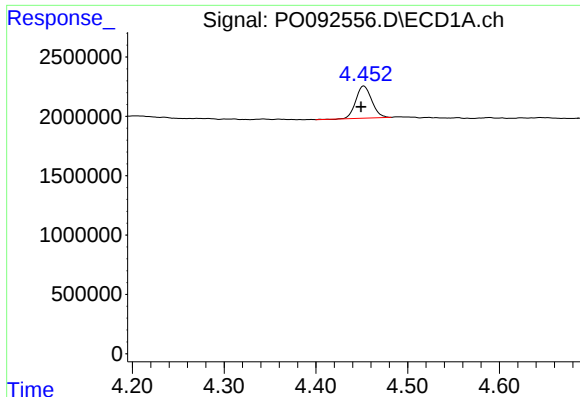

#1 Tetrachloro-m-xylene


R.T.: 4.452 min
Delta R.T.: 0.003 min
Response: 3270228
Conc: 1.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2

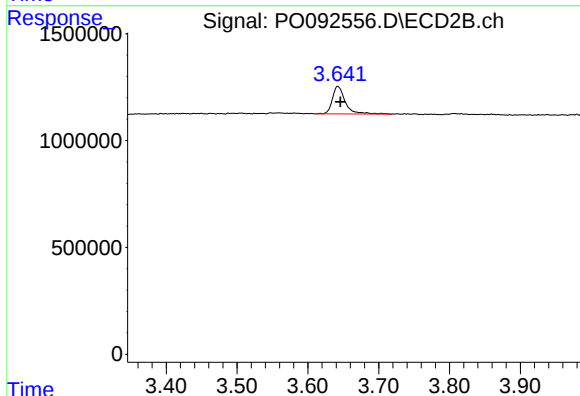


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.004 min
Response: 1639732
Conc: 1.17 ng/ml

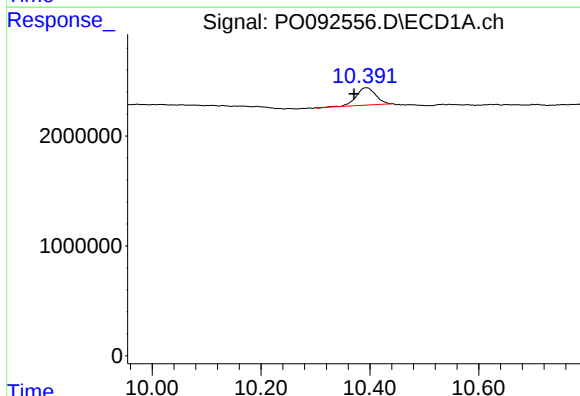


#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.022 min
Response: 3905016
Conc: 1.89 ng/ml

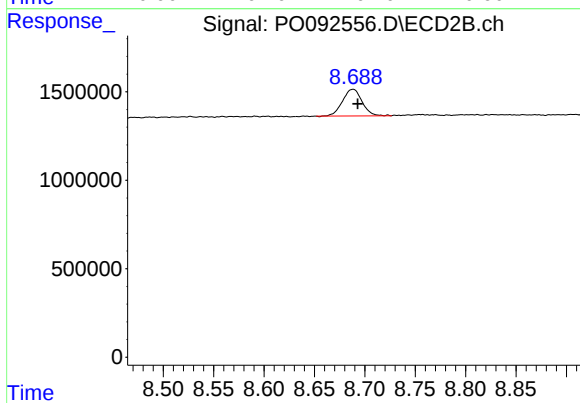

#2 Decachlorobiphenyl


R.T.: 8.688 min
Delta R.T.: -0.005 min
Response: 2039247
Conc: 1.81 ng/ml

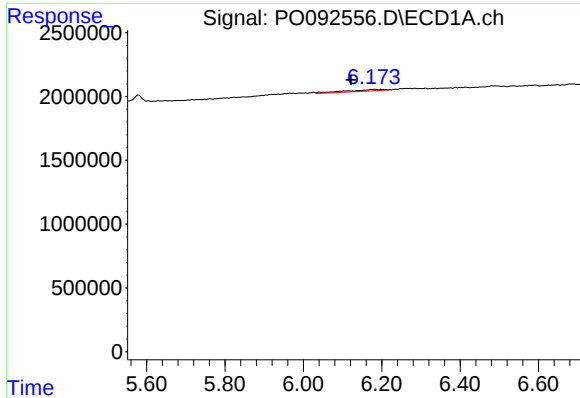

#7 AR-1016-5


R.T.: 6.173 min
Delta R.T.: 0.051 min
Response: 885515
Conc: 12.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2

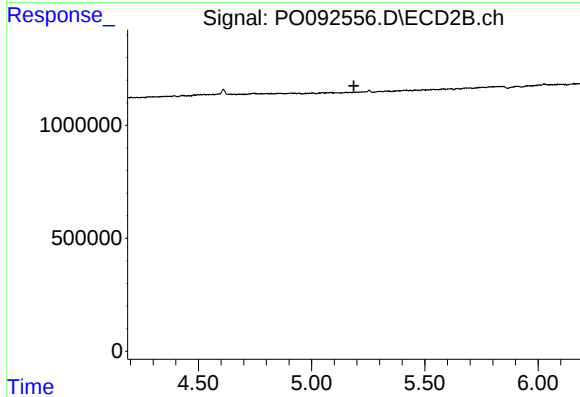


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.187 min
Response: 0
Conc: N.D.

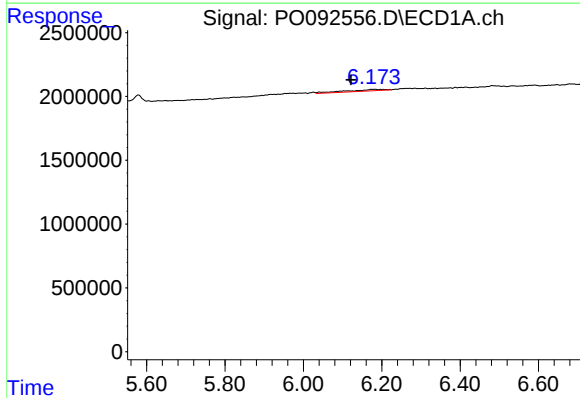


#23 AR-1248-3

R.T.: 6.173 min
Delta R.T.: 0.051 min
Response: 885515
Conc: 9.03 ng/ml

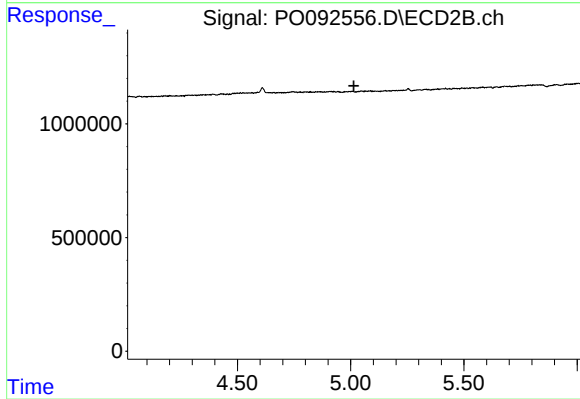

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T. : 5.014 min
Response: 0
Conc: N.D.

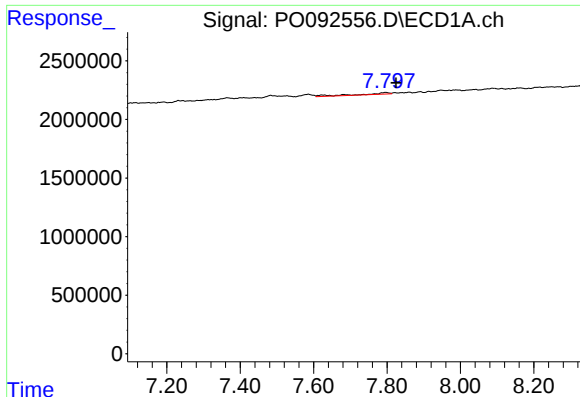

#30 AR-1254-5


R.T.: 7.797 min
Delta R.T.: -0.027 min
Response: 717114
Conc: 5.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2

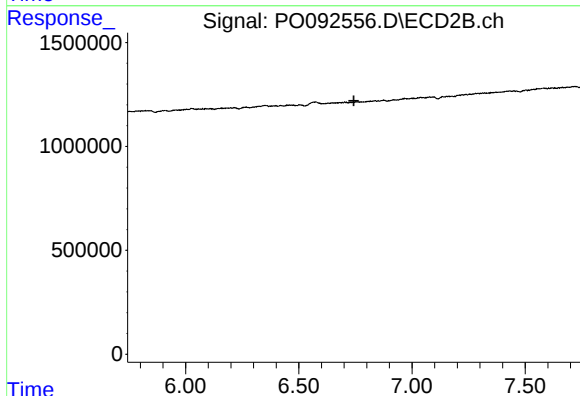


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.743 min
Response: 0
Conc: N.D.

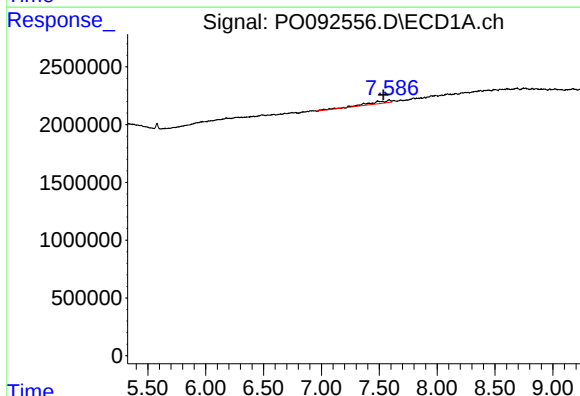


#32 AR-1260-2

R.T.: 7.586 min
Delta R.T.: 0.049 min
Response: 3185997
Conc: 21.49 ng/ml

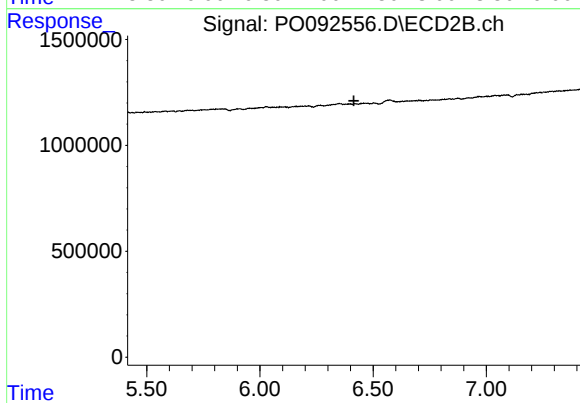

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

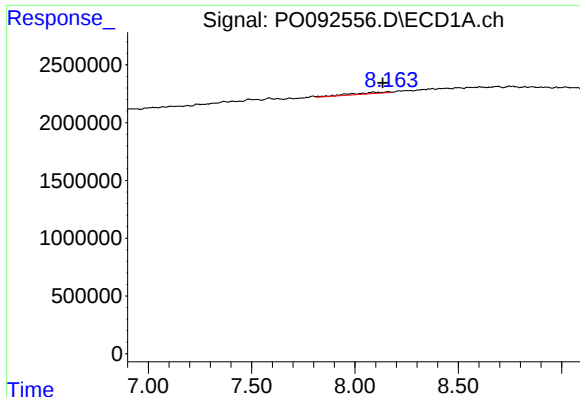

#34 AR-1260-4


R.T.: 8.163 min
Delta R.T.: 0.029 min
Response: 1657802
Conc: 13.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2

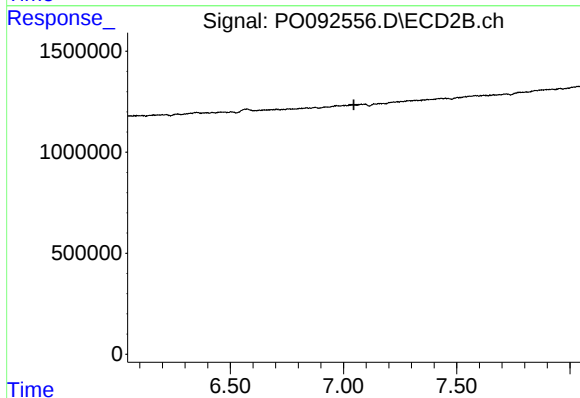


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

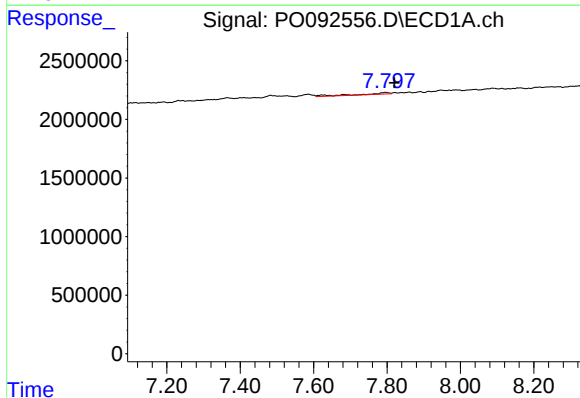


#36 AR-1262-1

R.T.: 7.797 min
Delta R.T.: -0.023 min
Response: 717114
Conc: 6.64 ng/ml

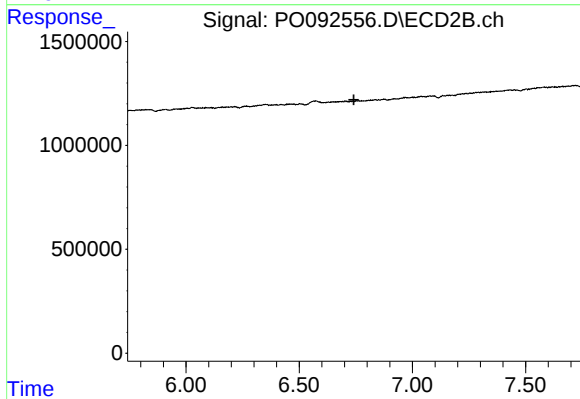

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.741 min
Response: 0
Conc: N.D.

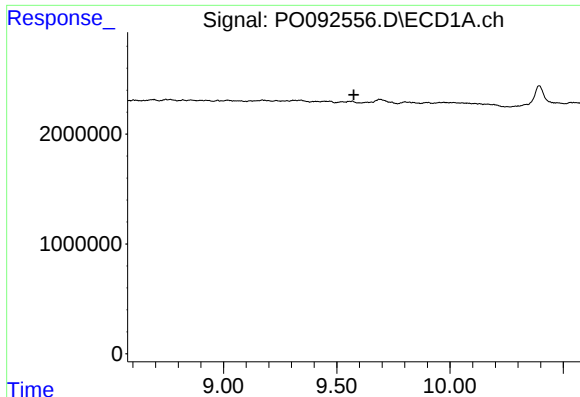

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2

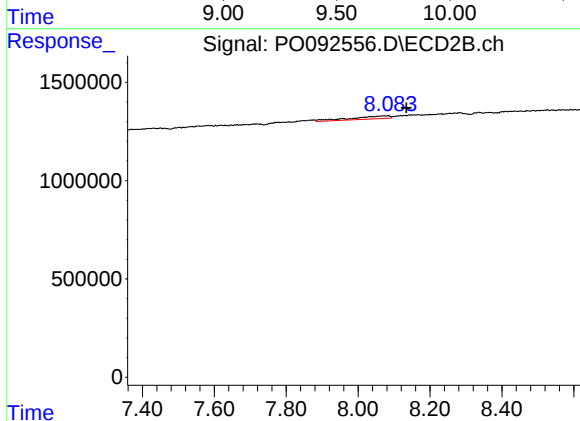


#40 AR-1262-5

R.T.: 8.083 min
Delta R.T.: -0.051 min
Response: 1075864
Conc: 20.88 ng/ml

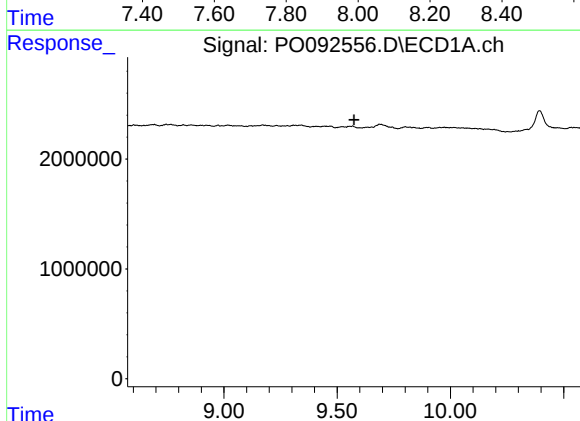

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.574 min
Response: 0
Conc: N.D.

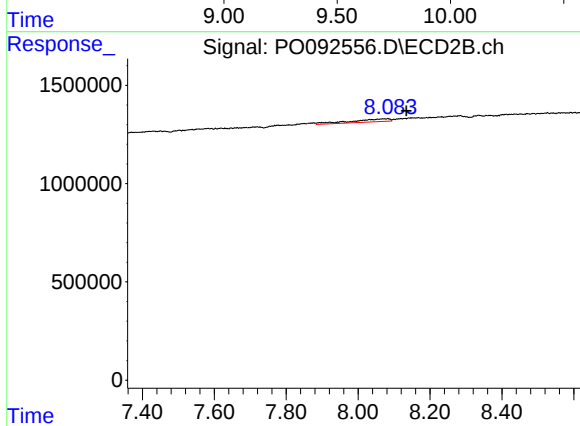

#44 AR-1268-4

R.T.: 8.083 min
Delta R.T.: -0.051 min
Response: 1075864
Conc: 17.14 ng/ml