

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 18:04
 Operator : YP/AJ
 Sample : 01592-03 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC226467-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 00:52:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.453	3.643	3748388	1718064	1.295	1.224
2)	SA Decachlor...	10.391	8.686	3925934	1943520	1.902	1.722
Target Compounds							
3)	L1 AR-1016-1	5.630	0.000	475215	0	5.196	N.D. #
4)	L1 AR-1016-2	5.648	0.000	237781	0	1.776	N.D. #
5)	L1 AR-1016-3	5.711	0.000	847909	0	9.853	N.D. #
13)	L3 AR-1232-3	5.648	0.000	237781	0	3.884	N.D. #
16)	L4 AR-1242-1	5.630	0.000	475215	0	6.093	N.D. #
17)	L4 AR-1242-2	5.648	0.000	237781	0	2.112	N.D. #
18)	L4 AR-1242-3	5.711	0.000	847909	0	11.680	N.D. #
21)	L5 AR-1248-1	5.630	0.000	475215	0	8.187	N.D. #
32)	L7 AR-1260-2	7.582f	0.000	409465	0	2.761	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021723\
Data File : PO092566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 18:04
Operator : YP/AJ
Sample : 01592-03 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC226467-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 00:52:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

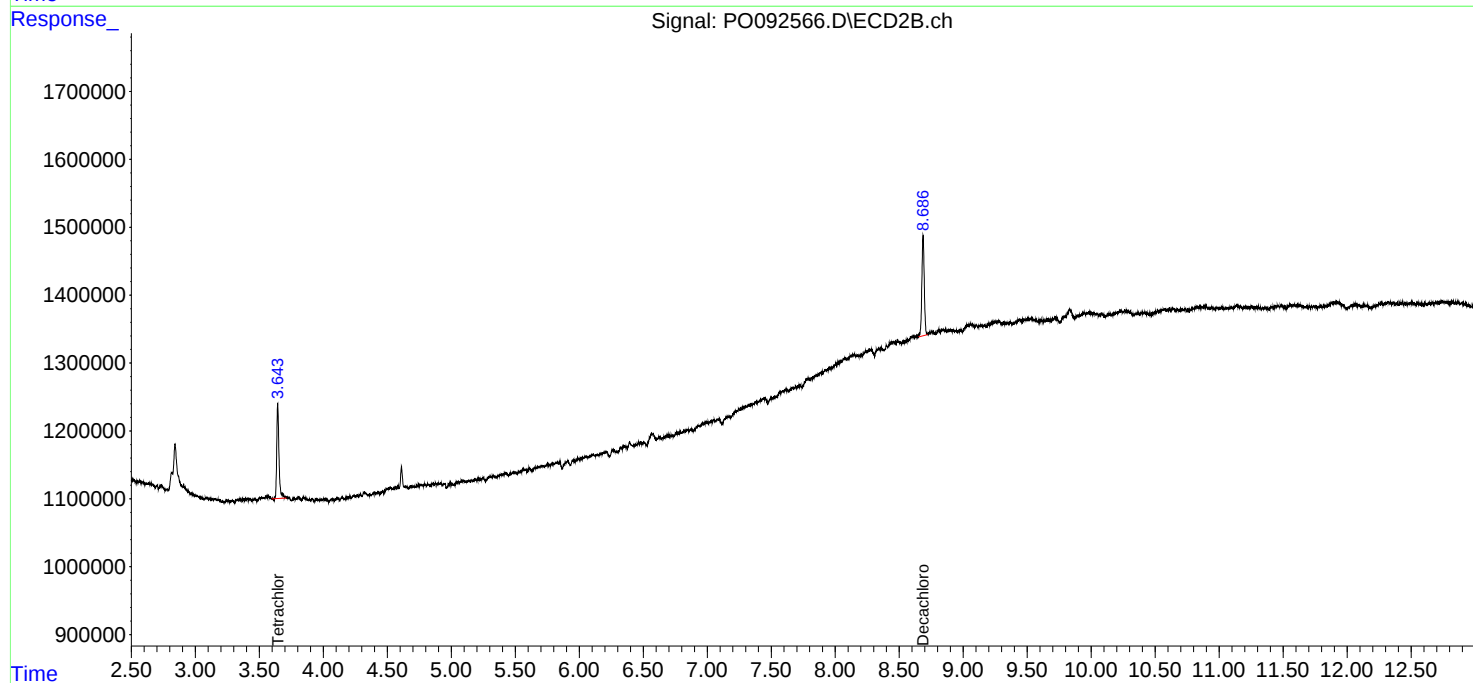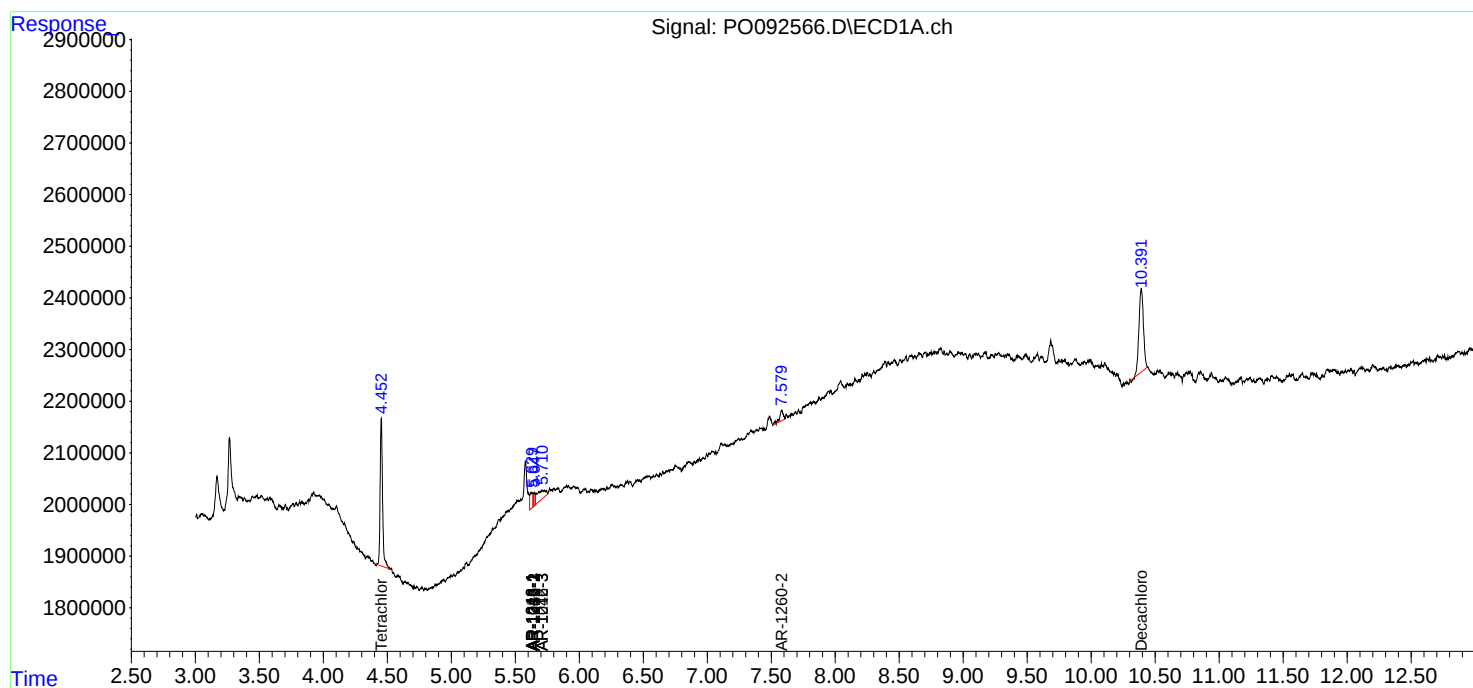


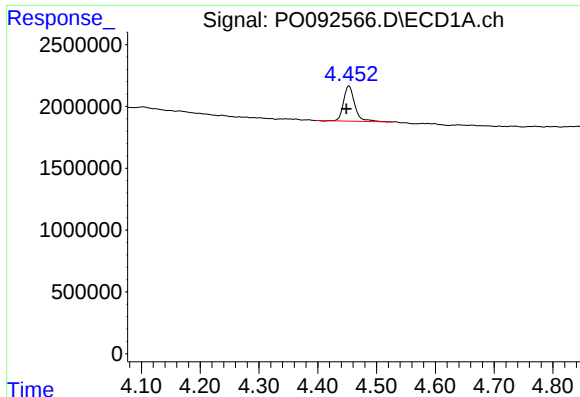

#1 Tetrachloro-m-xylene


R.T.: 4.453 min
Delta R.T.: 0.004 min
Response: 3748388
Conc: 1.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226467-1-1

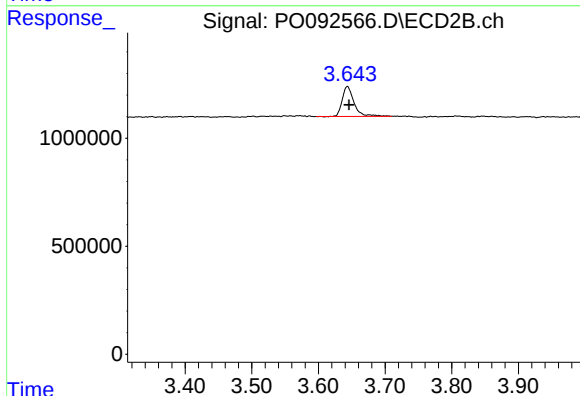


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.003 min
Response: 1718064
Conc: 1.22 ng/ml

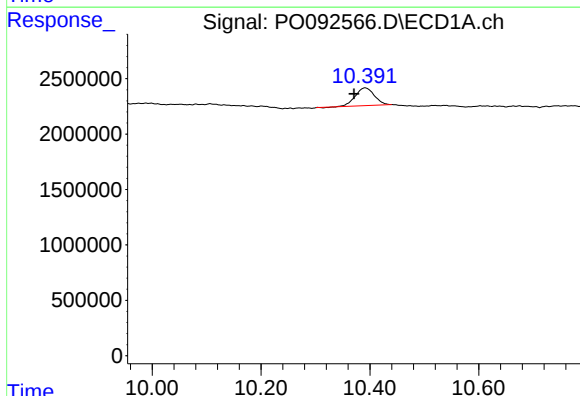


#2 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: 0.020 min
Response: 3925934
Conc: 1.90 ng/ml

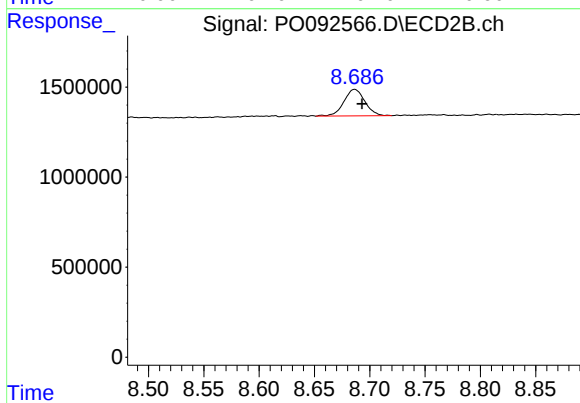

#2 Decachlorobiphenyl


R.T.: 8.686 min
Delta R.T.: -0.007 min
Response: 1943520
Conc: 1.72 ng/ml

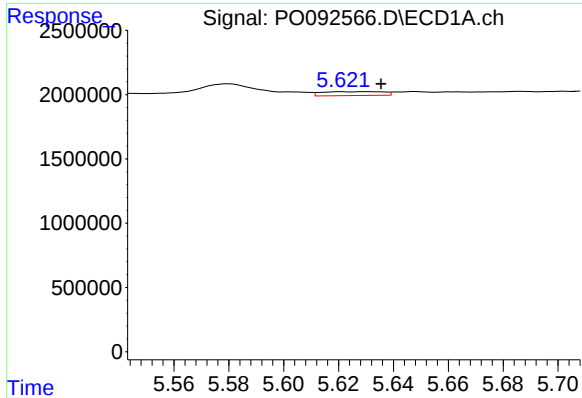

#3 AR-1016-1


R.T.: 5.630 min
Delta R.T.: -0.005 min
Response: 475215
Conc: 5.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226467-1-1

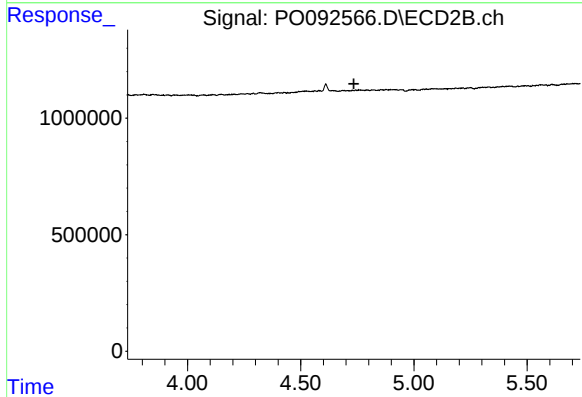


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

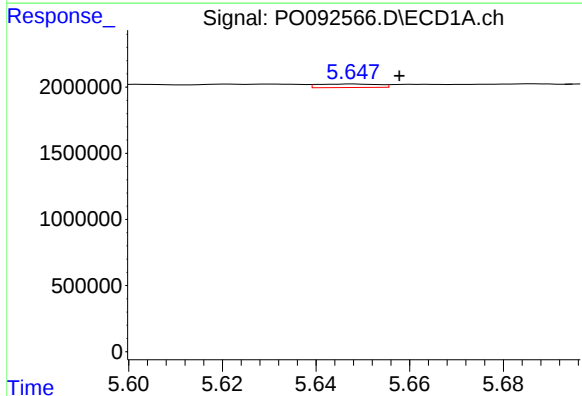


#4 AR-1016-2

R.T.: 5.648 min
Delta R.T.: -0.010 min
Response: 237781
Conc: 1.78 ng/ml

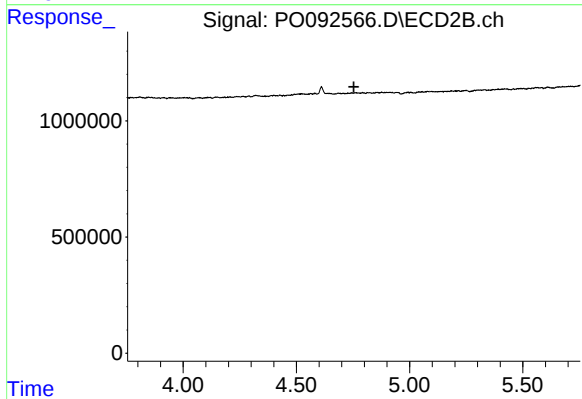

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.754 min
Response: 0
Conc: N.D.

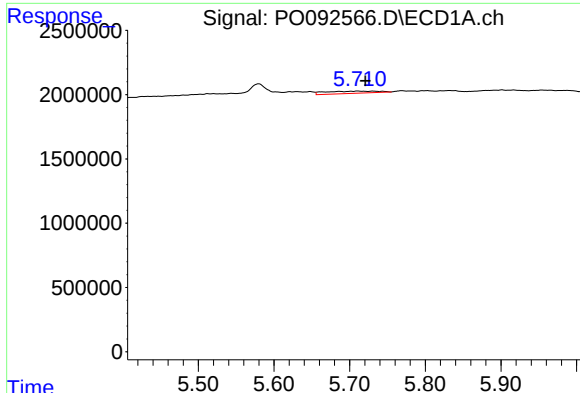

#5 AR-1016-3


R.T.: 5.711 min
Delta R.T.: -0.010 min
Response: 847909
Conc: 9.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226467-1-1

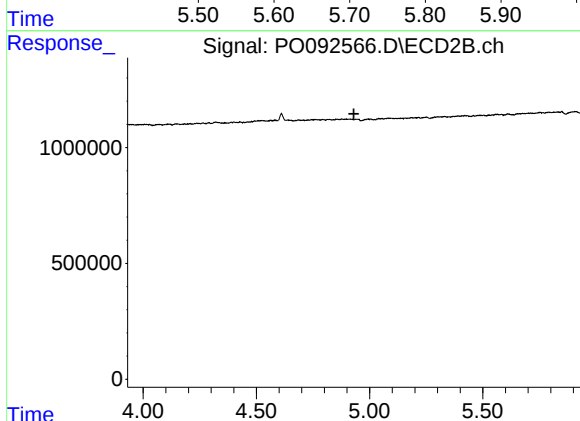


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.931 min
Response: 0
Conc: N.D.

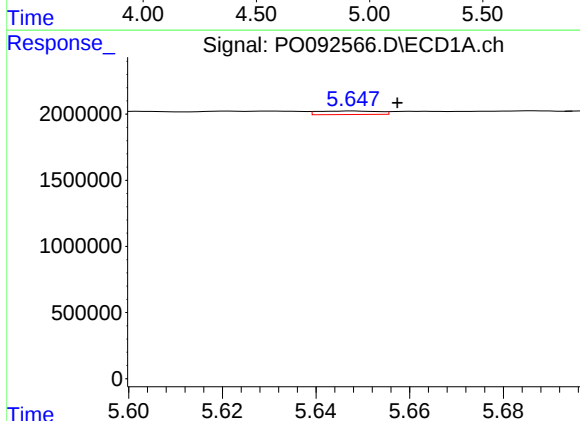


#13 AR-1232-3

R.T.: 5.648 min
Delta R.T.: -0.009 min
Response: 237781
Conc: 3.88 ng/ml

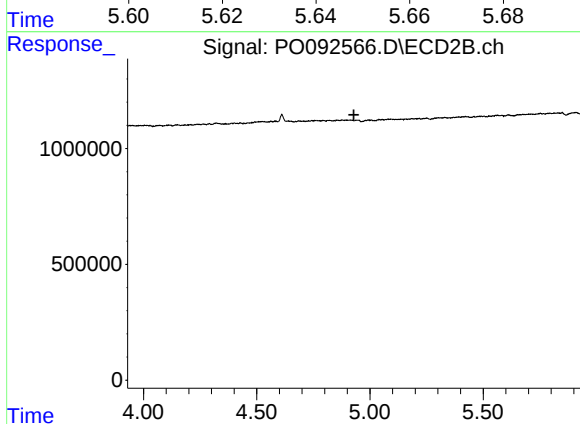

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

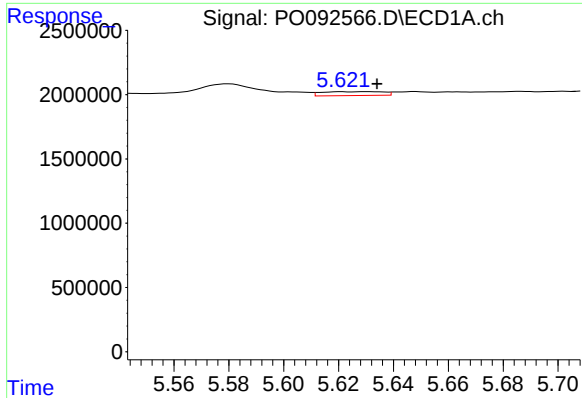

#16 AR-1242-1


R.T.: 5.630 min
Delta R.T.: -0.004 min
Response: 475215
Conc: 6.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226467-1-1

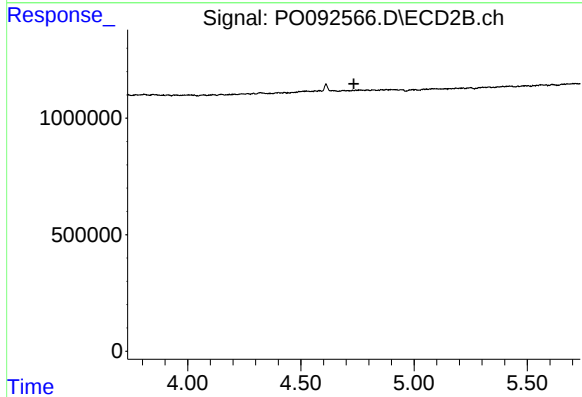


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

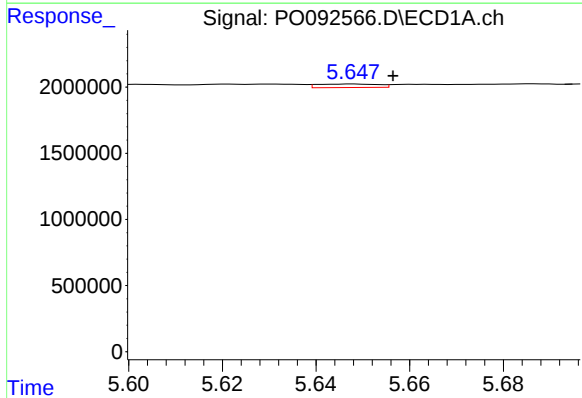


#17 AR-1242-2

R.T.: 5.648 min
Delta R.T.: -0.009 min
Response: 237781
Conc: 2.11 ng/ml

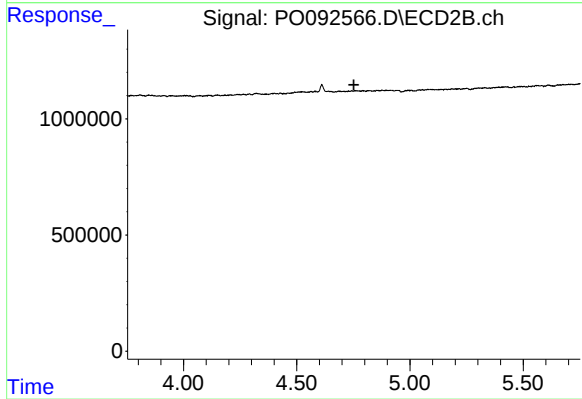

#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.753 min
Response: 0
Conc: N.D.

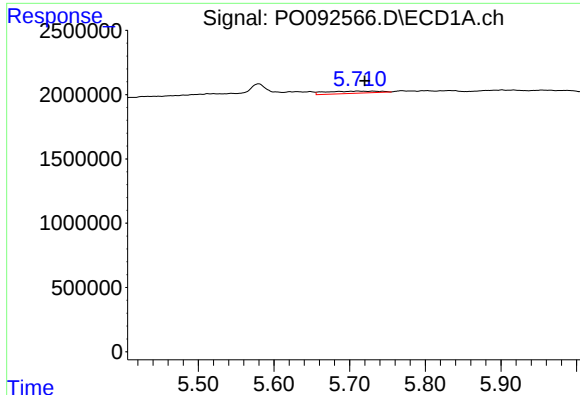

#18 AR-1242-3

R.T.: 5.711 min
Delta R.T.: -0.009 min
Response: 847909
Conc: 11.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226467-1-1

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

#21 AR-1248-1

R.T.: 5.630 min
Delta R.T.: -0.005 min
Response: 475215
Conc: 8.19 ng/ml

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

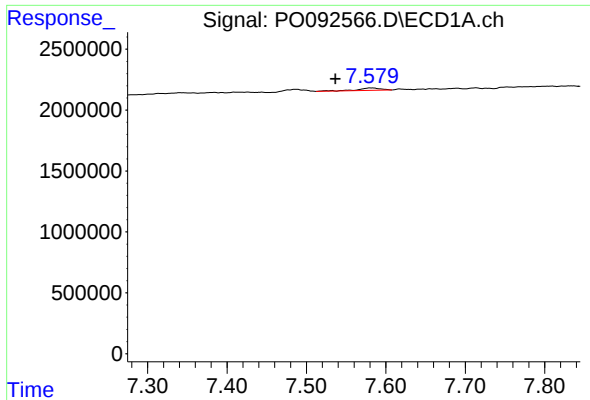

#32 AR-1260-2

R.T.: 7.582 min
Delta R.T.: 0.045 min
Response: 409465
Conc: 2.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226467-1-1

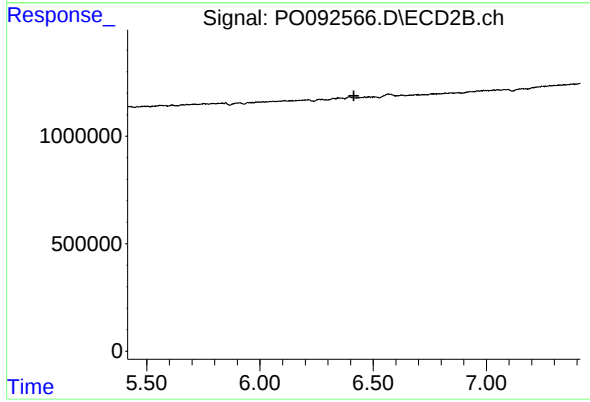

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.