

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2023 06:57
 Operator : YP/AJ
 Sample : 01582-04
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 08:01:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.640	55230479	23548666	19.079	16.771
2) SA Decachlor...	10.379	8.676	45736854	21602826	22.160	19.136
Target Compounds						
3) L1 AR-1016-1	5.573f	0.000	720362	0	7.876	N.D. #
8) L2 AR-1221-1	4.654	3.939f	1781983	560448	47.136	29.605 #
9) L2 AR-1221-2	4.756	3.939	813725	560448	29.403	39.878 #
10) L2 AR-1221-3	4.756f	0.000	813725	0	9.643	N.D. #
11) L3 AR-1232-1	4.756f	0.000	813725	0	11.760	N.D. #
12) L3 AR-1232-2	5.331	0.000	850581	0	24.345	N.D. #
16) L4 AR-1242-1	5.573f	0.000	720362	0	9.237	N.D. #
21) L5 AR-1248-1	5.573f	0.000	720362	0	12.411	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
Data File : P0092605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2023 06:57
Operator : YP/AJ
Sample : 01582-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 08:01:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

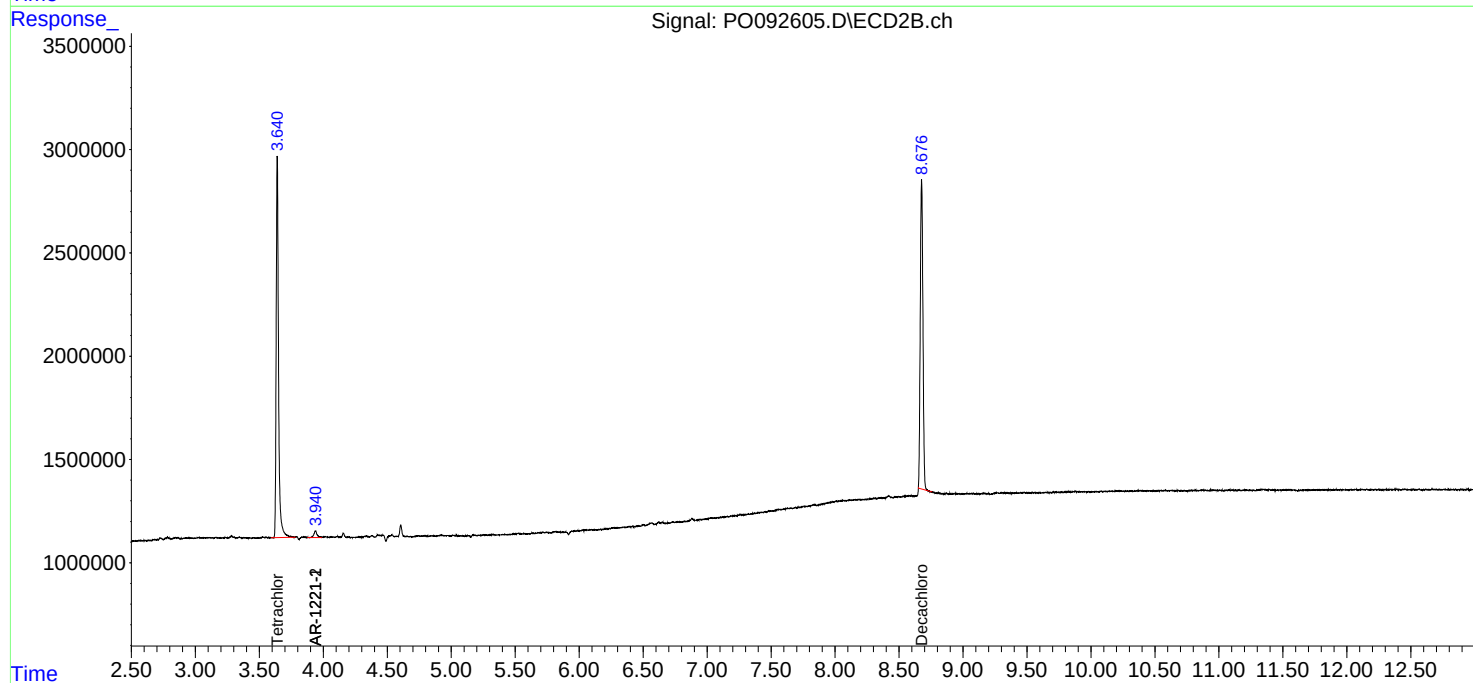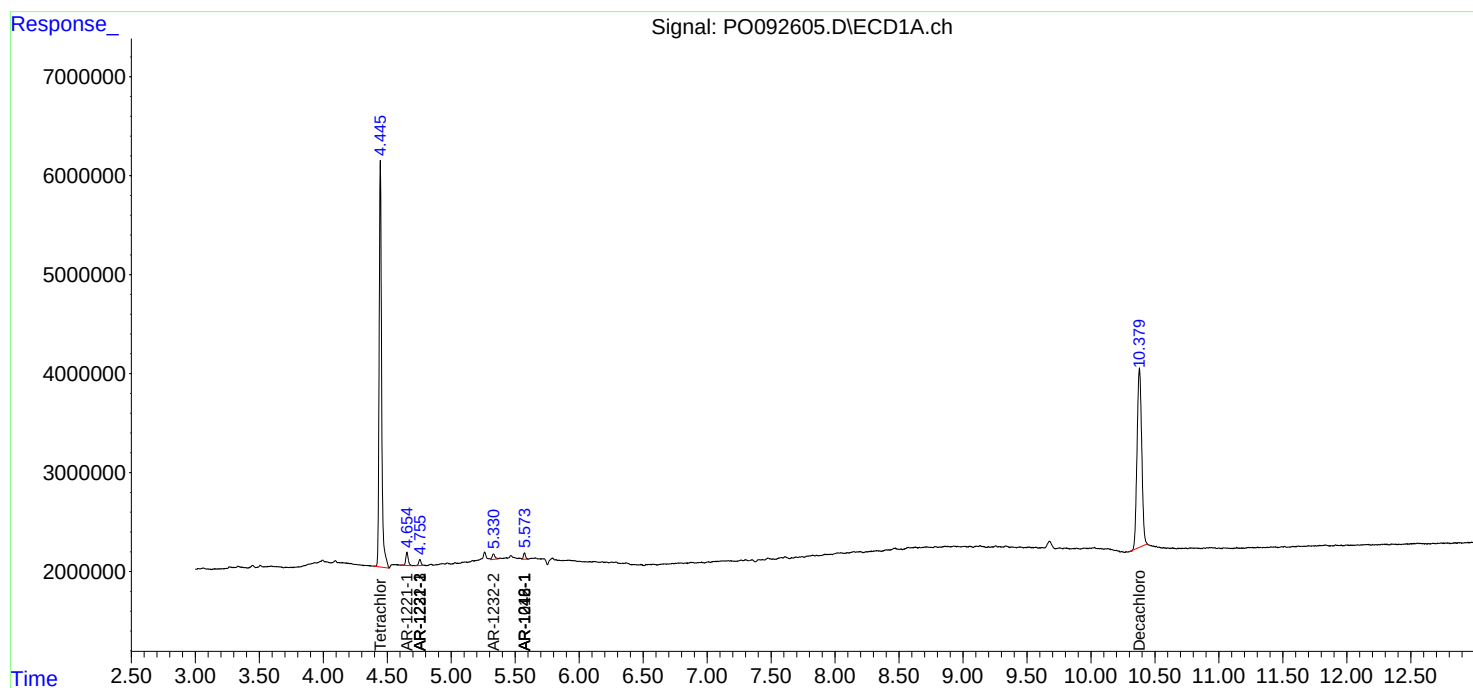


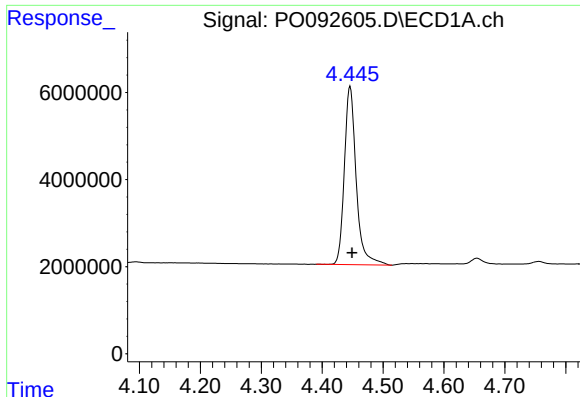

#1 Tetrachloro-m-xylene


R.T.: 4.446 min
Delta R.T.: -0.003 min
Response: 55230479
Conc: 19.08 ng/ml

Instrument :
ECD_O
ClientSampleId :

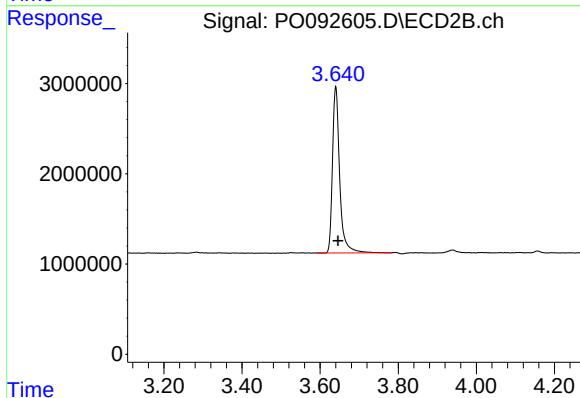


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: -0.006 min
Response: 23548666
Conc: 16.77 ng/ml

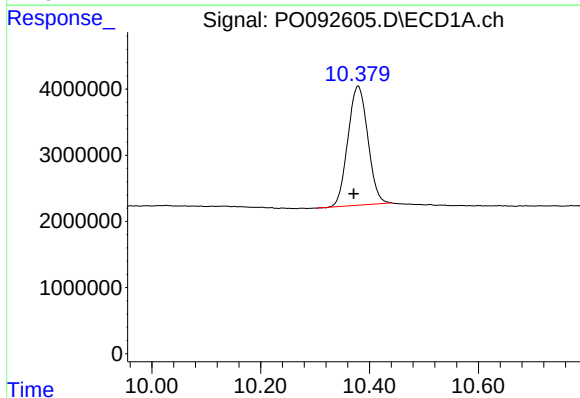


#2 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: 0.008 min
Response: 45736854
Conc: 22.16 ng/ml

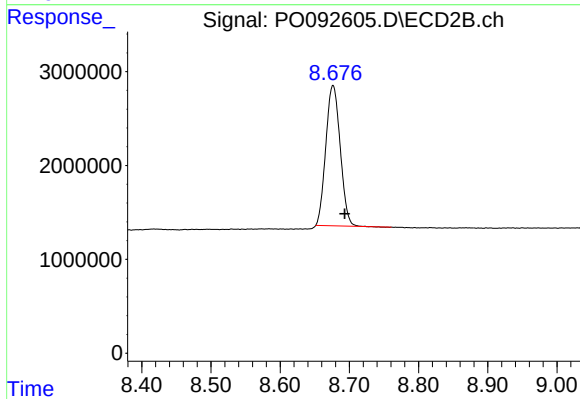

#2 Decachlorobiphenyl


R.T.: 8.676 min
Delta R.T.: -0.017 min
Response: 21602826
Conc: 19.14 ng/ml

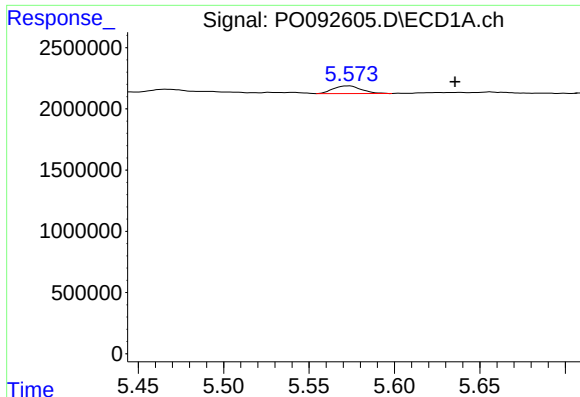

#3 AR-1016-1


R.T.: 5.573 min
Delta R.T.: -0.062 min
Response: 720362
Conc: 7.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

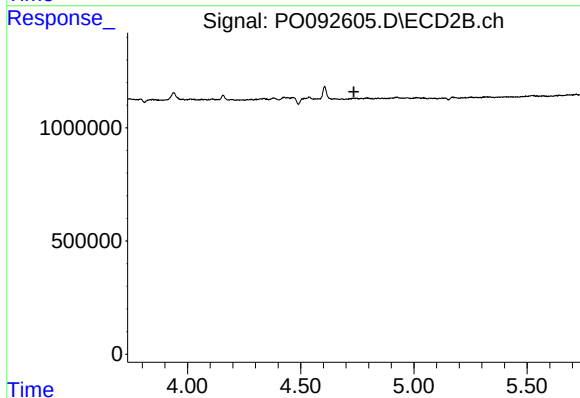


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

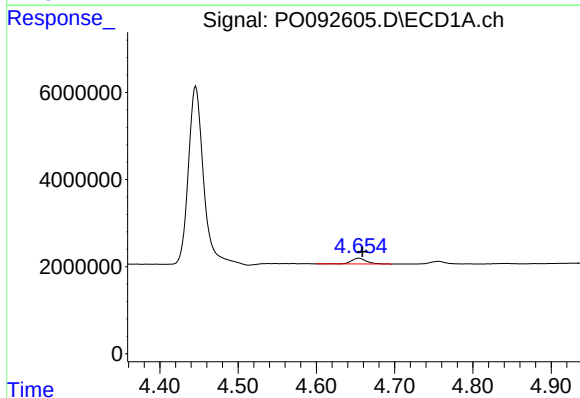


#8 AR-1221-1

R.T.: 4.654 min
Delta R.T.: -0.005 min
Response: 1781983
Conc: 47.14 ng/ml

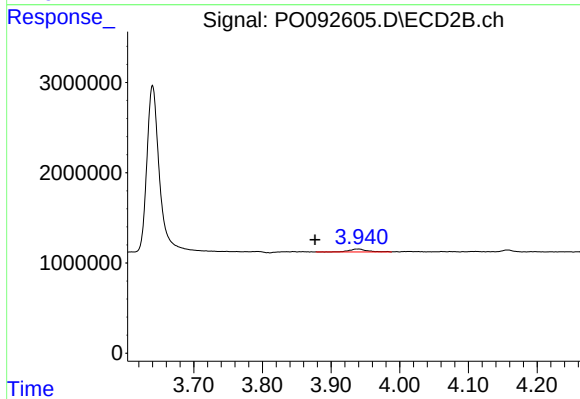

#8 AR-1221-1


R.T.: 3.939 min
Delta R.T.: 0.063 min
Response: 560448
Conc: 29.61 ng/ml

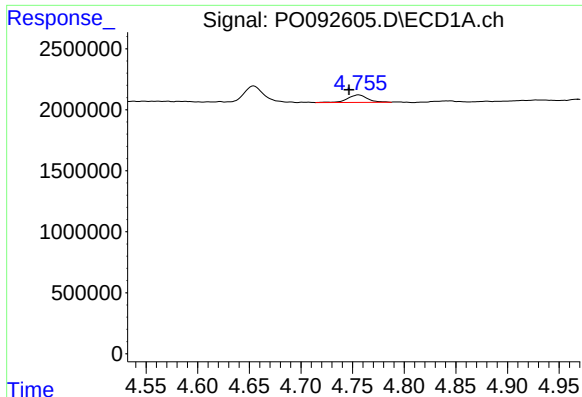

#9 AR-1221-2


R.T.: 4.756 min
Delta R.T.: 0.009 min
Response: 813725
Conc: 29.40 ng/ml

Instrument :
ECD_O
ClientSampleId :

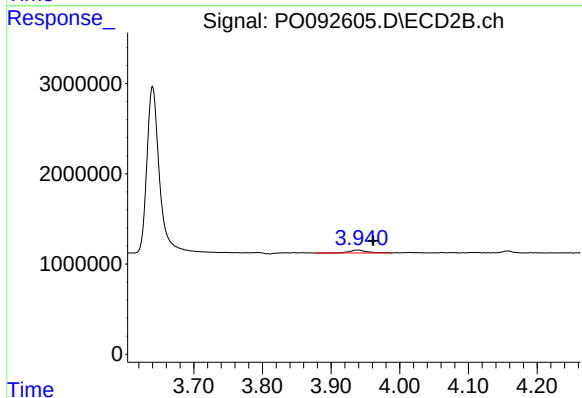


#9 AR-1221-2

R.T.: 3.939 min
Delta R.T.: -0.022 min
Response: 560448
Conc: 39.88 ng/ml

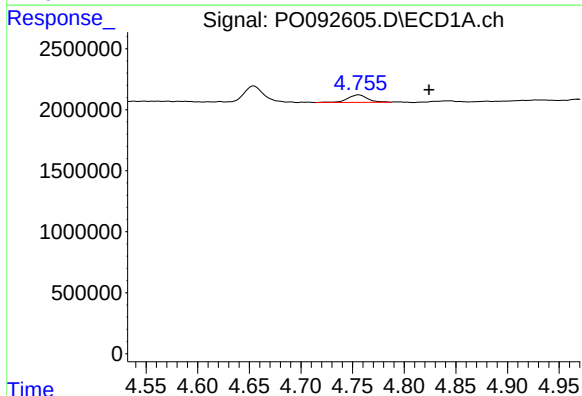


#10 AR-1221-3

R.T.: 4.756 min
Delta R.T.: -0.068 min
Response: 813725
Conc: 9.64 ng/ml

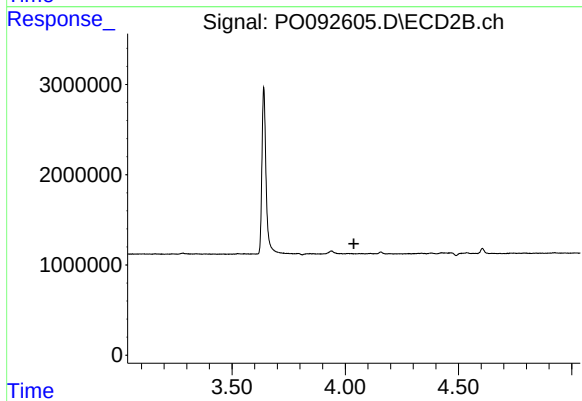

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.038 min
Response: 0
Conc: N.D.

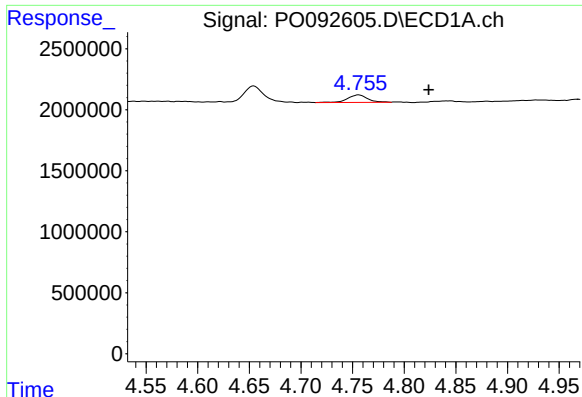

#11 AR-1232-1


R.T.: 4.756 min
Delta R.T.: -0.068 min
Response: 813725
Conc: 11.76 ng/ml

Instrument :
ECD_O
ClientSampleId :

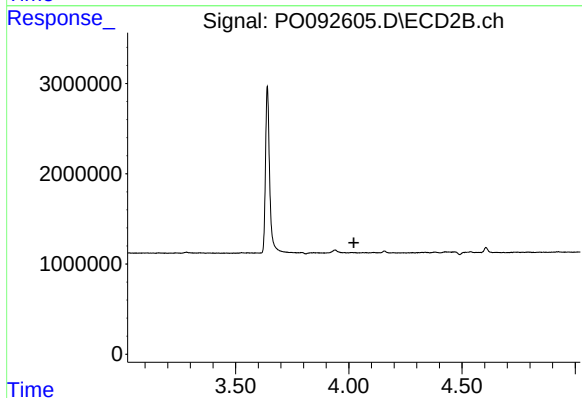


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.022 min
Response: 0
Conc: N.D.

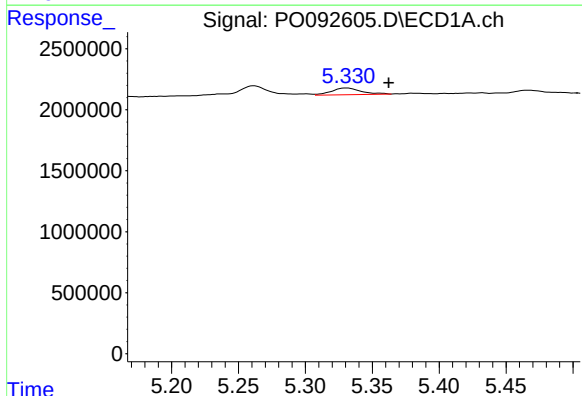


#12 AR-1232-2

R.T.: 5.331 min
Delta R.T.: -0.032 min
Response: 850581
Conc: 24.34 ng/ml

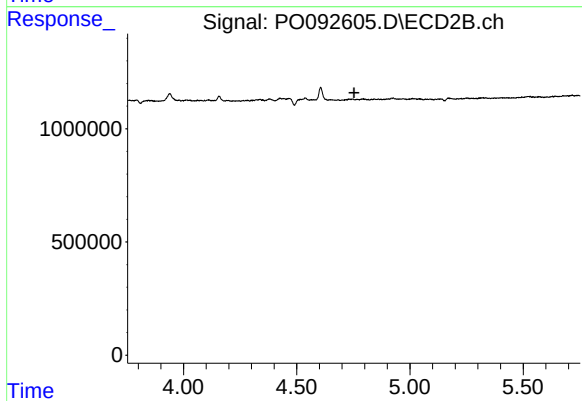

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.753 min
Response: 0
Conc: N.D.

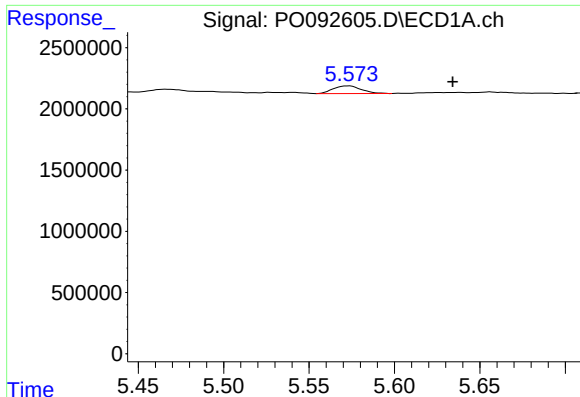

#16 AR-1242-1


R.T.: 5.573 min
Delta R.T.: -0.061 min
Response: 720362
Conc: 9.24 ng/ml

Instrument :
ECD_O
ClientSampleId :

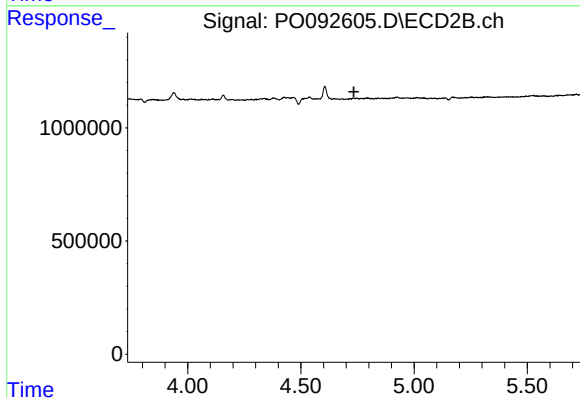


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

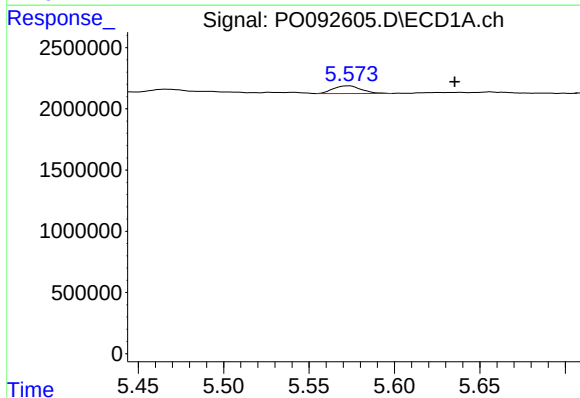

#21 AR-1248-1

R.T.: 5.573 min
Delta R.T.: -0.062 min
Response: 720362
Conc: 12.41 ng/ml

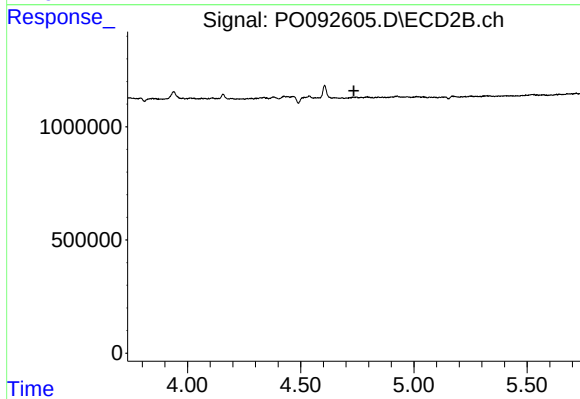

#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.