

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2023 13:23
 Operator : YP/AJ
 Sample : 01593-10
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 03:29:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.445	3.640	41404083	17412855	14.302	12.401
2)	SA Decachlor...	10.378	8.676	30878934	14801198	14.961	13.111
Target Compounds							
3)	L1 AR-1016-1	5.571f	0.000	4566846	0	49.934	N.D. #
8)	L2 AR-1221-1	4.653	3.938f	2054406	1105920	54.342	58.420
9)	L2 AR-1221-2	0.000	3.938	0	1105920	N.D.	78.691 #
16)	L4 AR-1242-1	5.571f	0.000	4566846	0	58.558	N.D. #
21)	L5 AR-1248-1	5.571f	0.000	4566846	0	78.678	N.D. #
32)	L7 AR-1260-2	7.527	6.478f	881119	531168	5.942	6.063
40)	L8 AR-1262-5	0.000	8.073f	0	336456	N.D.	6.530 #
44)	L9 AR-1268-4	0.000	8.073f	0	336456	N.D.	5.360 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
Data File : P0092626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2023 13:23
Operator : YP/AJ
Sample : 01593-10
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 03:29:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

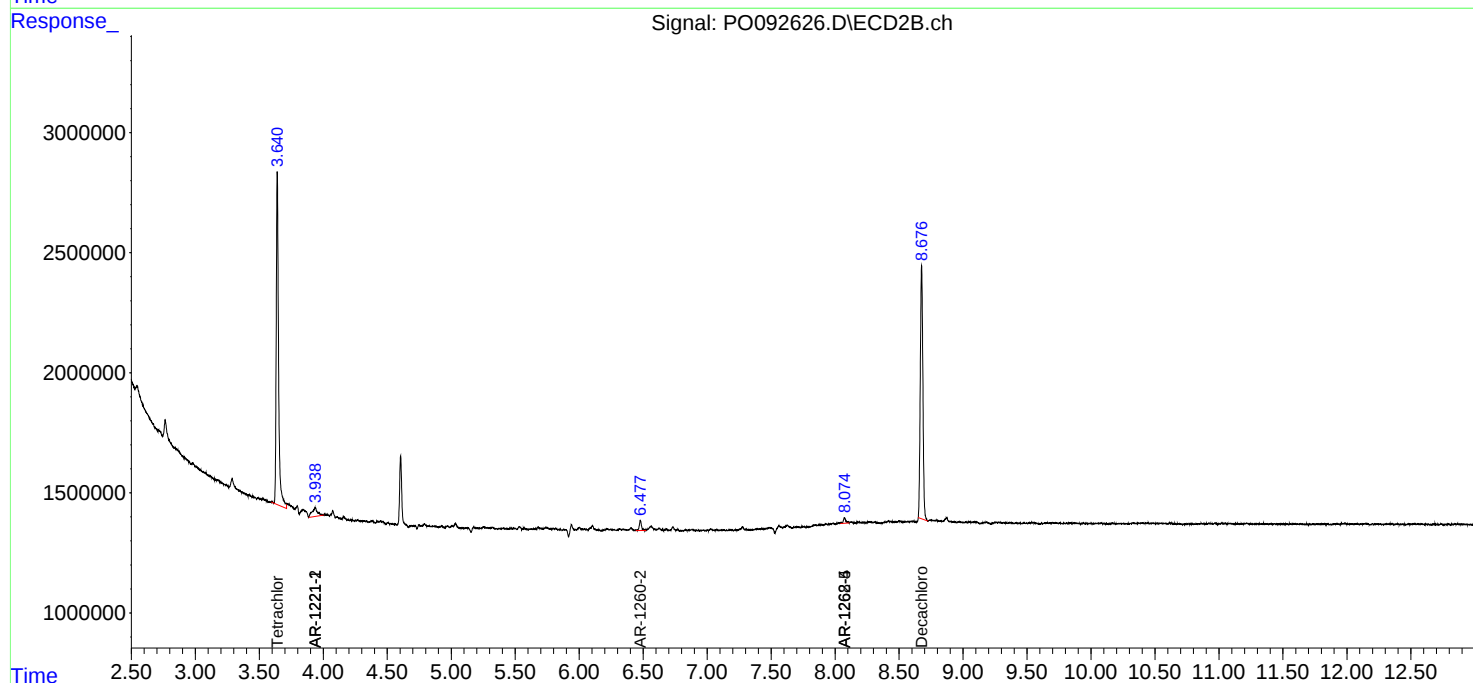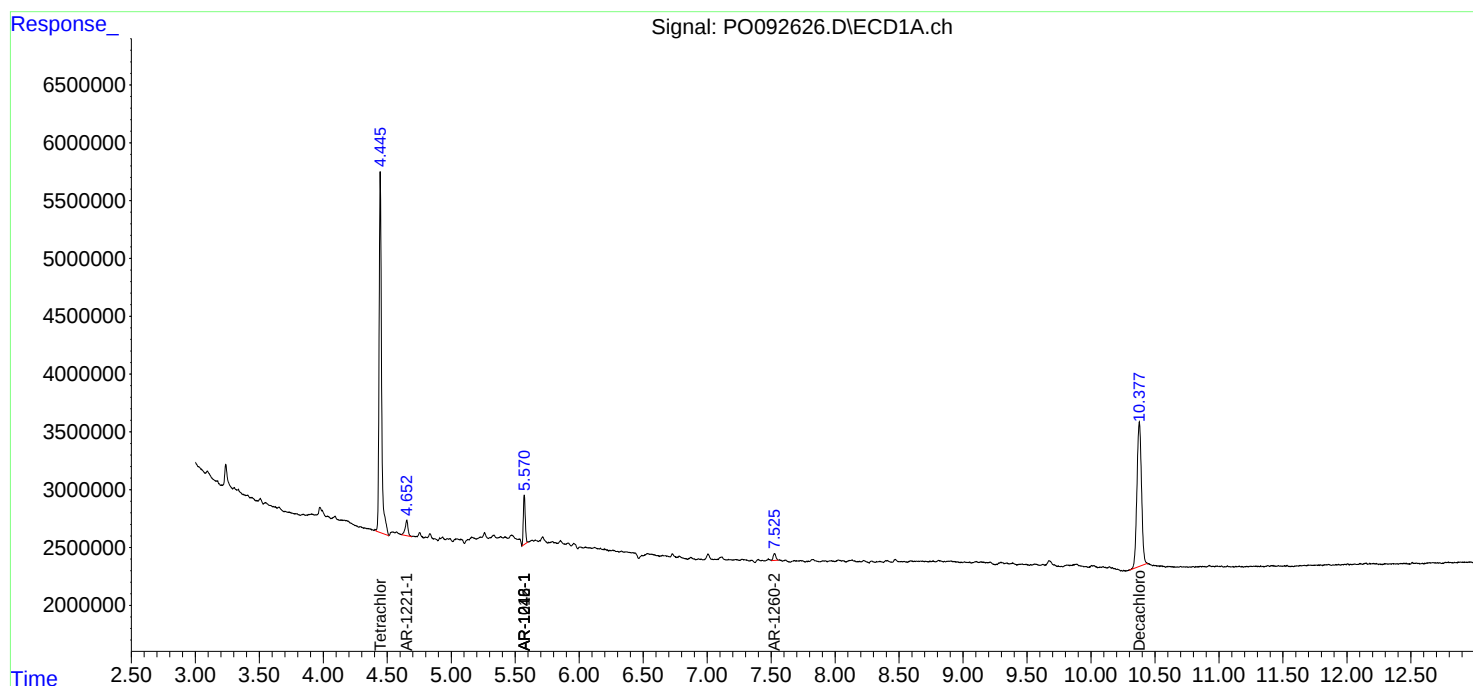


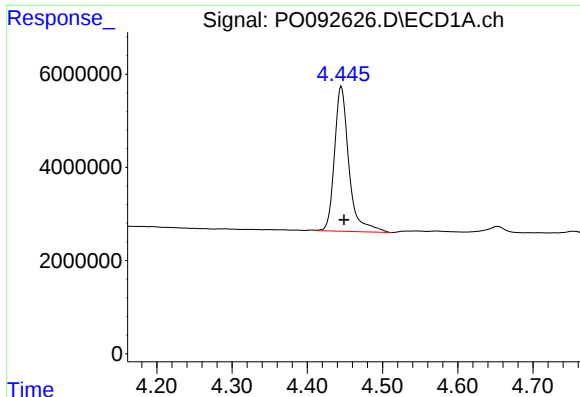

#1 Tetrachloro-m-xylene


R.T.: 4.445 min
Delta R.T.: -0.004 min
Response: 41404083
Conc: 14.30 ng/ml

Instrument :
ECD_O
ClientSampleId :

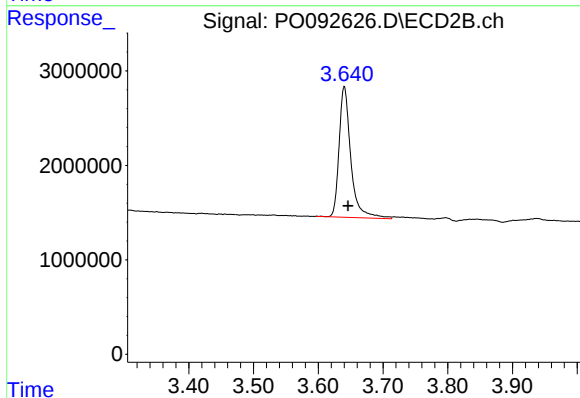


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: -0.006 min
Response: 17412855
Conc: 12.40 ng/ml

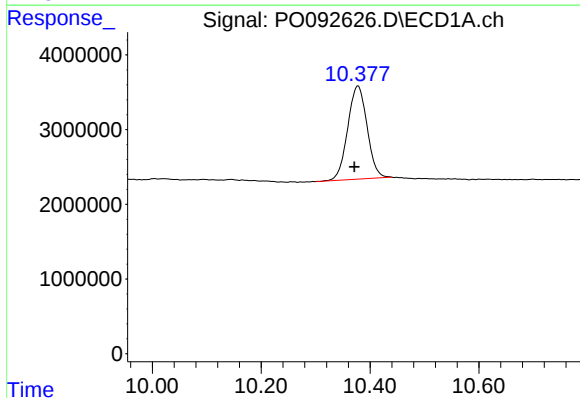


#2 Decachlorobiphenyl

R.T.: 10.378 min
Delta R.T.: 0.007 min
Response: 30878934
Conc: 14.96 ng/ml

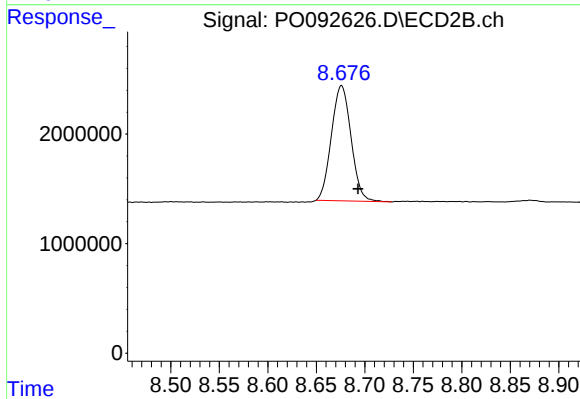

#2 Decachlorobiphenyl


R.T.: 8.676 min
Delta R.T.: -0.017 min
Response: 14801198
Conc: 13.11 ng/ml

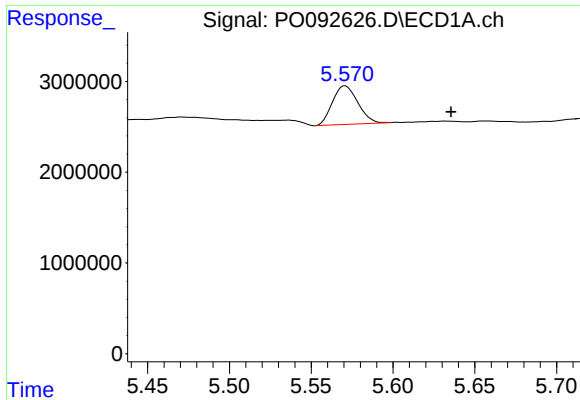

#3 AR-1016-1


R.T.: 5.571 min
Delta R.T.: -0.065 min
Response: 4566846
Conc: 49.93 ng/ml

Instrument :
ECD_O
ClientSampleId :

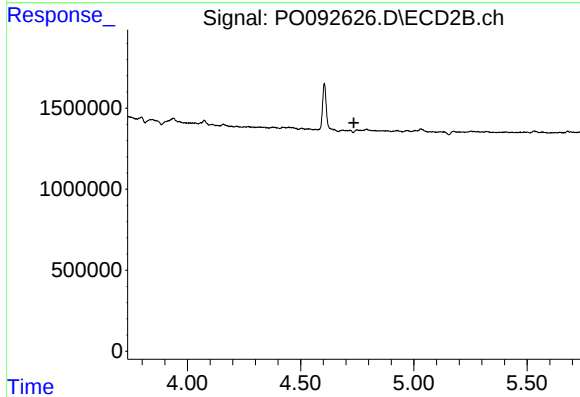


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.735 min
Response: 0
Conc: N.D.

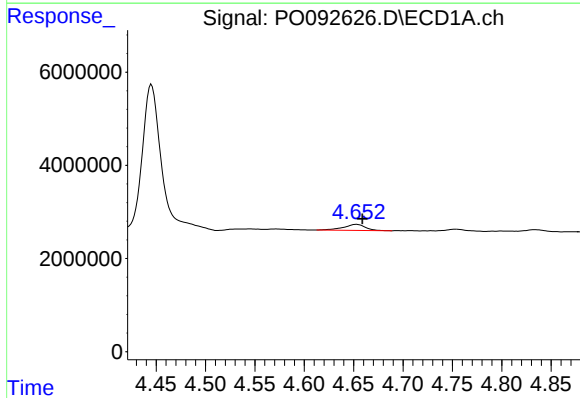


#8 AR-1221-1

R.T.: 4.653 min
Delta R.T.: -0.006 min
Response: 2054406
Conc: 54.34 ng/ml

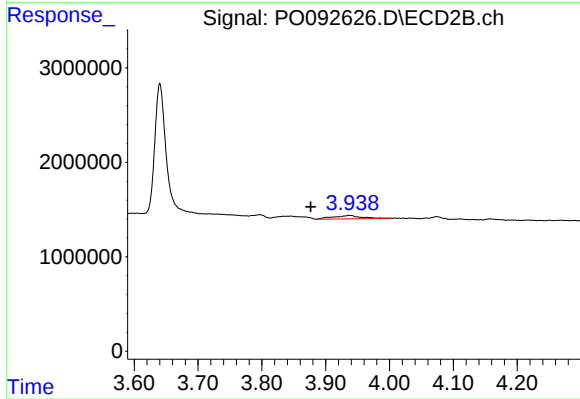

#8 AR-1221-1


R.T.: 3.938 min
Delta R.T.: 0.061 min
Response: 1105920
Conc: 58.42 ng/ml

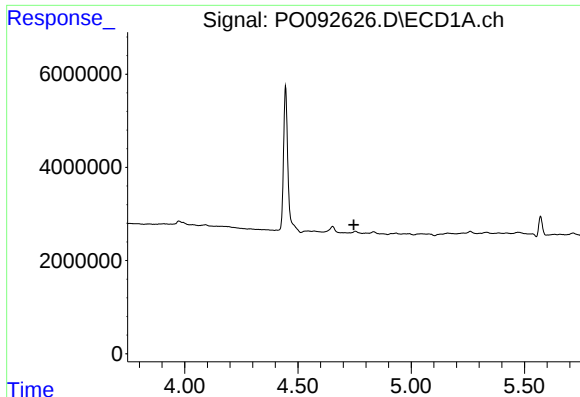

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

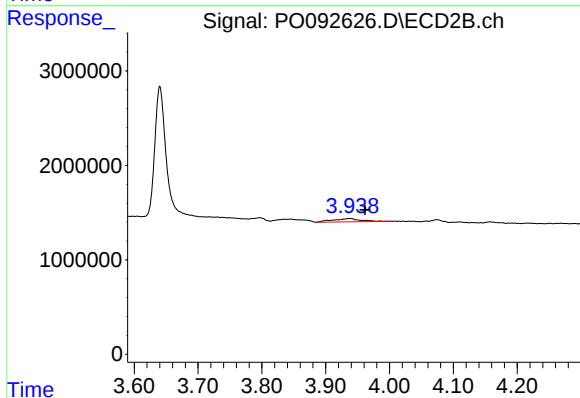


#9 AR-1221-2

R.T.: 3.938 min
Delta R.T.: -0.024 min
Response: 1105920
Conc: 78.69 ng/ml

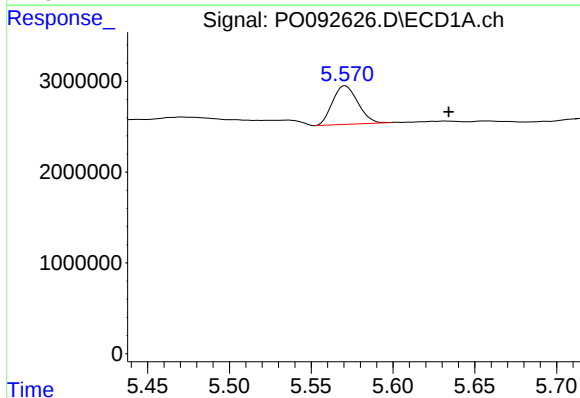


#16 AR-1242-1

R.T.: 5.571 min
Delta R.T.: -0.063 min
Response: 4566846
Conc: 58.56 ng/ml

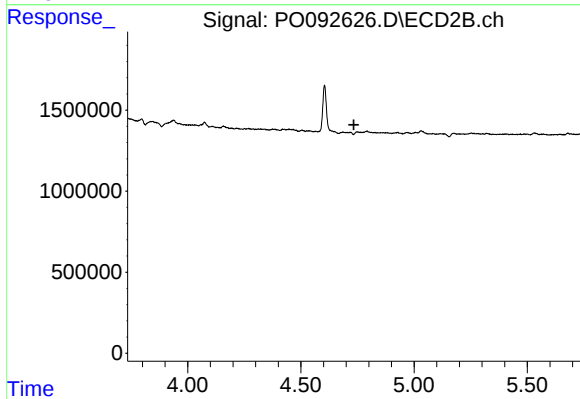

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 4.734 min
Response: 0
Conc: N.D.

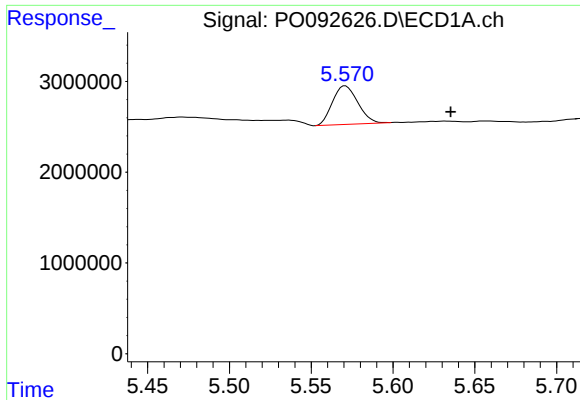

#21 AR-1248-1


R.T.: 5.571 min
Delta R.T.: -0.064 min
Response: 4566846
Conc: 78.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

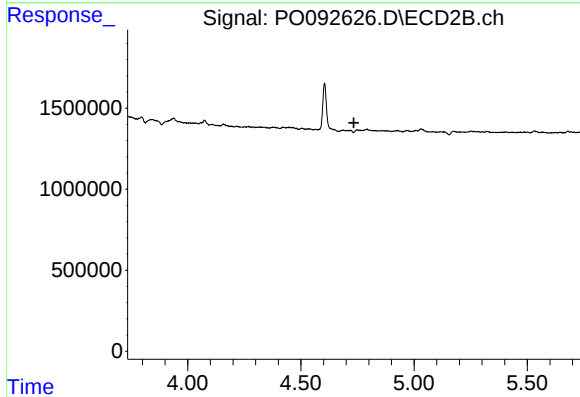


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

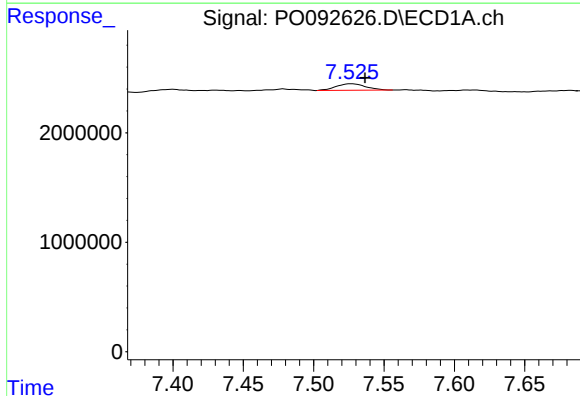


#32 AR-1260-2

R.T.: 7.527 min
Delta R.T.: -0.010 min
Response: 881119
Conc: 5.94 ng/ml

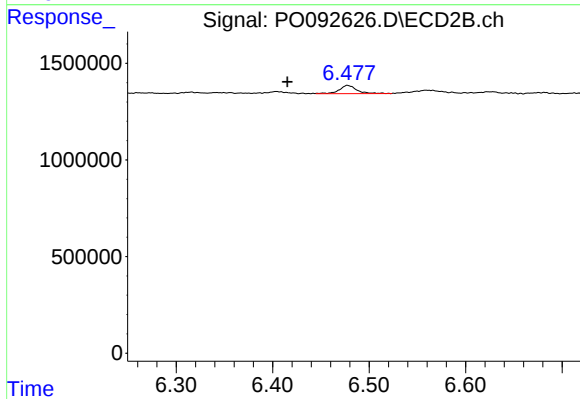

#32 AR-1260-2


R.T.: 6.478 min
Delta R.T.: 0.062 min
Response: 531168
Conc: 6.06 ng/ml

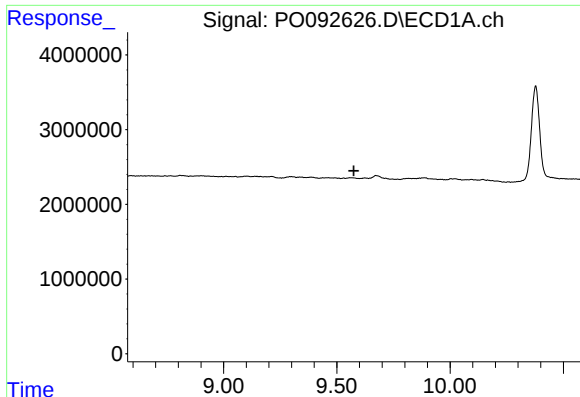

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.575 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

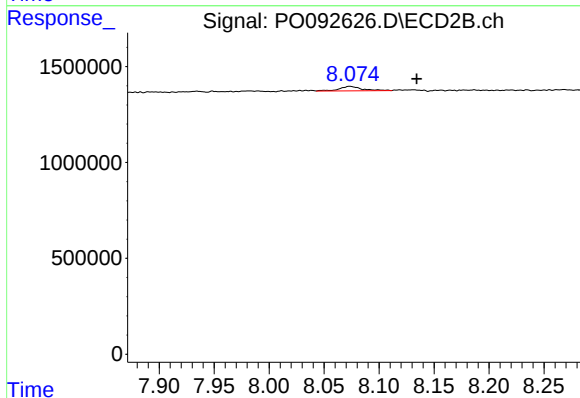


#40 AR-1262-5

R.T.: 8.073 min
Delta R.T.: -0.061 min
Response: 336456
Conc: 6.53 ng/ml

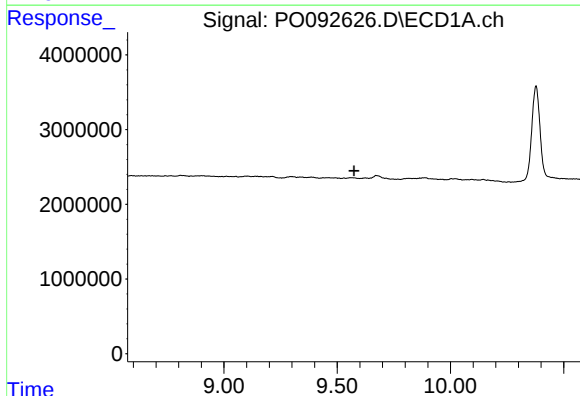

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.574 min
Response: 0
Conc: N.D.

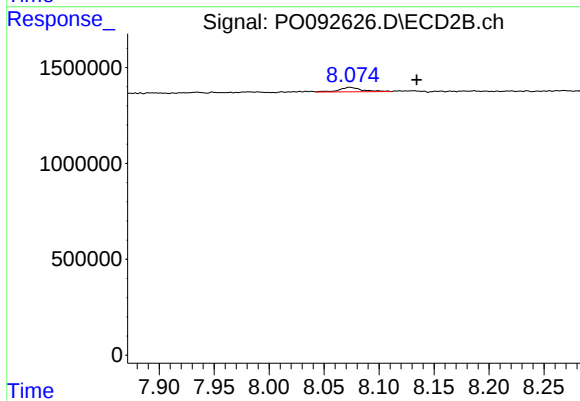

#44 AR-1268-4

R.T.: 8.073 min
Delta R.T.: -0.061 min
Response: 336456
Conc: 5.36 ng/ml