

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 13:49
 Operator : YP/AJ
 Sample : 01590-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260967LOZ-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2023
 Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 14:14:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.453	3.644	3537871	1676444	1.222	1.194
2) SA Decachlor...	10.393	8.687	4128444	1908032	2.000	1.690
Target Compounds						
26) L6 AR-1254-1	6.516	5.537	14872941	8360993	134.335	106.659
27) L6 AR-1254-2	6.740	5.685	20690811	8011232	127.285	115.785
28) L6 AR-1254-3	7.114	6.091	15181327	9109692	92.047	85.349
29) L6 AR-1254-4	7.407	6.321	9812116	4336557	89.702	73.633
30) L6 AR-1254-5	7.836	6.741	10929101	6404016	77.677m	70.362

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021723\
Data File : PO092553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 13:49
Operator : YP/AJ
Sample : 01590-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC260967LOZ-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 14:14:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

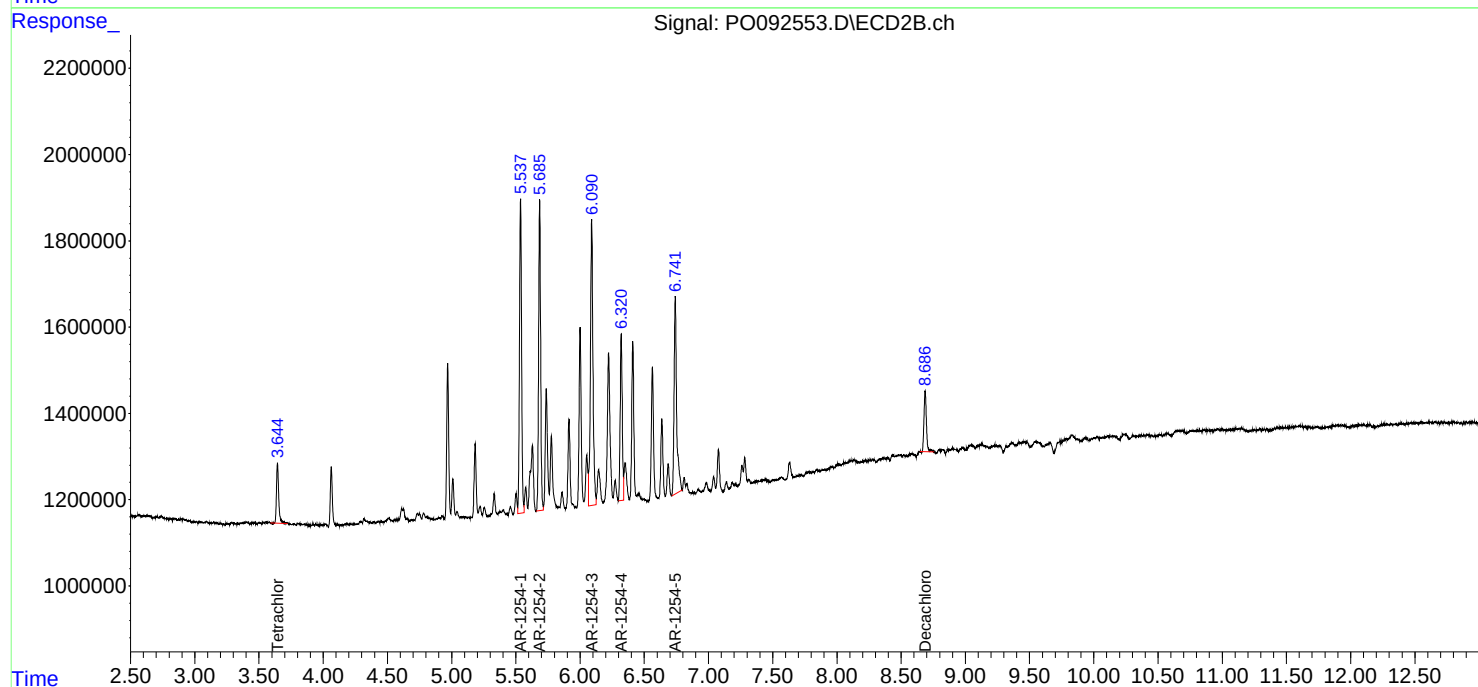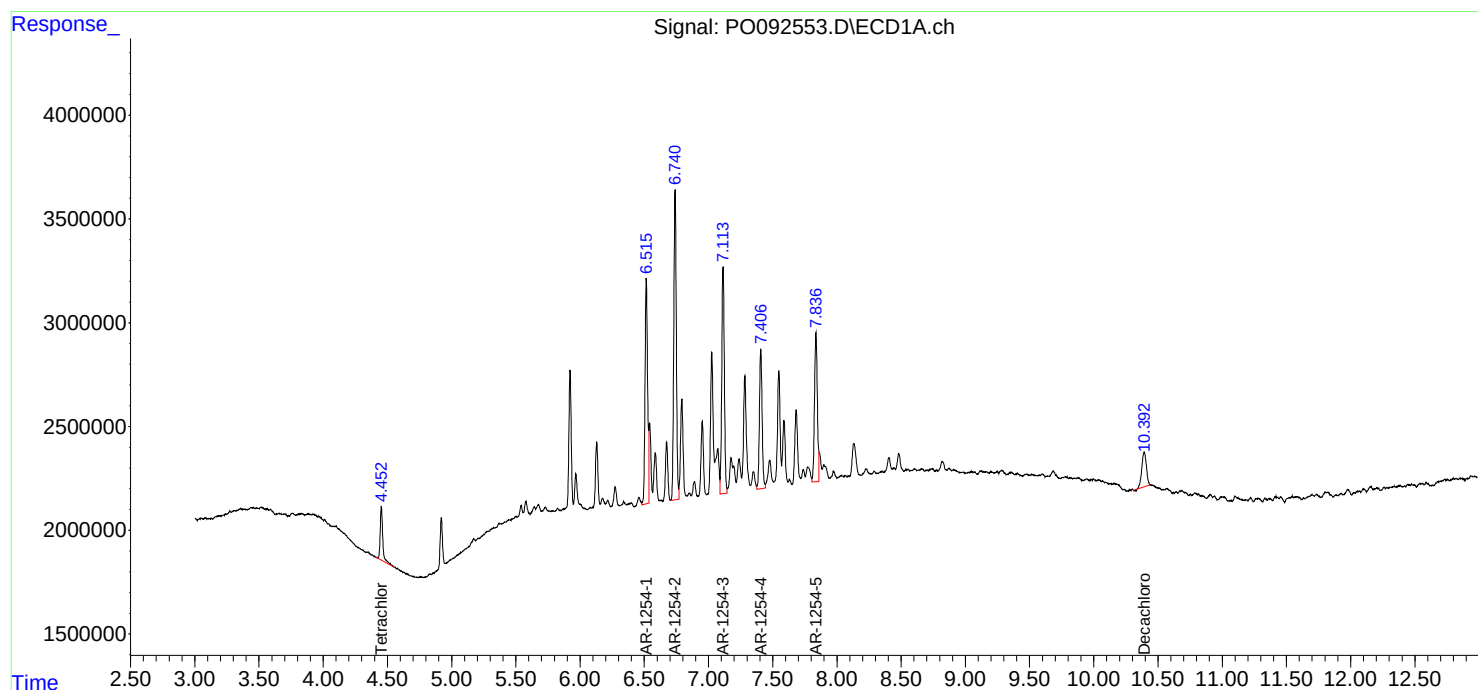

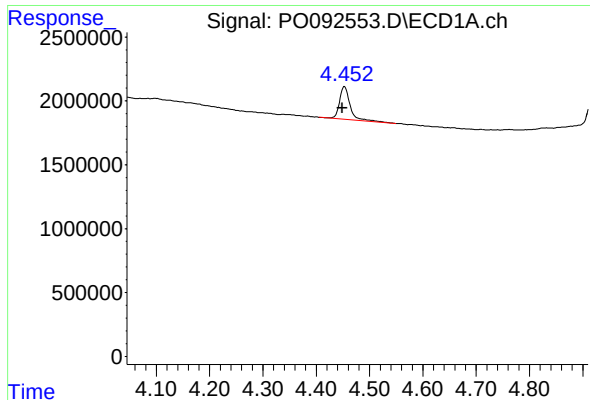


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: 0.004 min
Response: 3537871
Conc: 1.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260967LOZ-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

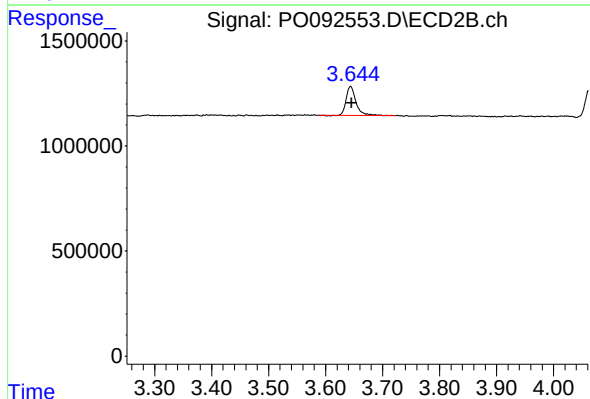


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.002 min
Response: 1676444
Conc: 1.19 ng/ml

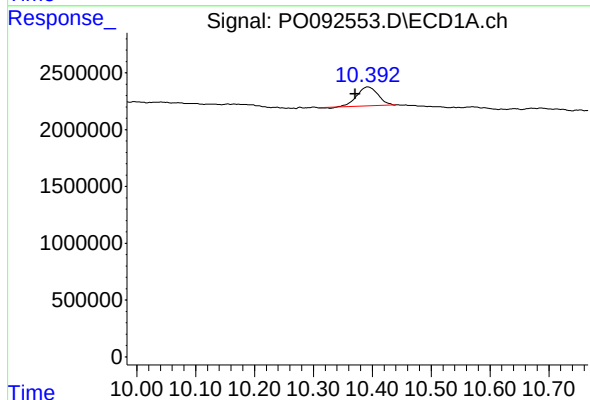


#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.022 min
Response: 4128444
Conc: 2.00 ng/ml

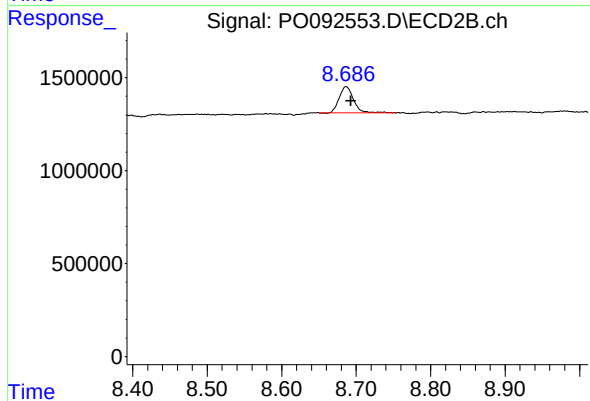

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: -0.006 min
Response: 1908032
Conc: 1.69 ng/ml

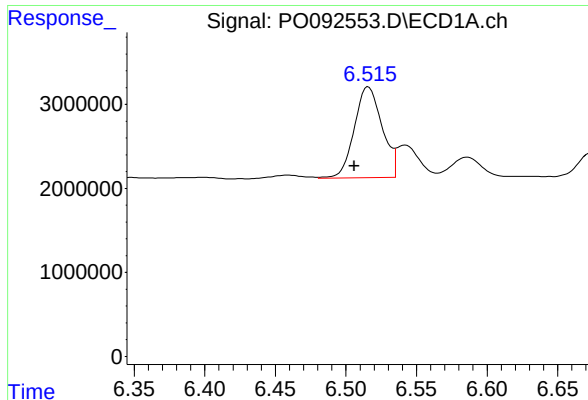


#26 AR-1254-1

R.T.: 6.516 min
Delta R.T.: 0.010 min
Response: 14872941
Conc: 134.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260967LOZ-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

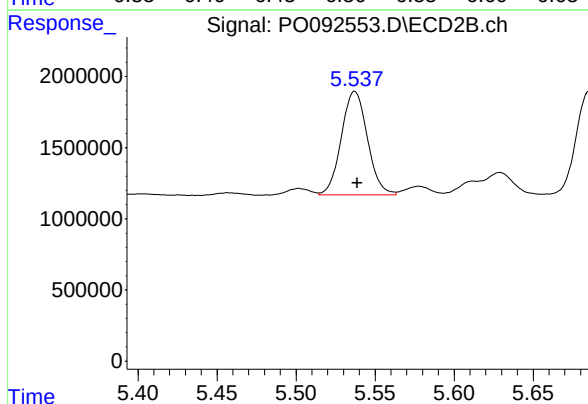


#26 AR-1254-1

R.T.: 5.537 min
Delta R.T.: -0.002 min
Response: 8360993
Conc: 106.66 ng/ml

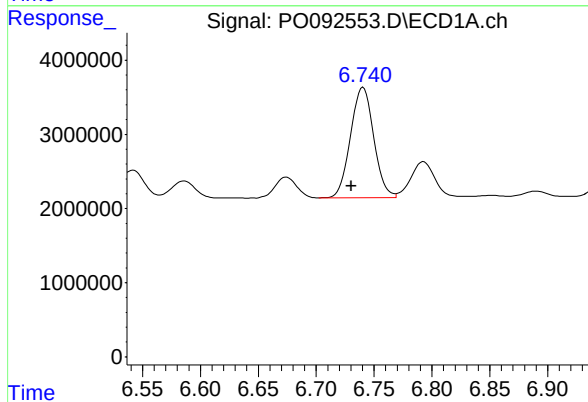


#27 AR-1254-2

R.T.: 6.740 min
Delta R.T.: 0.010 min
Response: 20690811
Conc: 127.29 ng/ml

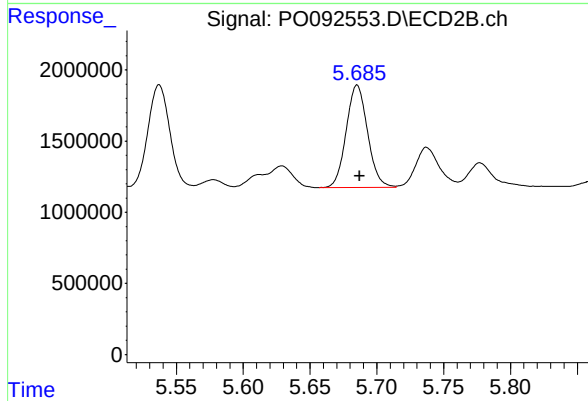

#27 AR-1254-2

R.T.: 5.685 min
Delta R.T.: -0.002 min
Response: 8011232
Conc: 115.78 ng/ml

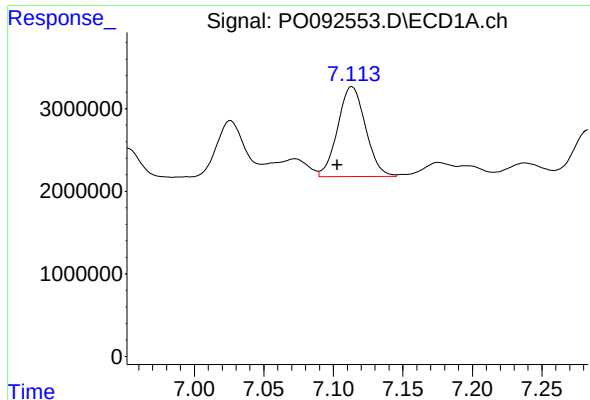


#28 AR-1254-3

R.T.: 7.114 min
Delta R.T.: 0.011 min
Response: 15181327
Conc: 92.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260967LOZ-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

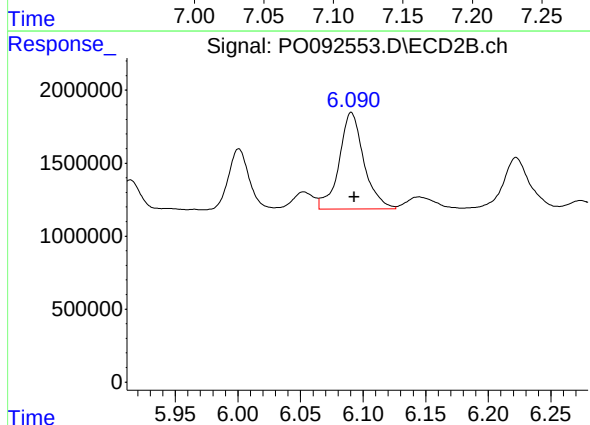


#28 AR-1254-3

R.T.: 6.091 min
Delta R.T.: -0.002 min
Response: 9109692
Conc: 85.35 ng/ml

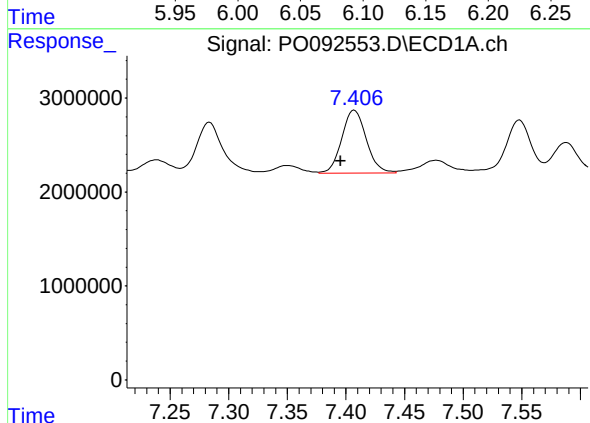


#29 AR-1254-4

R.T.: 7.407 min
Delta R.T.: 0.012 min
Response: 9812116
Conc: 89.70 ng/ml

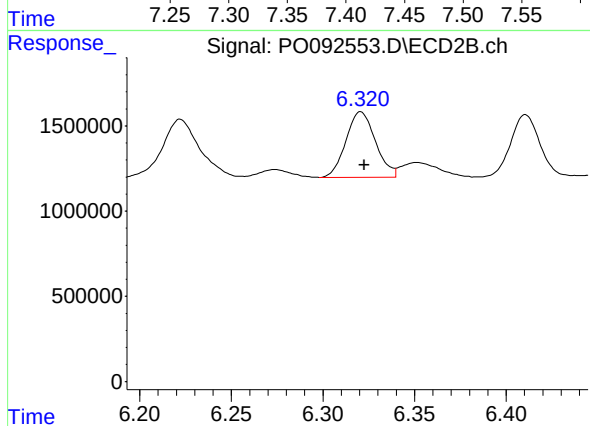

#29 AR-1254-4

R.T.: 6.321 min
Delta R.T.: -0.002 min
Response: 4336557
Conc: 73.63 ng/ml

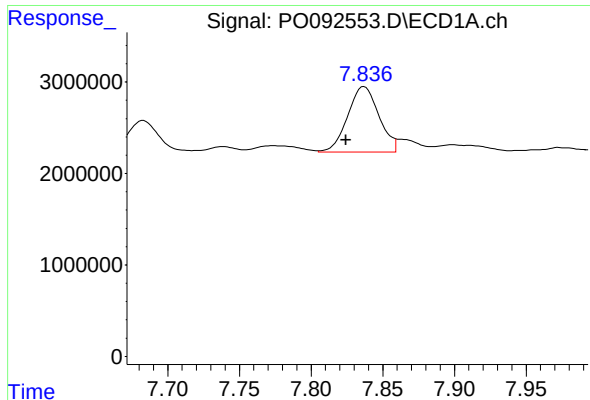


#30 AR-1254-5

R.T.: 7.836 min
Delta R.T.: 0.012 min
Response: 10929101
Conc: 77.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260967LOZ-1-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

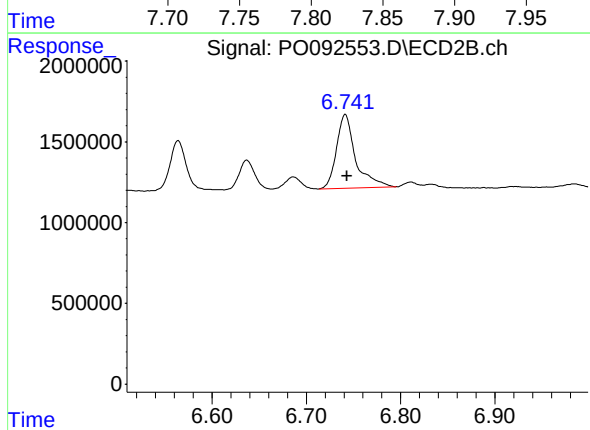

#30 AR-1254-5

R.T.: 6.741 min
Delta R.T.: -0.002 min
Response: 6404016
Conc: 70.36 ng/ml