

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 14:44
 Operator : YP/AJ
 Sample : 01590-04 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC271315LOZ-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2023
 Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 17 15:45:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.452	3.642	3351496	1639732	1.158m	1.168
2) SA Decachlor...	10.392	8.688	4351130	2039247	2.108m	1.806

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021723\
Data File : PO092556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 14:44
Operator : YP/AJ
Sample : 01590-04 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 17 15:45:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

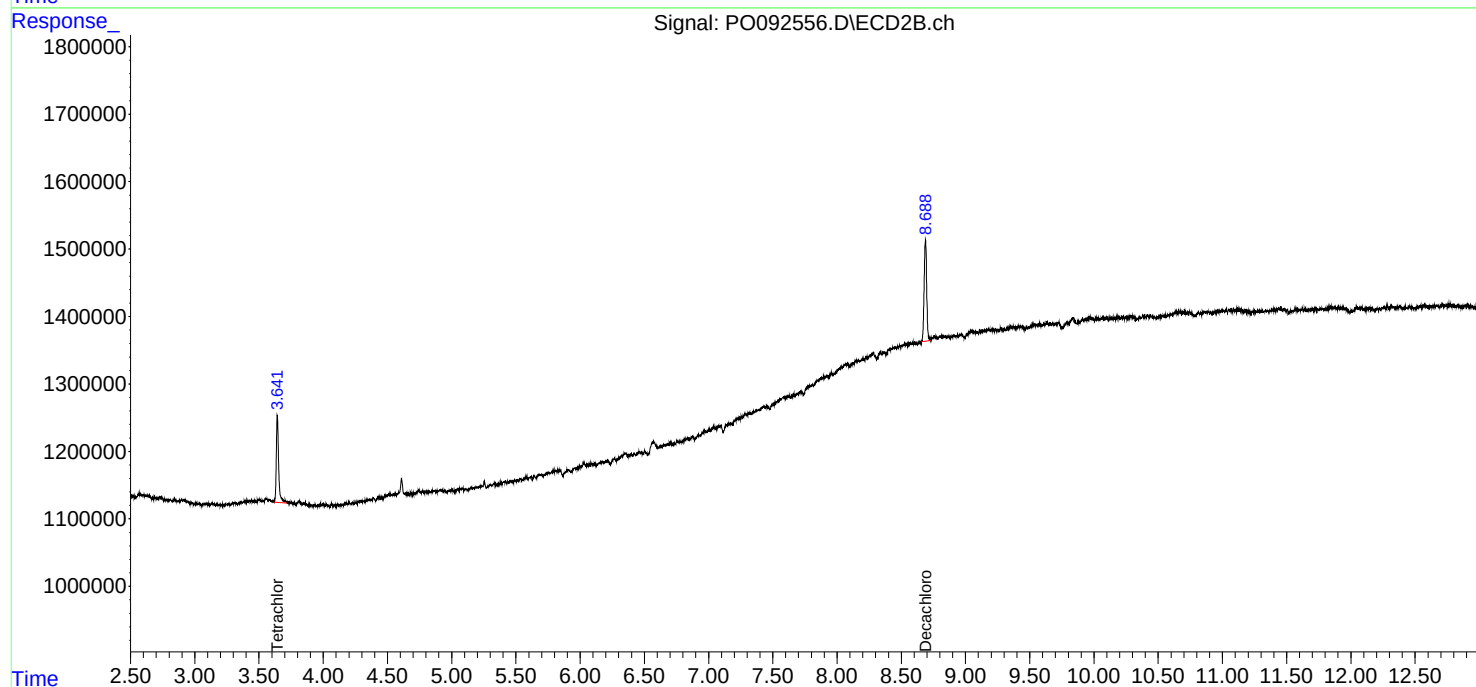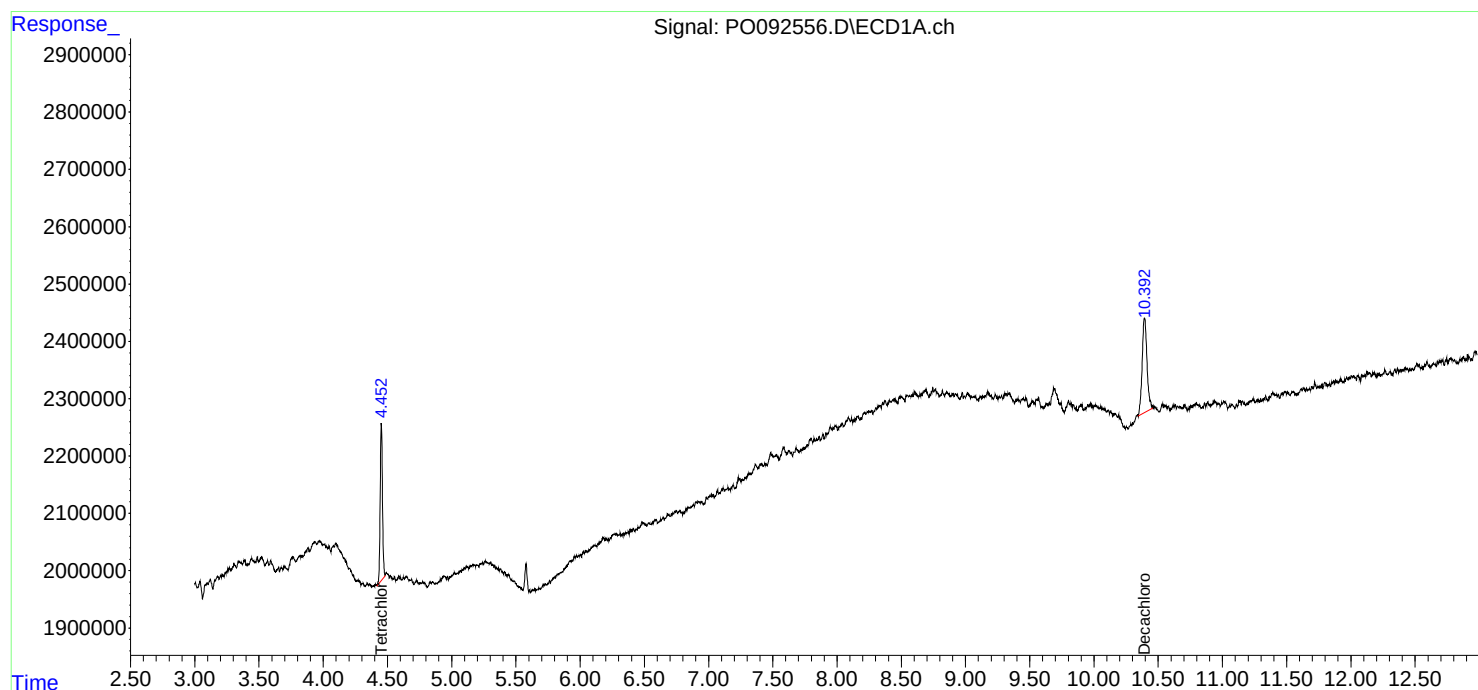

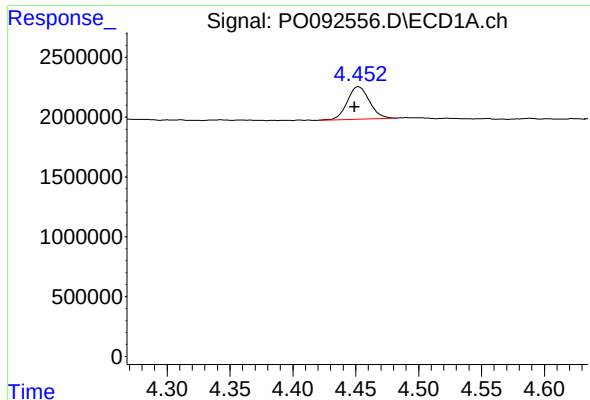


#1 Tetrachloro-m-xylene

R.T.: 4.452 min
Delta R.T.: 0.003 min
Response: 3351496
Conc: 1.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC271315LOZ-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

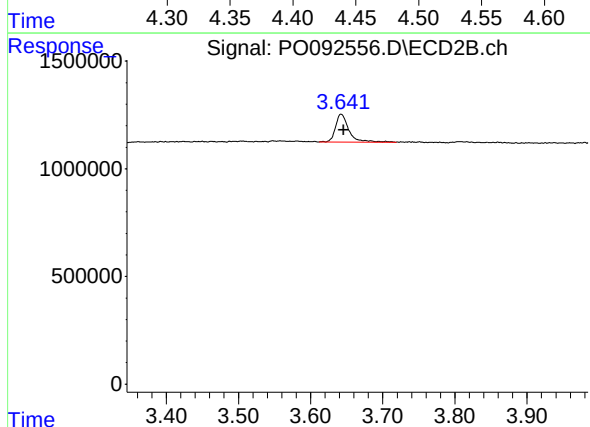


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.004 min
Response: 1639732
Conc: 1.17 ng/ml

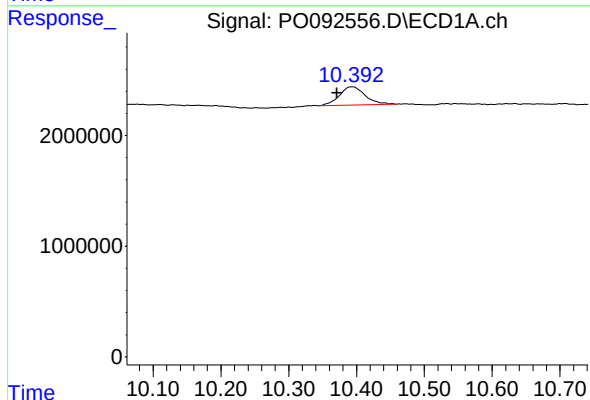

#2 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.021 min
Response: 4351130
Conc: 2.11 ng/ml m

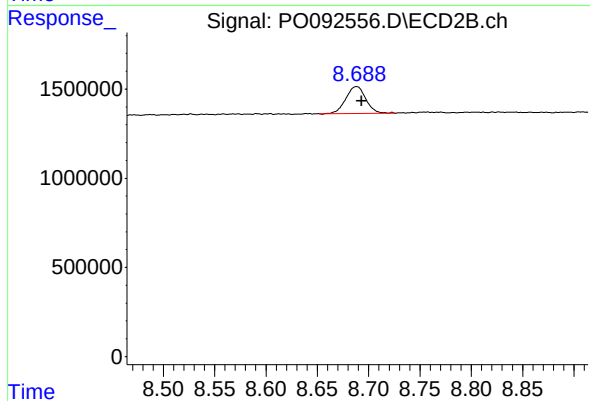

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: -0.005 min
Response: 2039247
Conc: 1.81 ng/ml