

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Feb 2023 19:17
 Operator : YP/AJ
 Sample : 01592-07 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF499K-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2023
 Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 00:52:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.451	3.642	3464863	1448136	1.197	1.031
2) SA Decachlor...	10.391	8.685	3683183	1740568	1.785m	1.542

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021723\
Data File : PO092570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Feb 2023 19:17
Operator : YP/AJ
Sample : 01592-07 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HEF499K-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 00:52:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

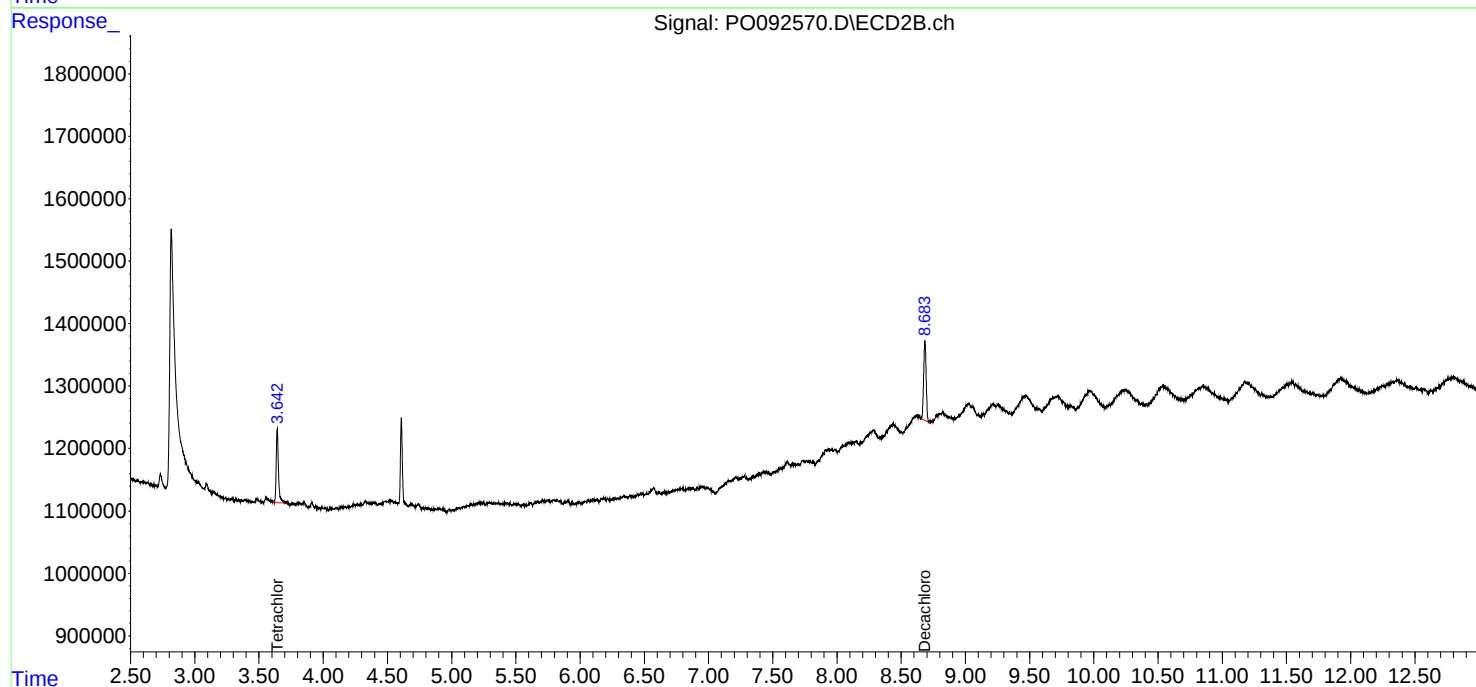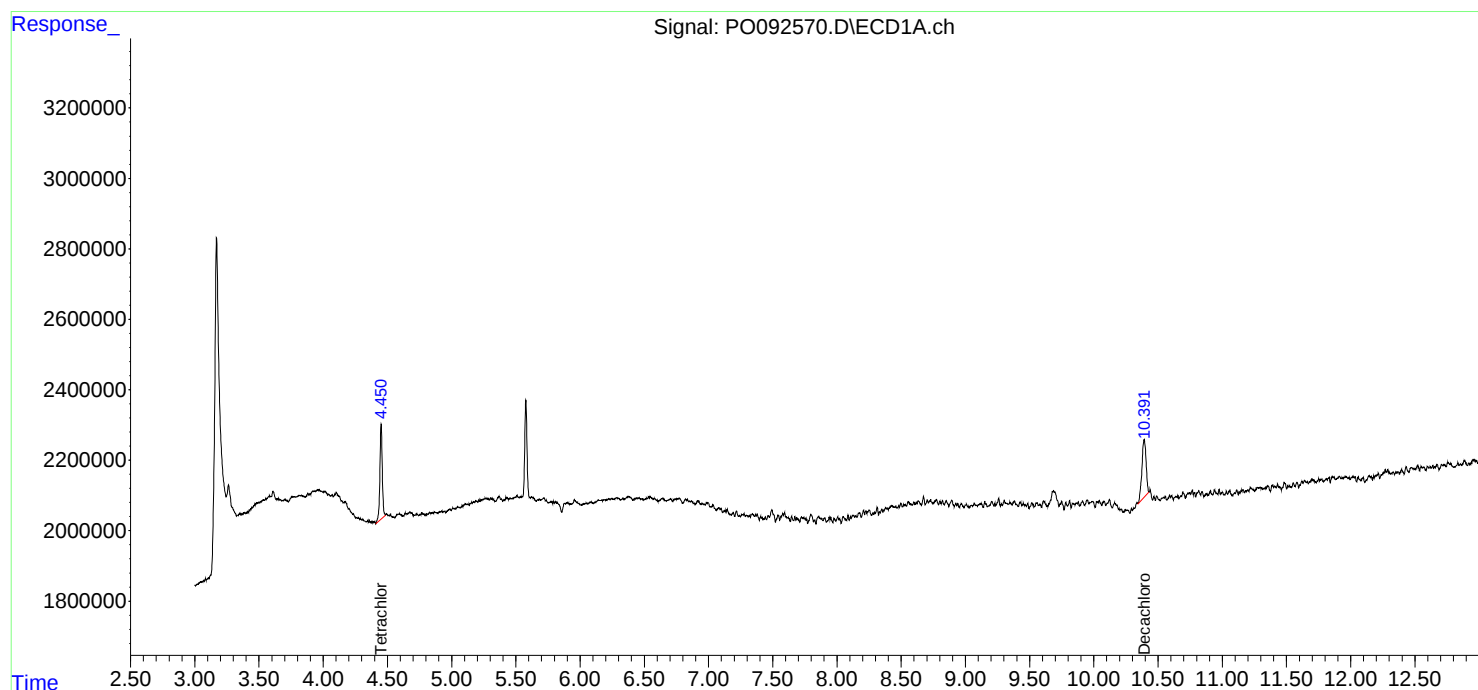

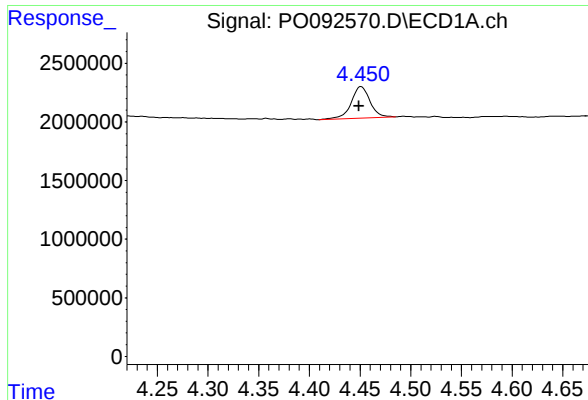


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: 0.002 min
Response: 3464863
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF499K-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

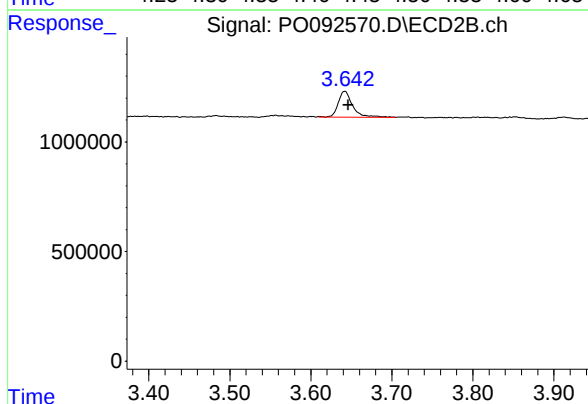


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.004 min
Response: 1448136
Conc: 1.03 ng/ml

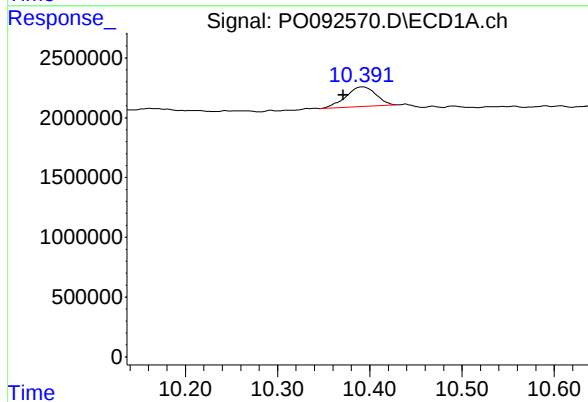

#2 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: 0.020 min
Response: 3683183
Conc: 1.78 ng/ml m

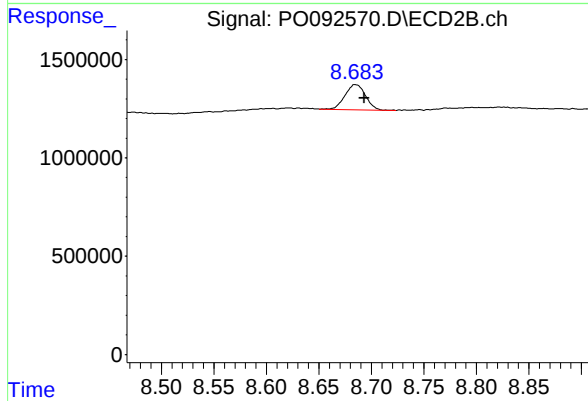

#2 Decachlorobiphenyl

R.T.: 8.685 min
Delta R.T.: -0.008 min
Response: 1740568
Conc: 1.54 ng/ml