

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2023 03:03
 Operator : YP/AJ
 Sample : 01576-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RE137-BAGFILTER-20220215

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2023
 Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 07:58:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.641	44495408	19483312	15.370m	13.876
2) SA Decachlor...	10.379	8.679	37016605	17676311	17.935	15.658

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
Data File : P0092593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2023 03:03
Operator : YP/AJ
Sample : 01576-01
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RE137-BAGFILTER-20220215


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 07:58:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

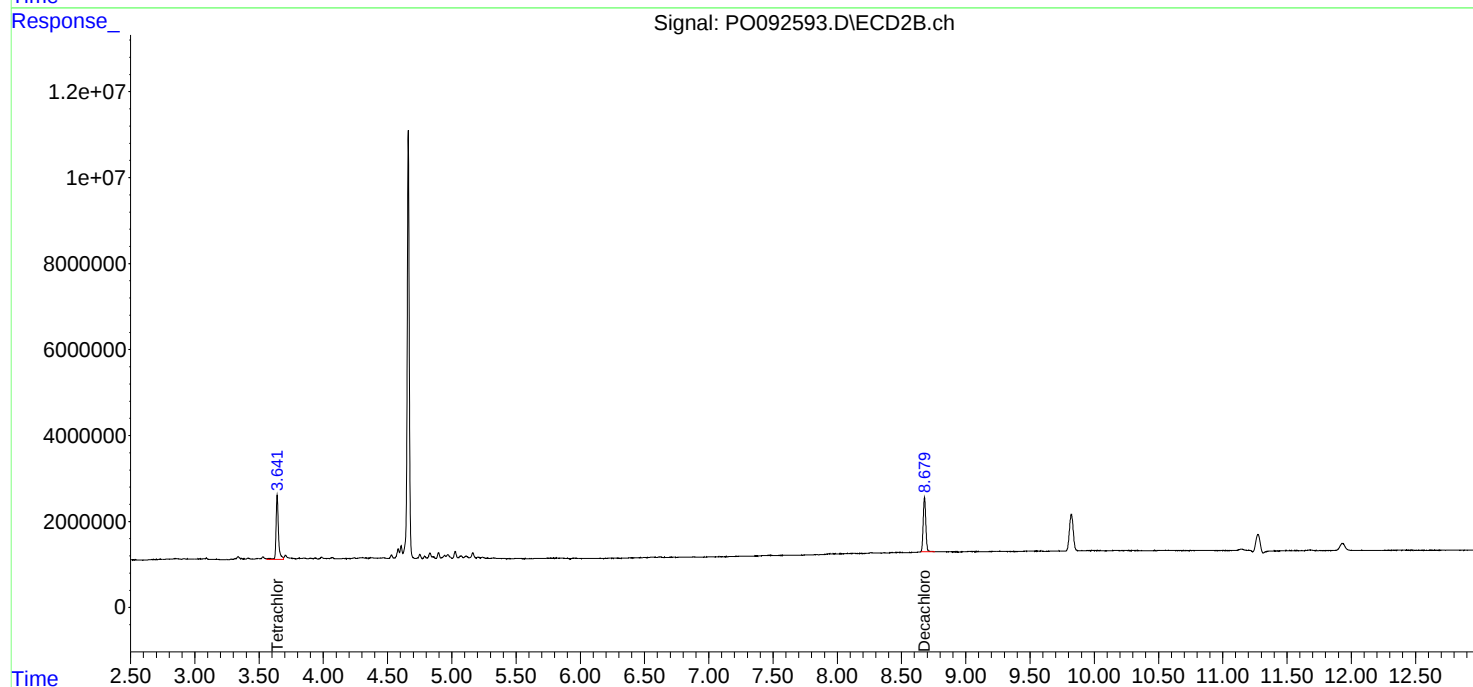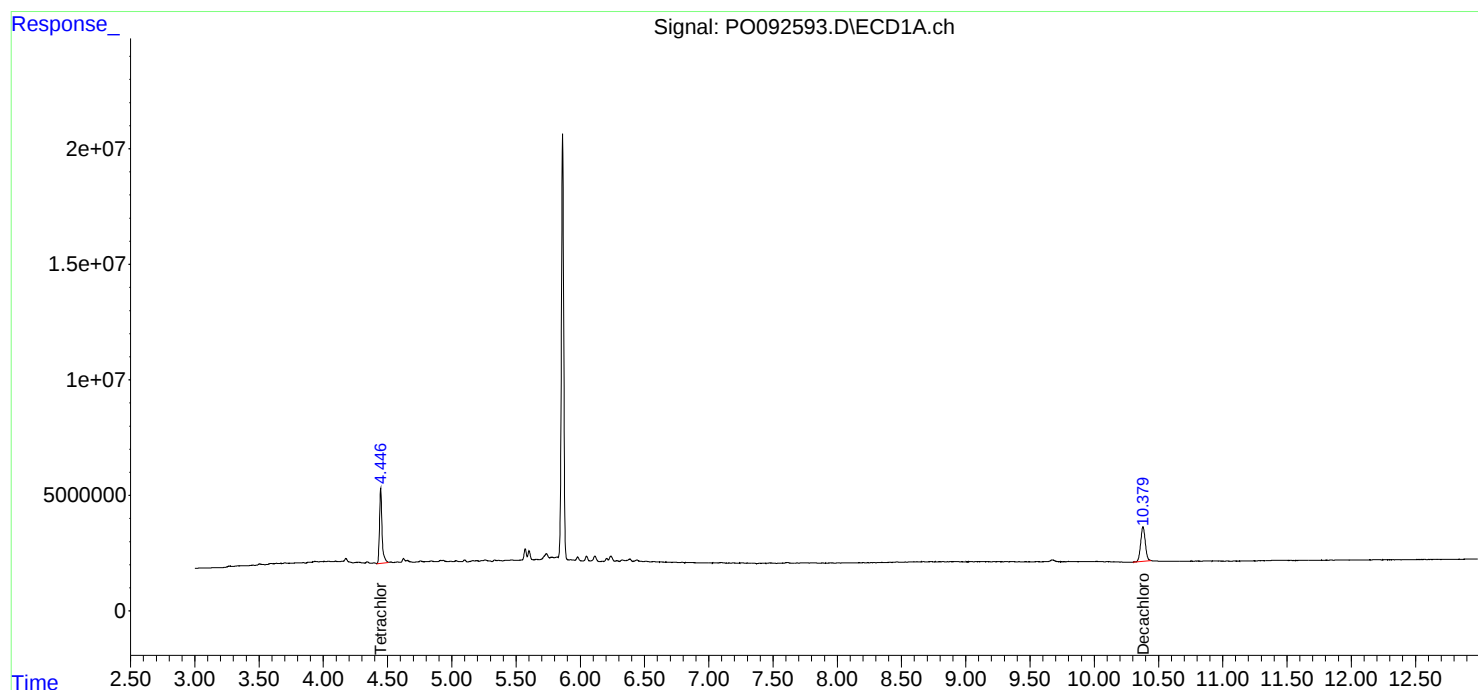

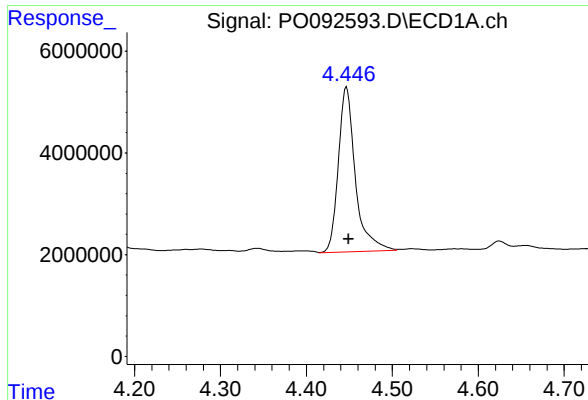


#1 Tetrachloro-m-xylene

R.T.: 4.446 min
Delta R.T.: -0.003 min
Response: 44495408
Conc: 15.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
RE137-BAGFILTER-20220215


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

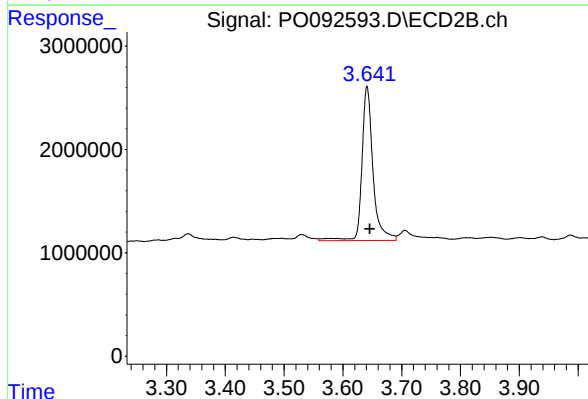


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: -0.005 min
Response: 19483312
Conc: 13.88 ng/ml

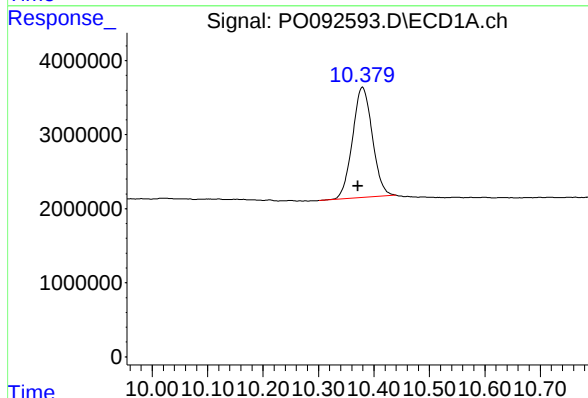

#2 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: 0.008 min
Response: 37016605
Conc: 17.93 ng/ml

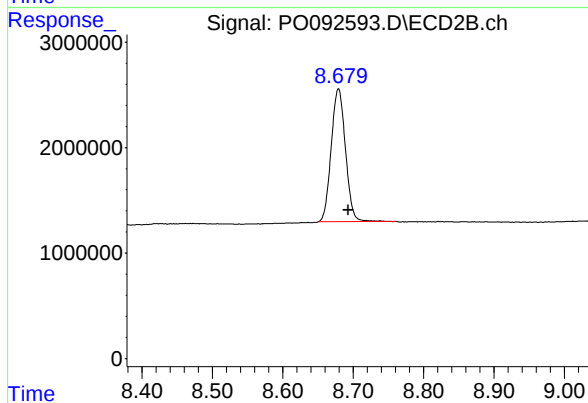

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.014 min
Response: 17676311
Conc: 15.66 ng/ml