

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2023 07:47
 Operator : YP/AJ
 Sample : 01586-05
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2023
 Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 03:19:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.445	3.640	55763757	24996443	19.263	17.802
2) SA Decachlor...	10.376	8.675	44674991	19263015	21.646	17.063m
Target Compounds						
31) L7 AR-1260-1	7.272	6.215	19809947	11017872	150.354m	145.856
32) L7 AR-1260-2	7.535	6.404	27138394	11227271	183.013m	128.145 #
33) L7 AR-1260-3	7.907	6.558	16634676	9845355	146.867	113.571
34) L7 AR-1260-4	8.136	7.032	18146447	6817847	146.384m	101.808 #
35) L7 AR-1260-5	8.473	7.275	31623115	15171426	142.410	106.616 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021723\
Data File : PO092608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2023 07:47
Operator : YP/AJ
Sample : 01586-05
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 03:19:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

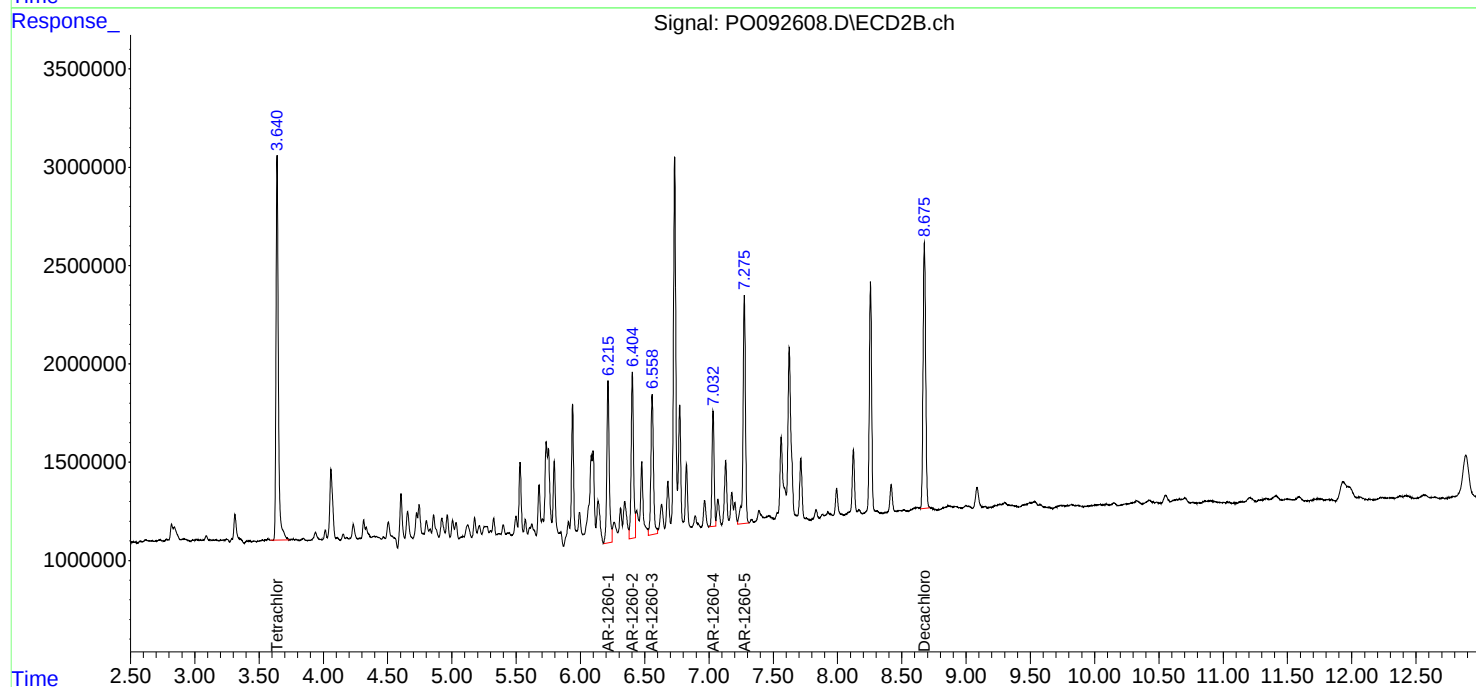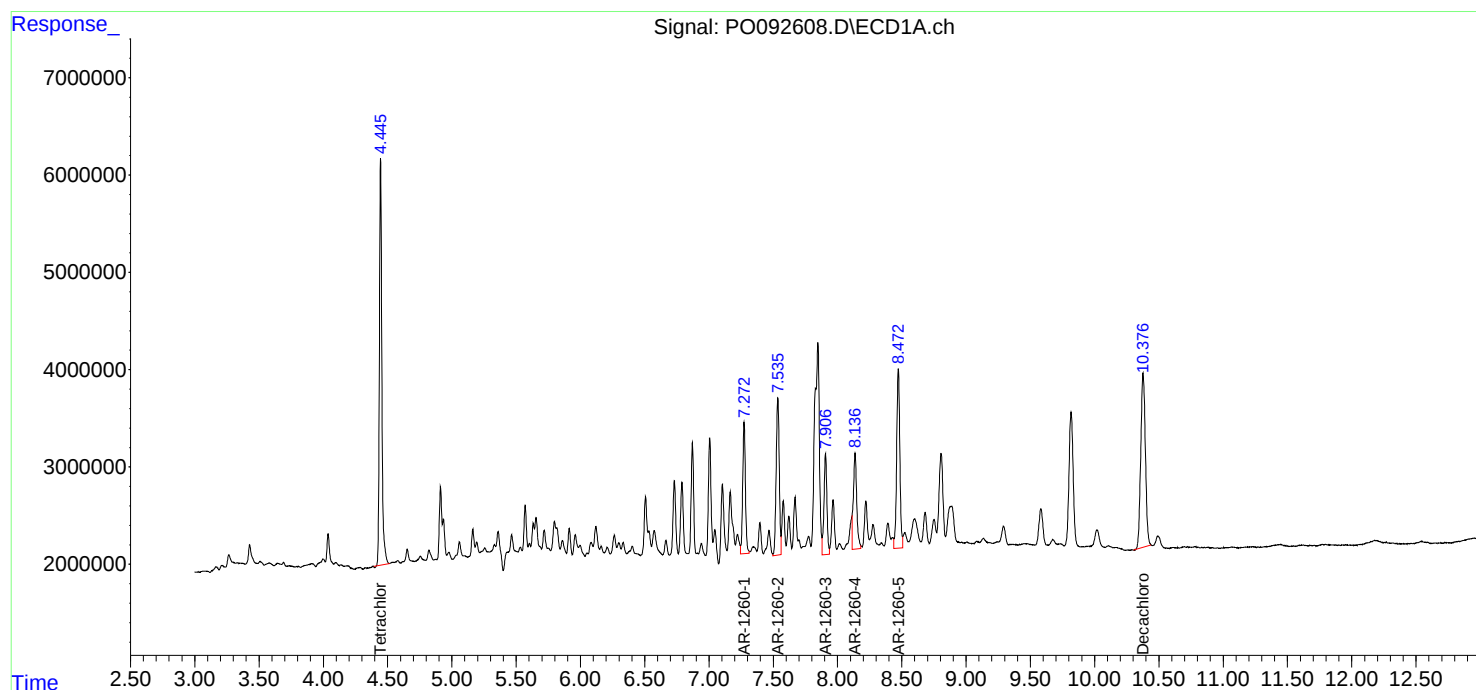

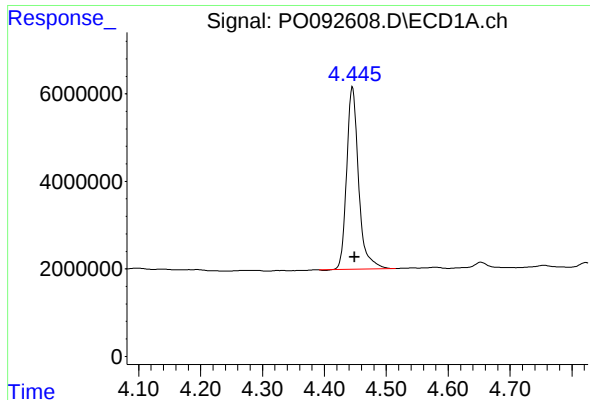


#1 Tetrachloro-m-xylene

R.T.: 4.445 min
Delta R.T.: -0.004 min
Response: 55763757
Conc: 19.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

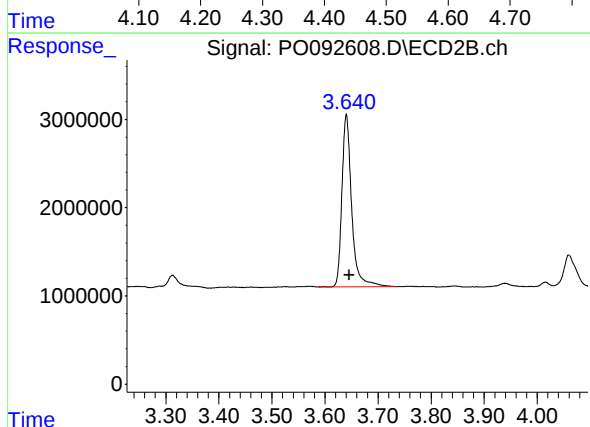


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: -0.006 min
Response: 24996443
Conc: 17.80 ng/ml

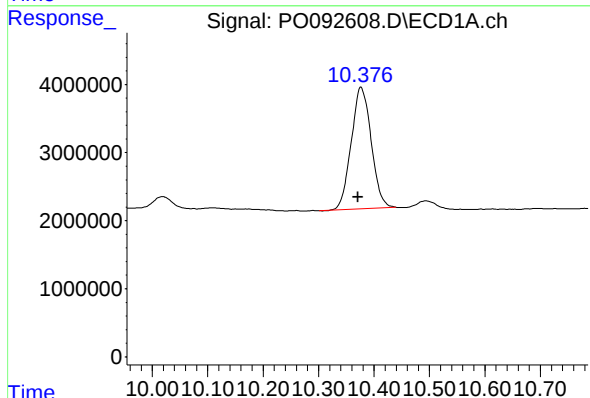


#2 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: 0.005 min
Response: 44674991
Conc: 21.65 ng/ml

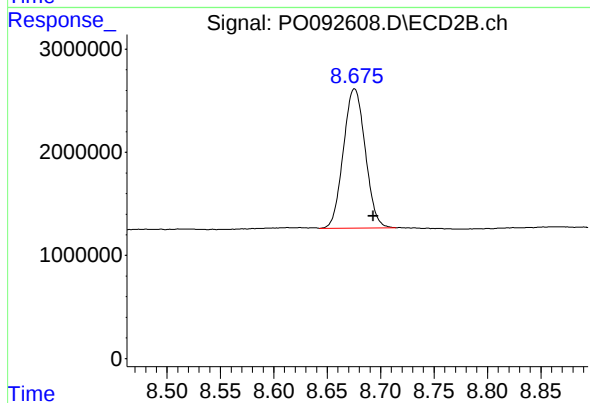

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: -0.018 min
Response: 19263015
Conc: 17.06 ng/ml m

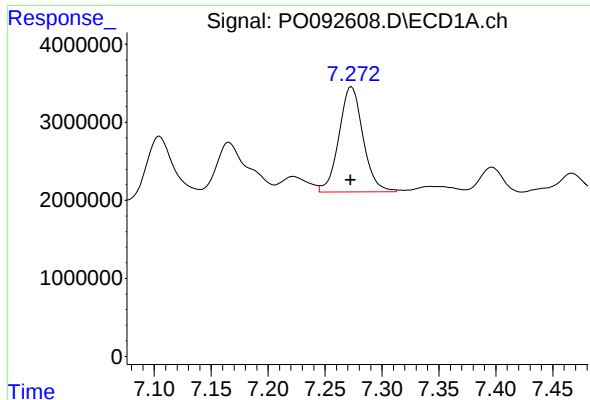


#31 AR-1260-1

R.T.: 7.272 min
Delta R.T.: 0.000 min
Response: 19809947
Conc: 150.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

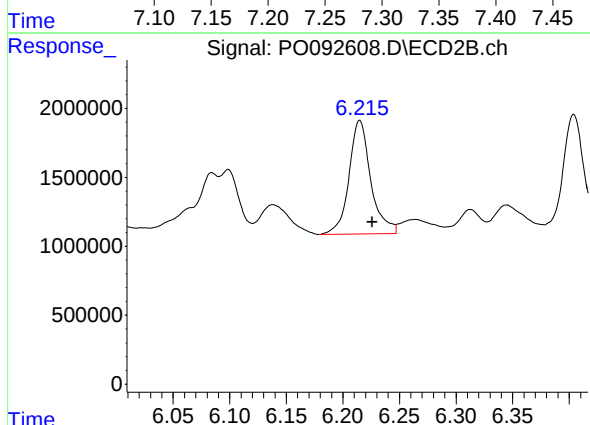


#31 AR-1260-1

R.T.: 6.215 min
Delta R.T.: -0.011 min
Response: 11017872
Conc: 145.86 ng/ml

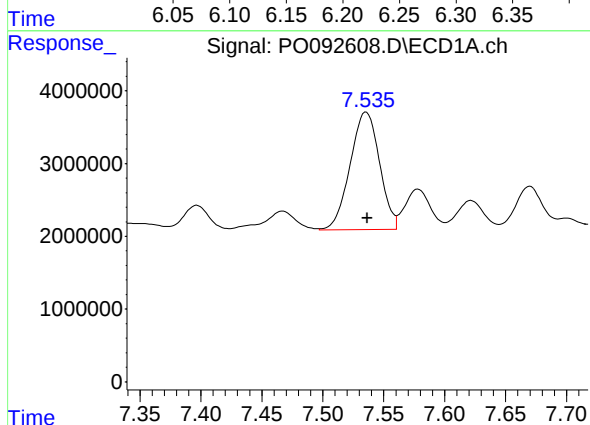


#32 AR-1260-2

R.T.: 7.535 min
Delta R.T.: -0.002 min
Response: 27138394
Conc: 183.01 ng/ml m

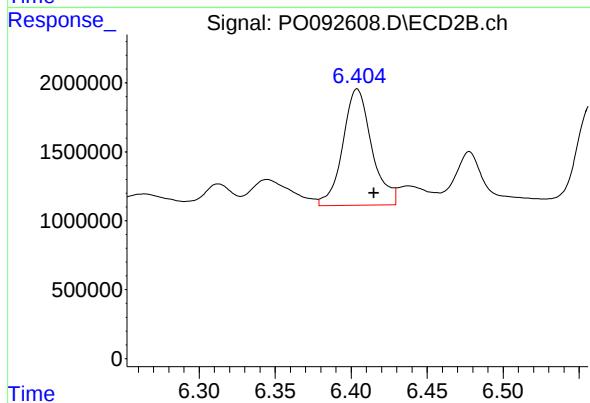

#32 AR-1260-2

R.T.: 6.404 min
Delta R.T.: -0.011 min
Response: 11227271
Conc: 128.15 ng/ml

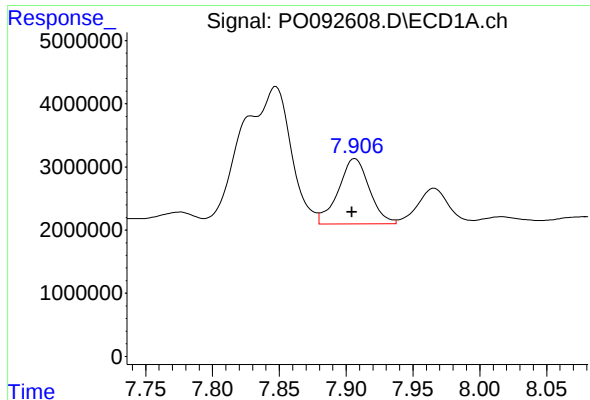


#33 AR-1260-3

R.T.: 7.907 min
Delta R.T.: 0.002 min
Response: 16634676
Conc: 146.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

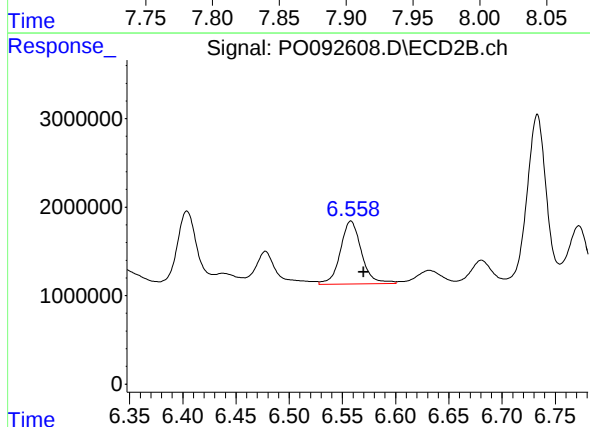


#33 AR-1260-3

R.T.: 6.558 min
Delta R.T.: -0.012 min
Response: 9845355
Conc: 113.57 ng/ml

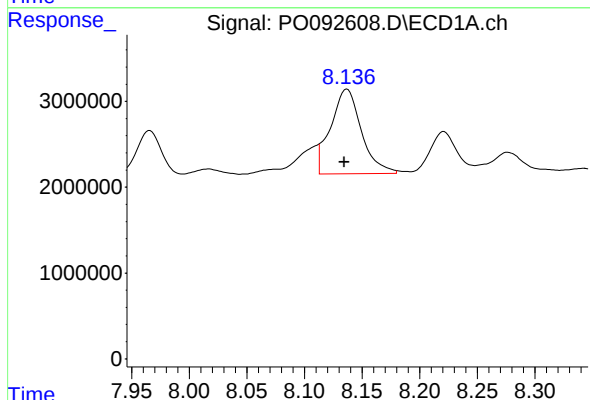


#34 AR-1260-4

R.T.: 8.136 min
Delta R.T.: 0.002 min
Response: 18146447
Conc: 146.38 ng/ml m

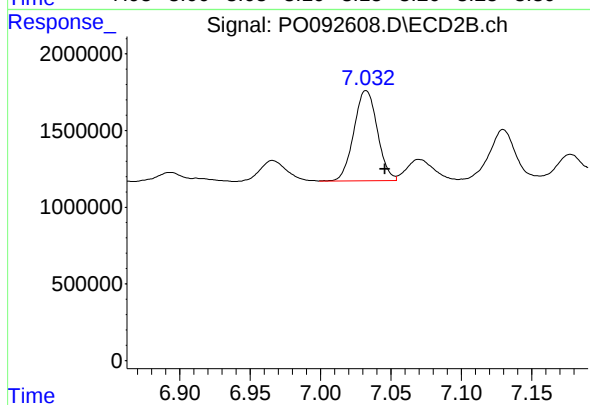

#34 AR-1260-4

R.T.: 7.032 min
Delta R.T.: -0.014 min
Response: 6817847
Conc: 101.81 ng/ml

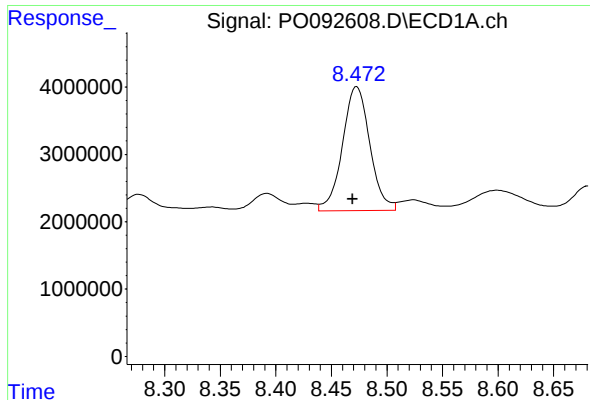


#35 AR-1260-5

R.T.: 8.473 min
Delta R.T.: 0.004 min
Response: 31623115
Conc: 142.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

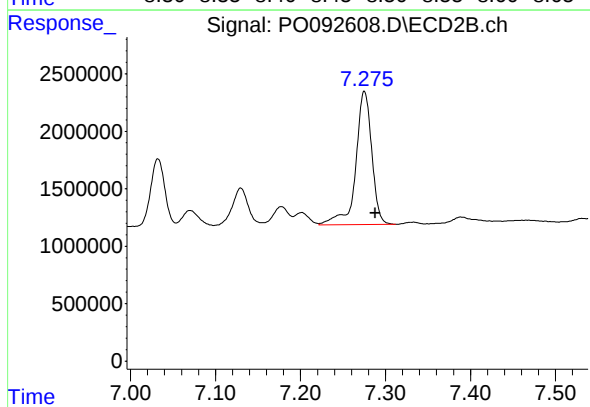

#35 AR-1260-5

R.T.: 7.275 min
Delta R.T.: -0.013 min
Response: 15171426
Conc: 106.62 ng/ml