

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021723\
 Data File : P0092635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2023 16:25
 Operator : YP/AJ
 Sample : 01589-01
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MIXED-DEMO

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/20/2023
 Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 03:32:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.445	3.639	55933773	23671822	19.322m	16.859m
2) SA Decachlor...	10.380	8.676	52972041	20594956	25.666	18.243 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO021723\
Data File : PO092635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2023 16:25
Operator : YP/AJ
Sample : 01589-01
Misc :
ALS Vial : 67 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MIXED-DEMO


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 03:32:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

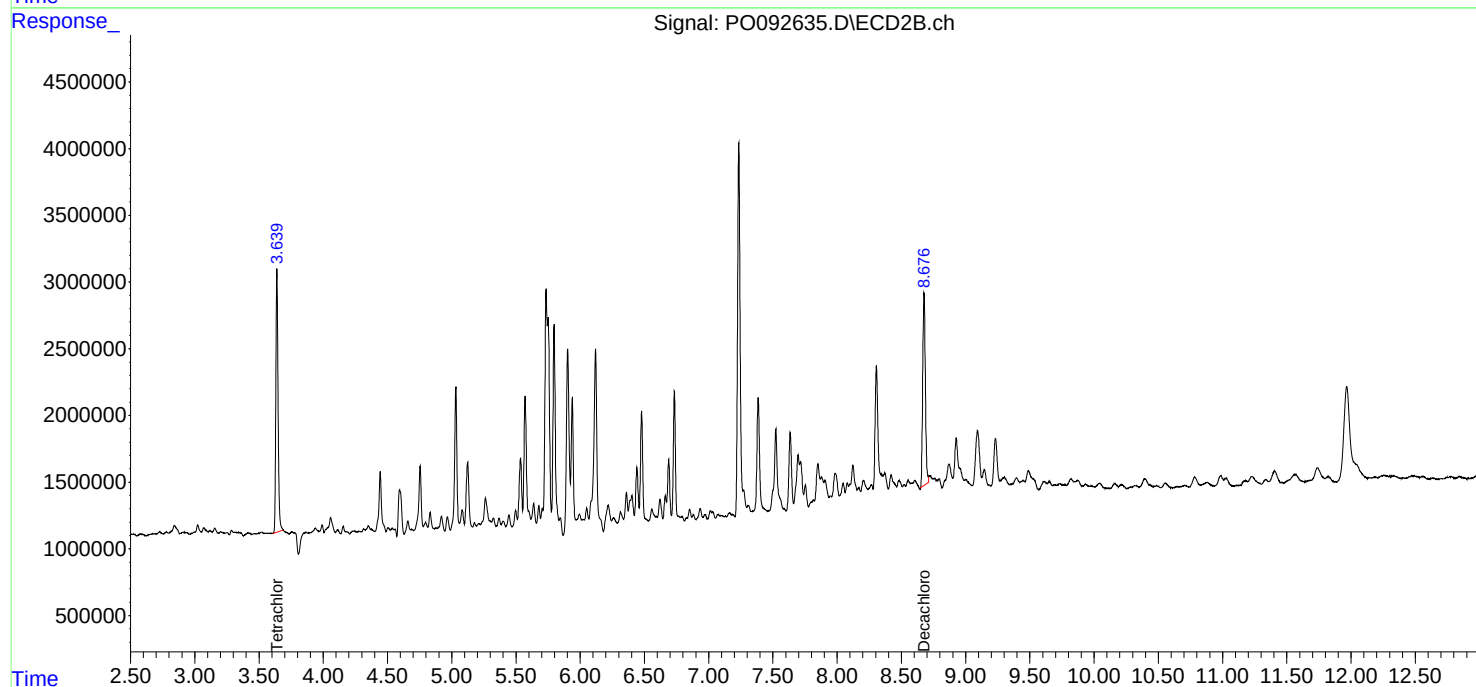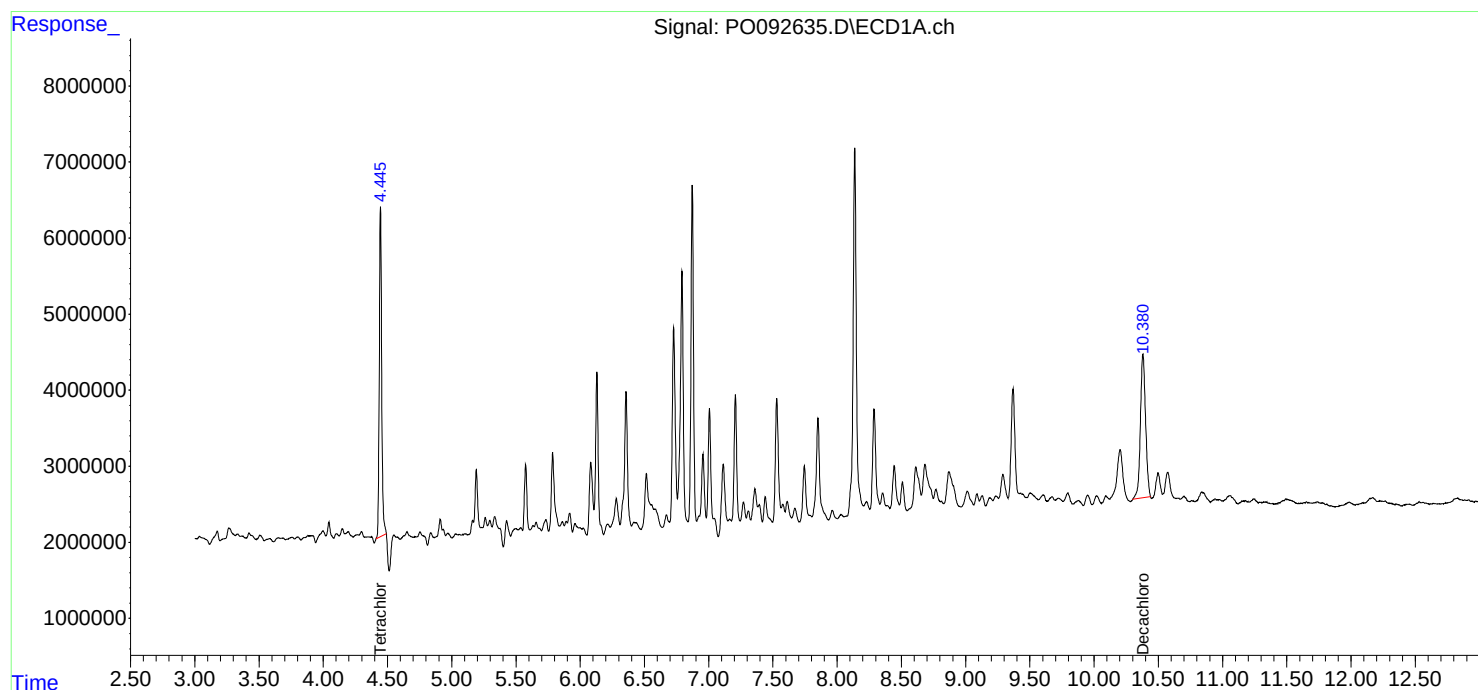

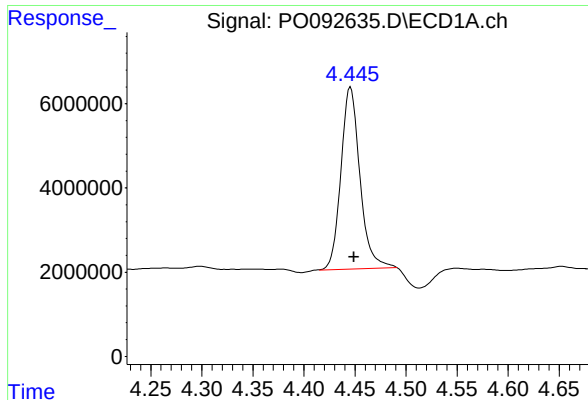


#1 Tetrachloro-m-xylene

R.T.: 4.445 min
Delta R.T.: -0.004 min
Response: 55933773
Conc: 19.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MIXED-DEMO


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/20/2023
Supervised By :Ankita Jodhani 02/20/2023

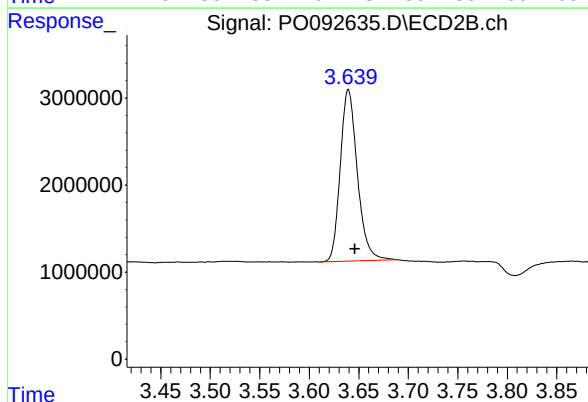


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.007 min
Response: 23671822
Conc: 16.86 ng/ml

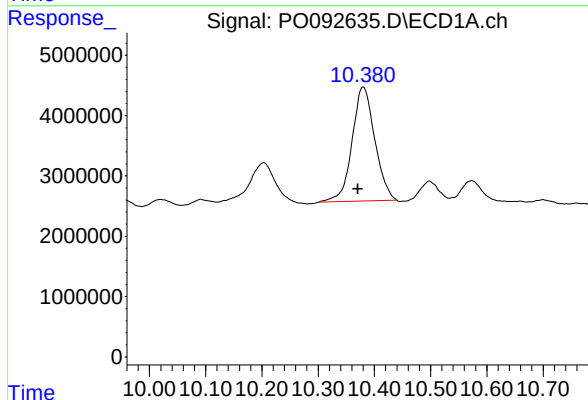

#2 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: 0.009 min
Response: 52972041
Conc: 25.67 ng/ml

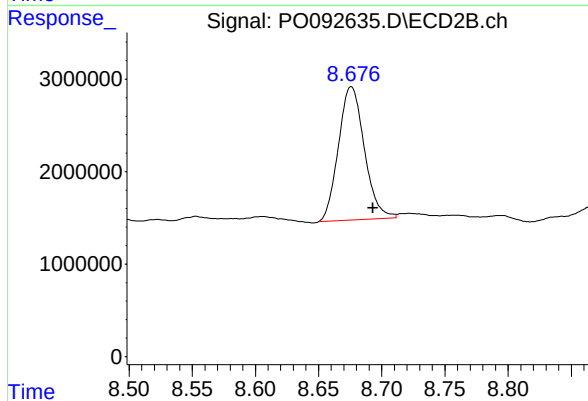

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.017 min
Response: 20594956
Conc: 18.24 ng/ml