

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022024\
 Data File : P0101903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2024 14:23
 Operator : YP/AJ
 Sample : PB159138BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB159138BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2024
 Supervised By :Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:15:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.282	3.393	70904589	52434181	22.995	19.726
2) SA Decachlor...	9.834	8.267	51393480	38936401	24.509m	20.494m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022024\
Data File : PO101903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 14:23
Operator : YP/AJ
Sample : PB159138BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB159138BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:15:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

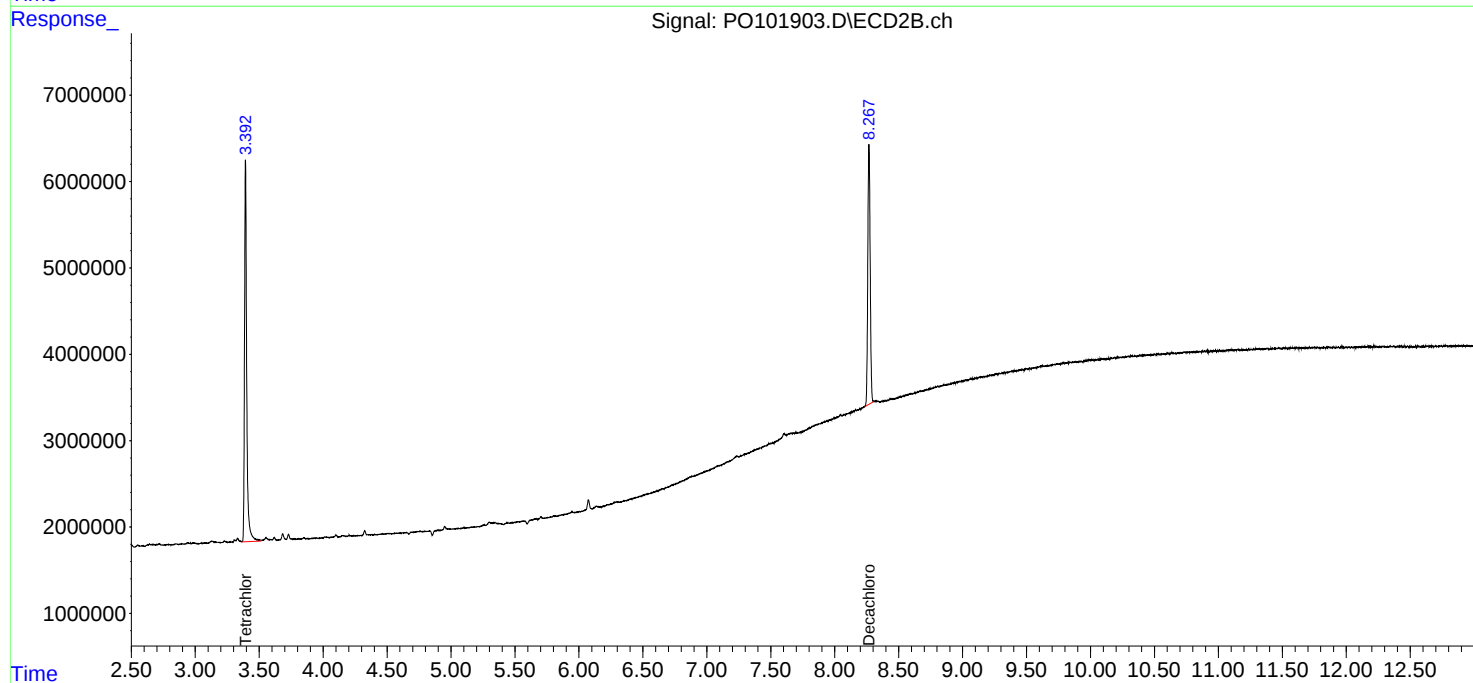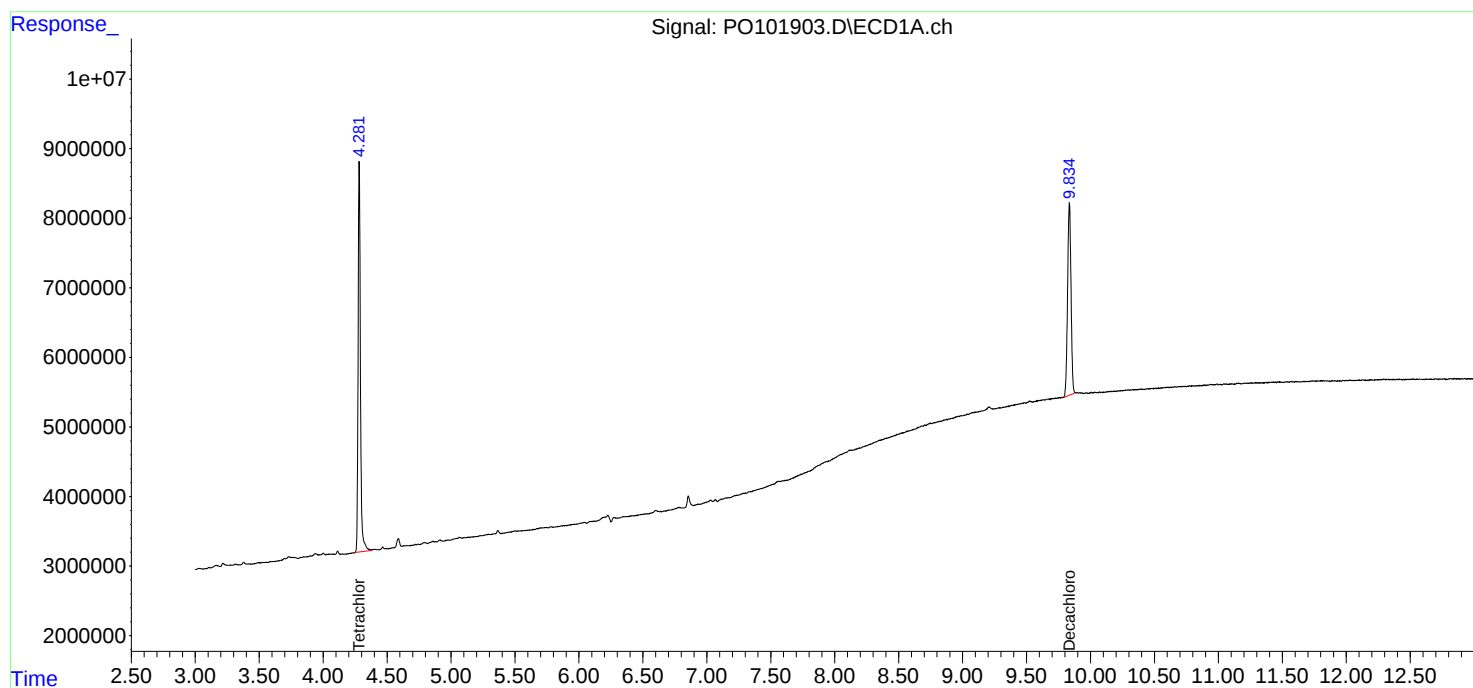

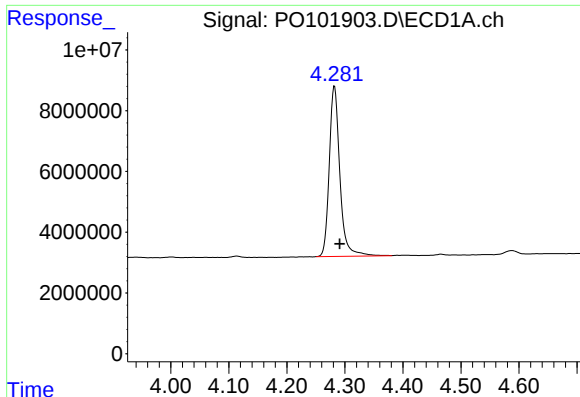

#1 Tetrachloro-m-xylene

R.T.: 4.282 min
Delta R.T.: -0.009 min
Response: 70904589
Conc: 22.99 ng/ml

Instrument :

ECD_O


ClientSampleId :

PB159138BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

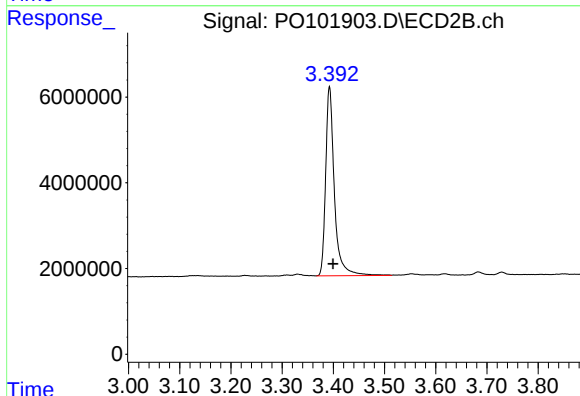


#1 Tetrachloro-m-xylene

R.T.: 3.393 min
Delta R.T.: -0.007 min
Response: 52434181
Conc: 19.73 ng/ml

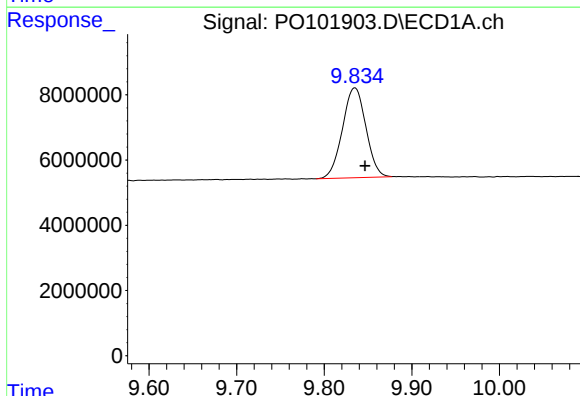

#2 Decachlorobiphenyl

R.T.: 9.834 min
Delta R.T.: -0.012 min
Response: 51393480
Conc: 24.51 ng/ml m

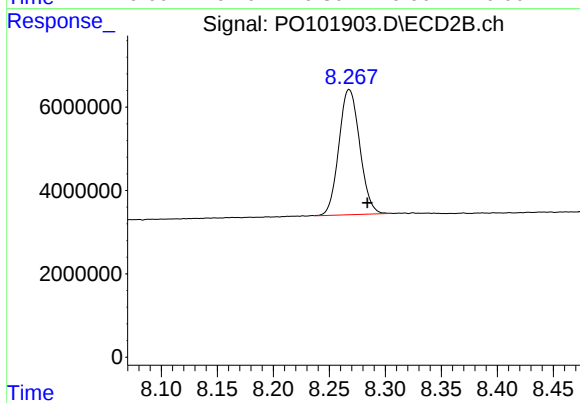

#2 Decachlorobiphenyl

R.T.: 8.267 min
Delta R.T.: -0.017 min
Response: 38936401
Conc: 20.49 ng/ml m