

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022024\
 Data File : P0101908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2024 15:48
 Operator : YP/AJ
 Sample : P1523-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20240764-COMPOSITE-39N-N-3-02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2024
 Supervised By :Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 00:16:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 12 05:22:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.282	3.394	50462106	39616479	16.365	14.904
2) SA Decachlor...	9.831	8.269	19116351	14403649	9.116m	7.581

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022024\
Data File : PO101908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 15:48
Operator : YP/AJ
Sample : P1523-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20240764-COMPOSITE-39N-N-3-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:16:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

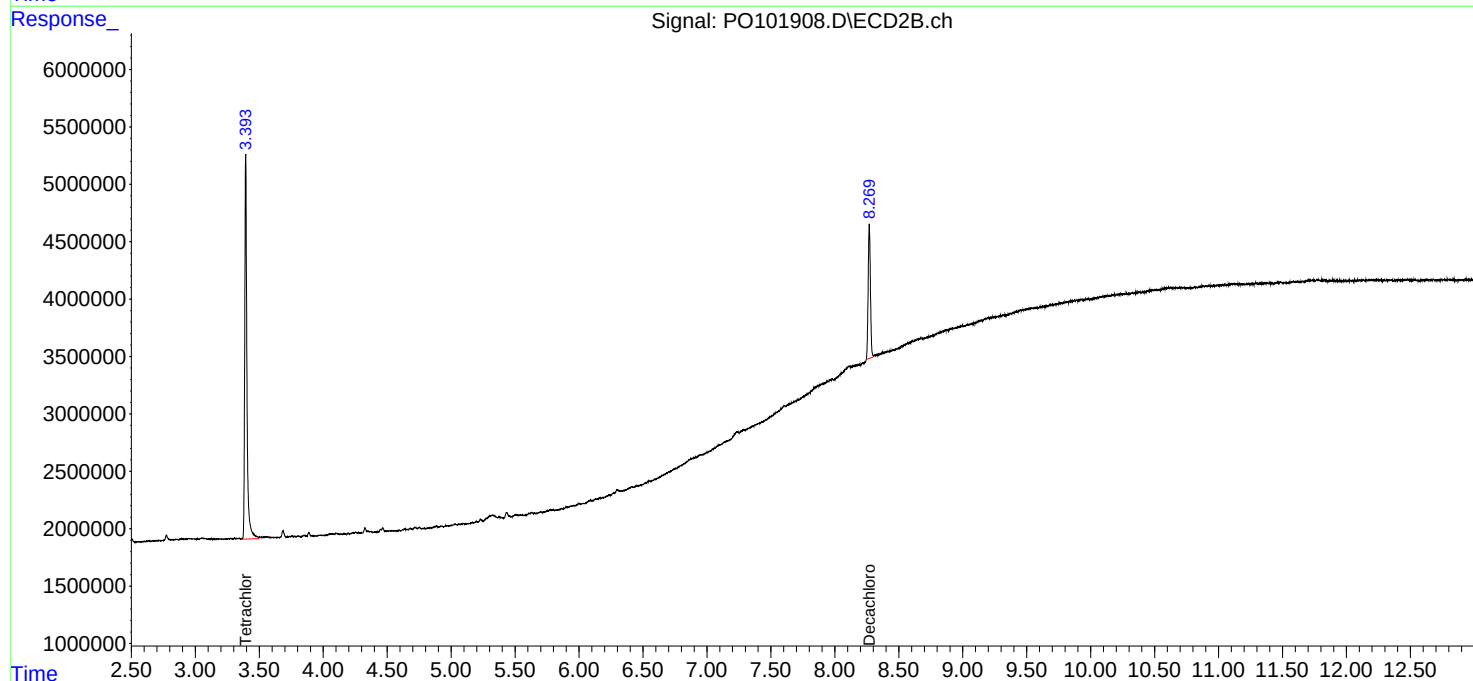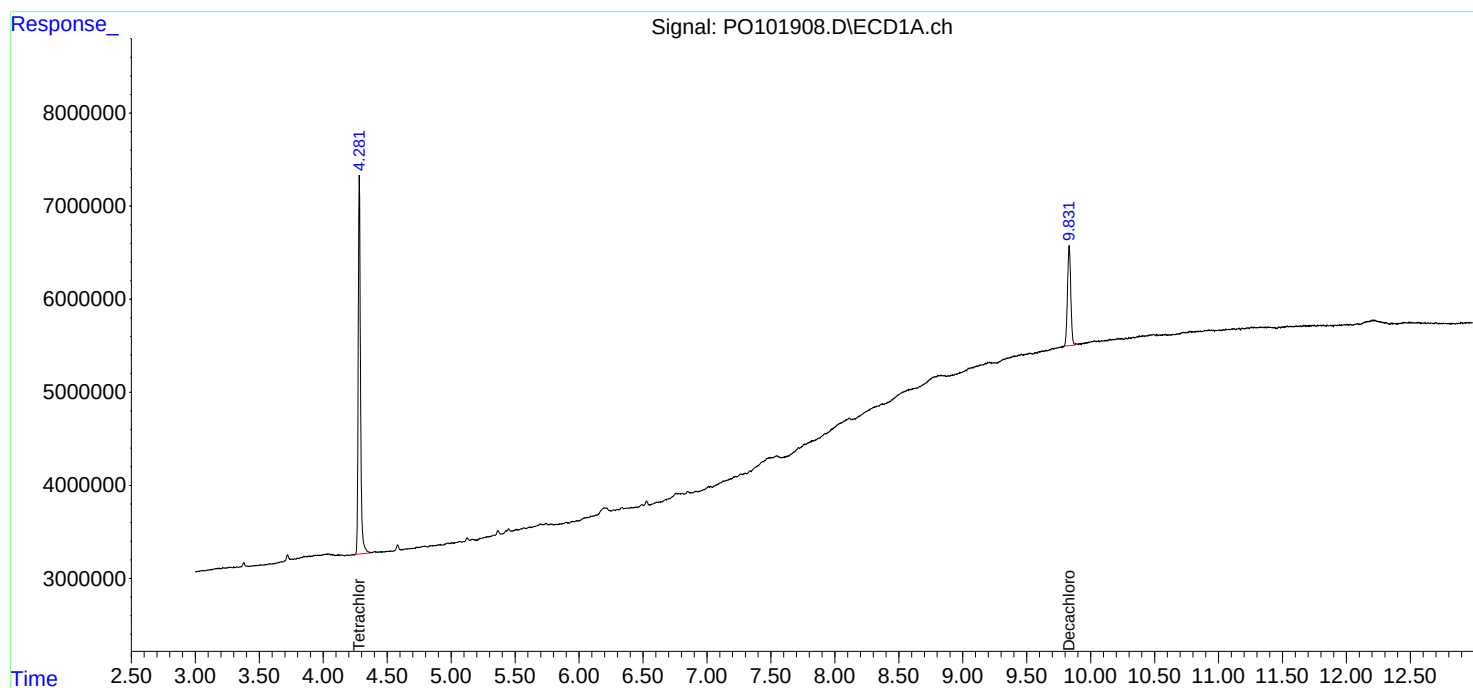

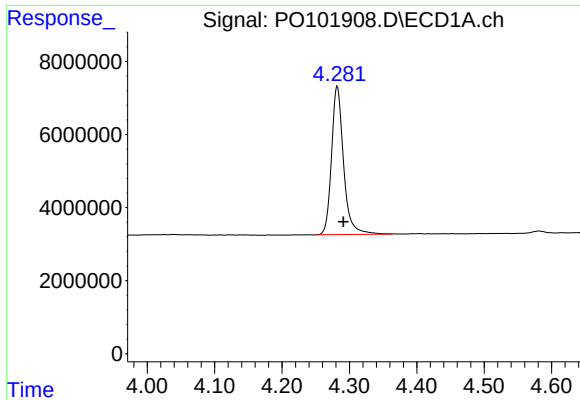


#1 Tetrachloro-m-xylene

R.T.: 4.282 min
Delta R.T.: -0.009 min
Response: 50462106
Conc: 16.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
20240764-COMPOSITE-39N-N-3-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

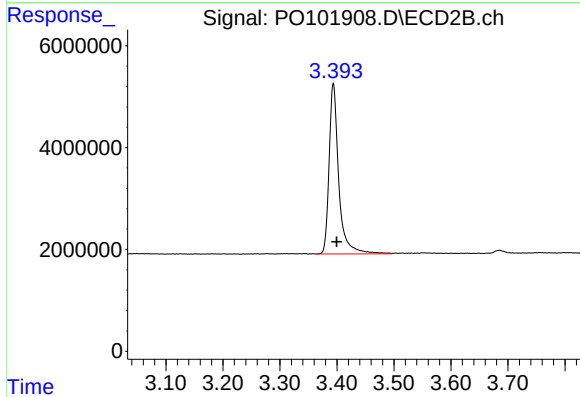


#1 Tetrachloro-m-xylene

R.T.: 3.394 min
Delta R.T.: -0.006 min
Response: 39616479
Conc: 14.90 ng/ml

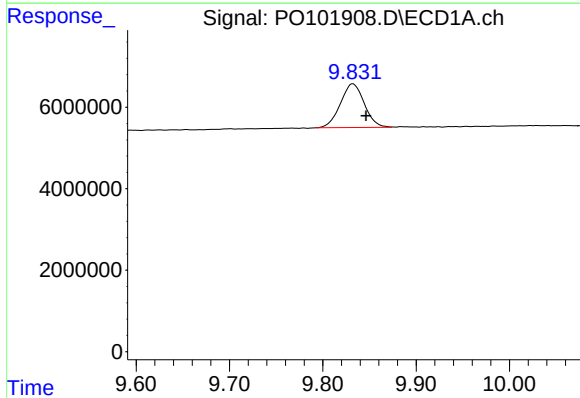

#2 Decachlorobiphenyl

R.T.: 9.831 min
Delta R.T.: -0.015 min
Response: 19116351
Conc: 9.12 ng/ml m

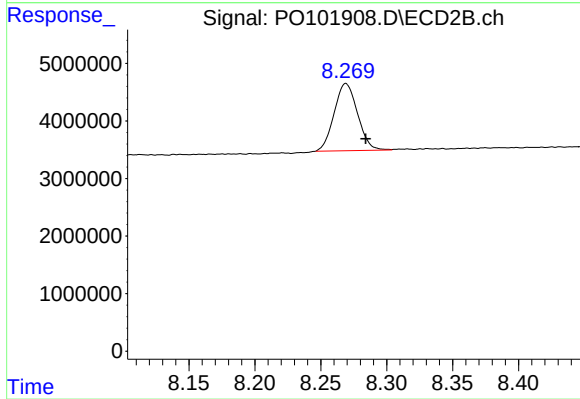

#2 Decachlorobiphenyl

R.T.: 8.269 min
Delta R.T.: -0.015 min
Response: 14403649
Conc: 7.58 ng/ml