

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022024\
Data File : P0101923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 20:33
Operator : YP/AJ
Sample : PB159137BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB159137BL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:21:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.283	3.394	65485932	50343494	21.237	18.939
2) SA Decachlor...	9.832	8.270	47672857	36869556	22.735m	19.406m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022024\
Data File : PO101923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2024 20:33
Operator : YP/AJ
Sample : PB159137BL
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB159137BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 00:21:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021024.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 12 05:22:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

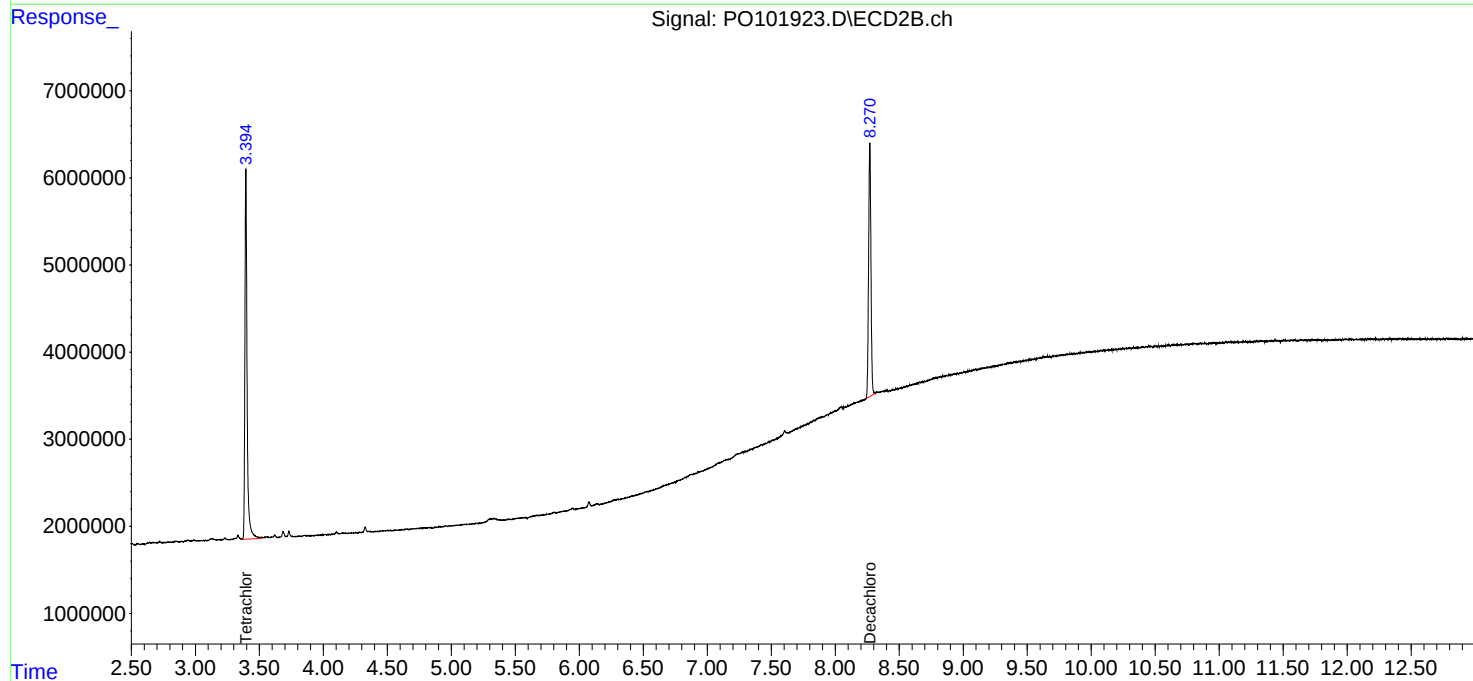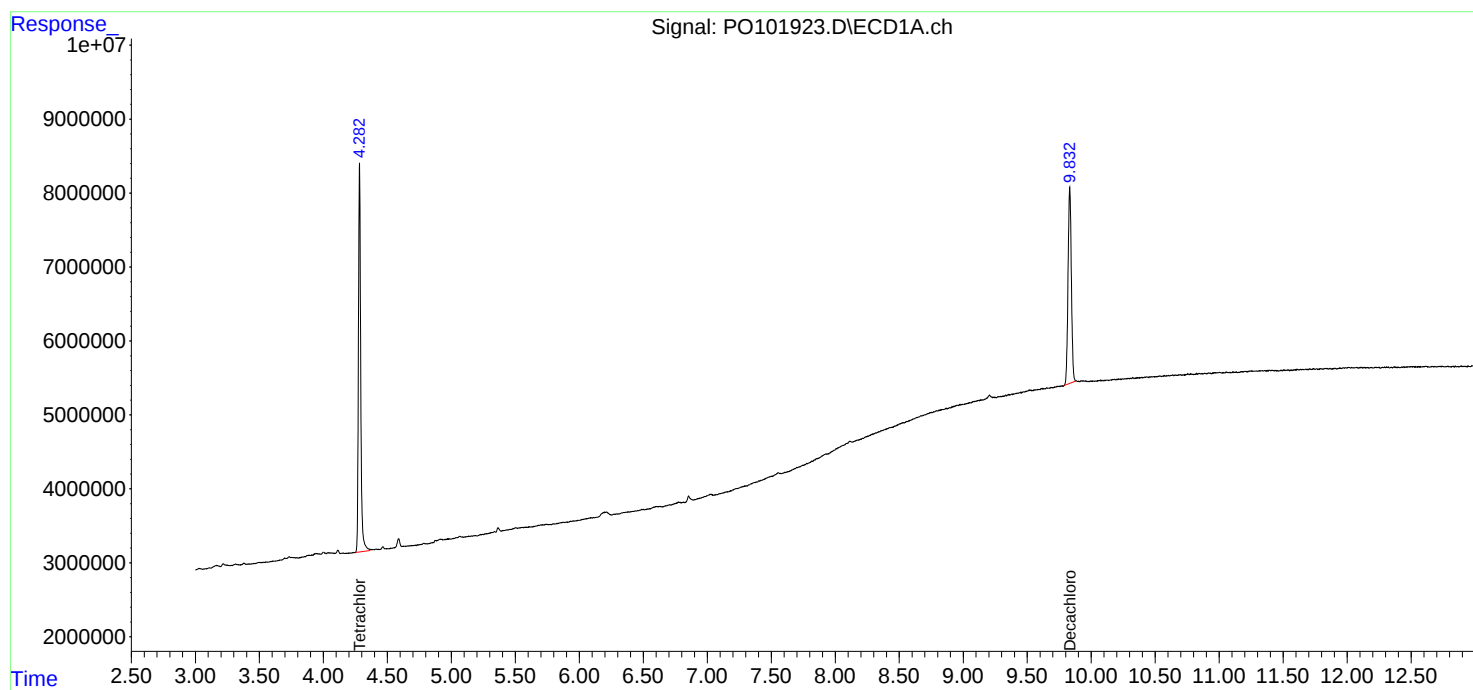

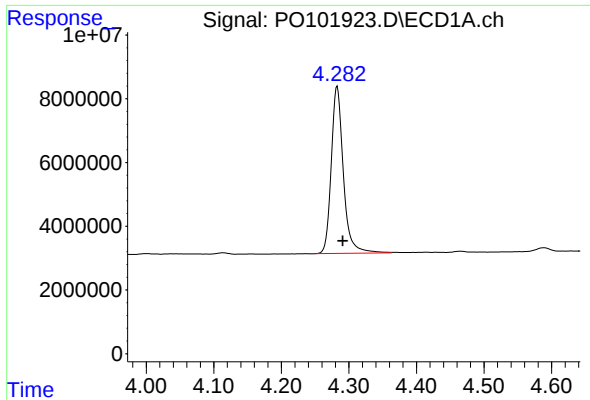


#1 Tetrachloro-m-xylene

R.T.: 4.283 min
Delta R.T.: -0.008 min
Response: 65485932
Conc: 21.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB159137BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :Ankita Jodhani 02/21/2024

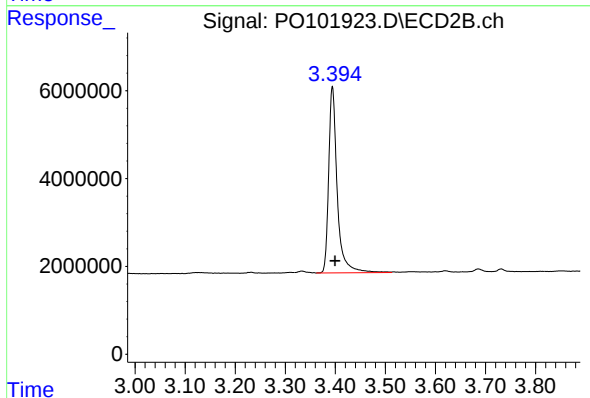


#1 Tetrachloro-m-xylene

R.T.: 3.394 min
Delta R.T.: -0.006 min
Response: 50343494
Conc: 18.94 ng/ml

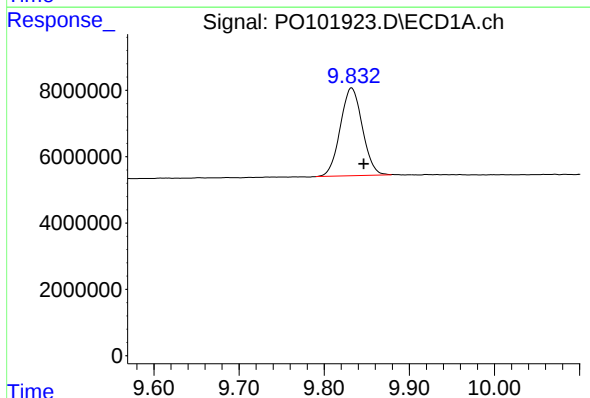

#2 Decachlorobiphenyl

R.T.: 9.832 min
Delta R.T.: -0.015 min
Response: 47672857
Conc: 22.73 ng/ml m

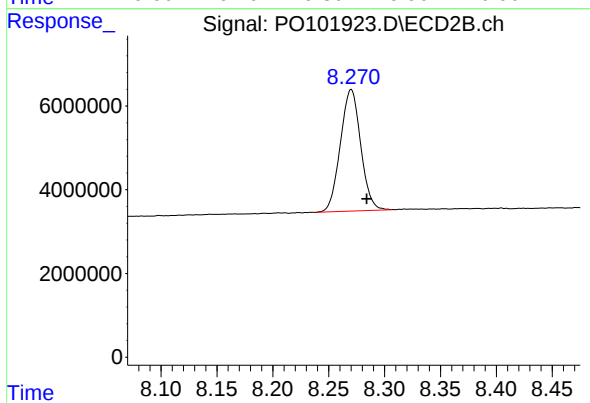

#2 Decachlorobiphenyl

R.T.: 8.270 min
Delta R.T.: -0.014 min
Response: 36869556
Conc: 19.41 ng/ml m